

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
 Data File : BF137652.D
 Acq On : 20 Mar 2024 13:40
 Operator : CG\JU
 Sample : PB159685BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159685BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.951	483	487	497	rBV	52968	87117	1.45%	0.235%
2	5.346	549	554	557	rBV	4962195	5114703	85.19%	13.785%
3	6.369	723	728	731	rBV	4705950	5221460	86.97%	14.073%
4	6.722	785	788	801	rBV	1145532	1160274	19.33%	3.127%
5	7.292	880	885	888	rBV	3402172	3483154	58.02%	9.388%
6	8.004	1003	1006	1029	rBV	1574615	1563790	26.05%	4.215%
7	9.086	1185	1190	1193	rBV	6467824	6003817	100.00%	16.182%
8	9.757	1300	1304	1319	rBV	2022484	1709191	28.47%	4.607%
9	10.545	1434	1438	1461	rBV	2973443	3150132	52.47%	8.490%
10	11.239	1553	1556	1580	rBV	1695222	1636062	27.25%	4.410%
11	12.833	1822	1827	1830	rBV	5788413	5754245	95.84%	15.509%
12	13.874	2001	2004	2023	rBV	1085502	1114946	18.57%	3.005%
13	15.298	2242	2246	2268	rBV	626637	955777	15.92%	2.576%
14	16.221	2397	2403	2409	rBV3	34608	62761	1.05%	0.169%
15	16.380	2420	2430	2442	rBV6	22246	84806	1.41%	0.229%




Sum of corrected areas: 37102235

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
Data File : BF137652.D
Acq On : 20 Mar 2024 13:40
Operator : CG\JU
Sample : PB159685BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159685BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

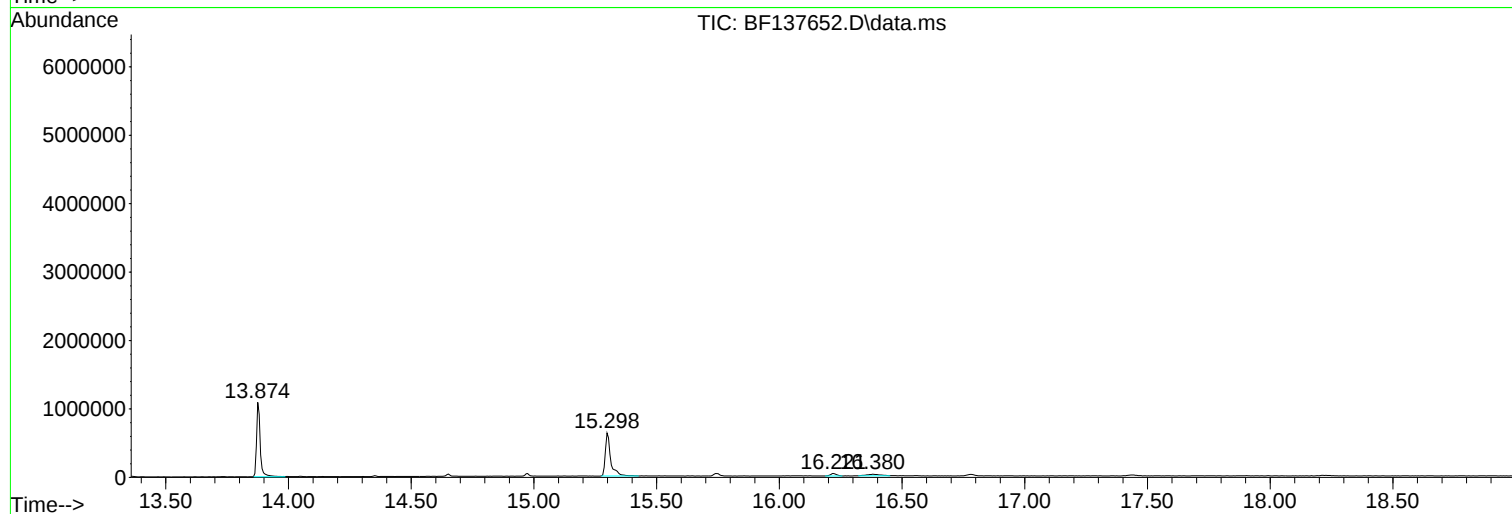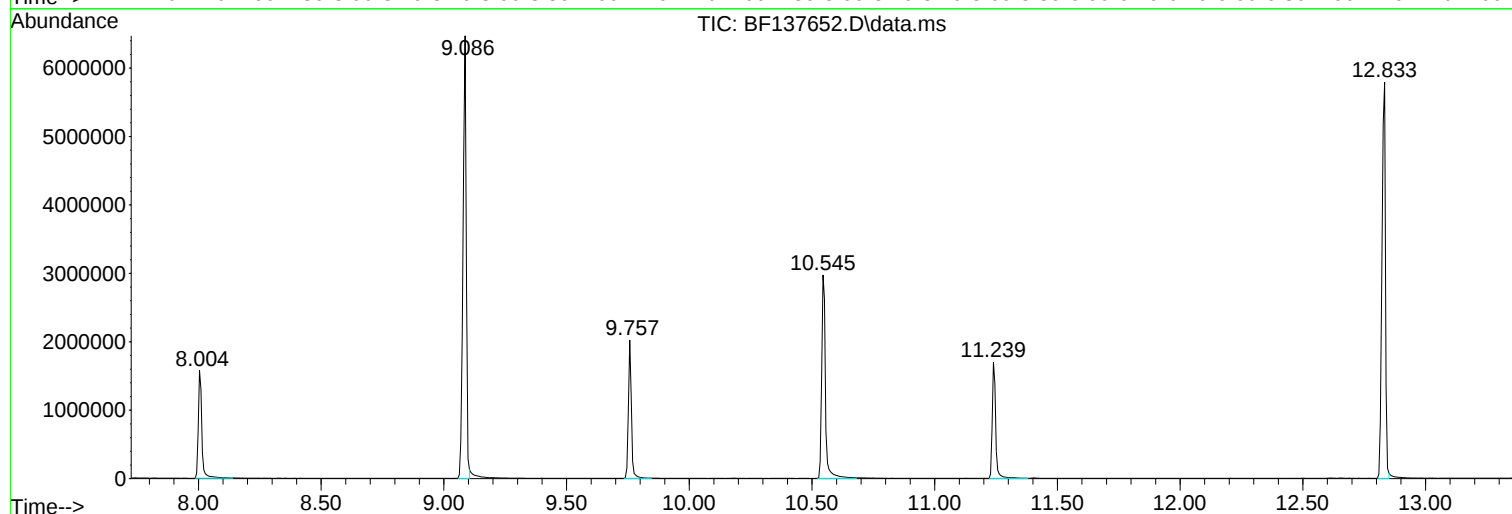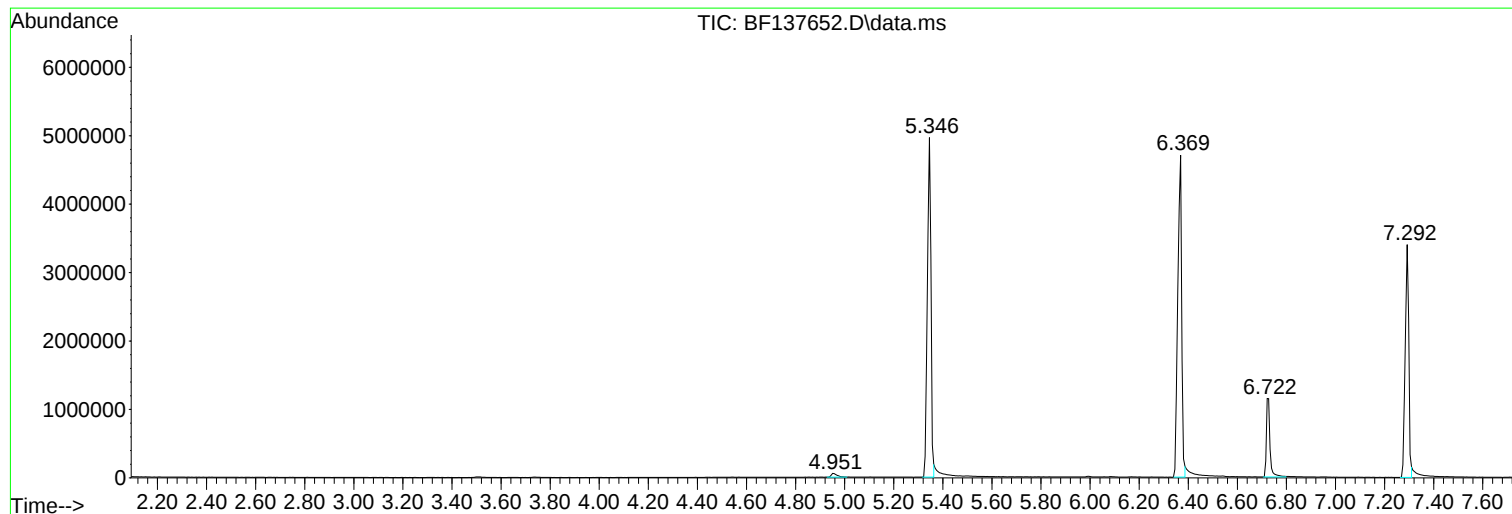

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
Data File : BF137652.D
Acq On : 20 Mar 2024 13:40
Operator : CG\JU
Sample : PB159685BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159685BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
Data File : BF137652.D
Acq On : 20 Mar 2024 13:40
Operator : CG\JU
Sample : PB159685BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159685BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------