
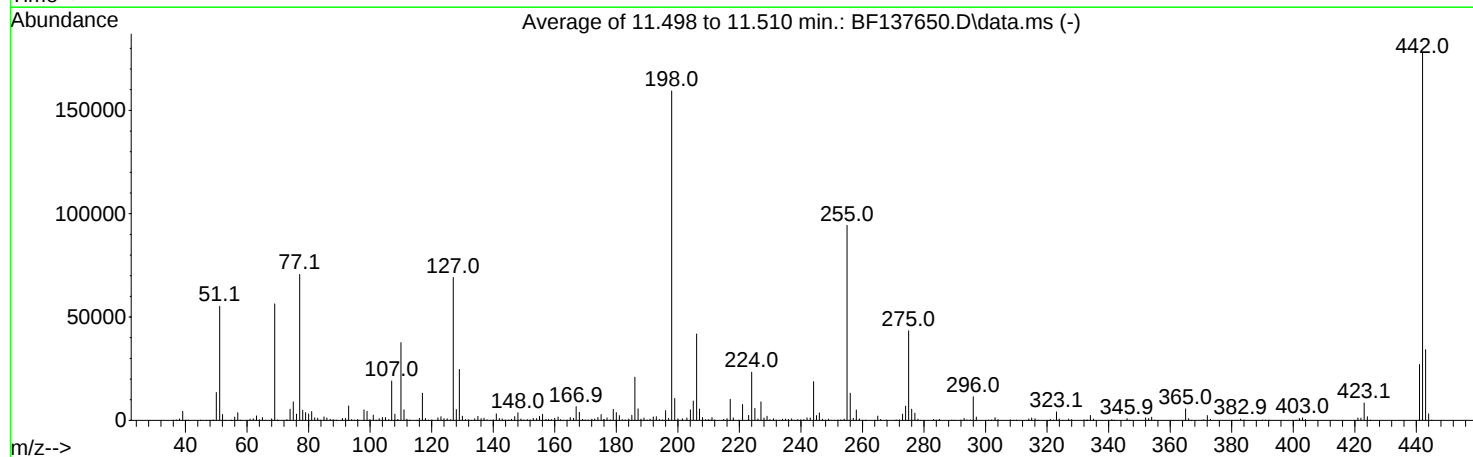


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
Data File : BF137650.D
Acq On : 20 Mar 2024 12:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

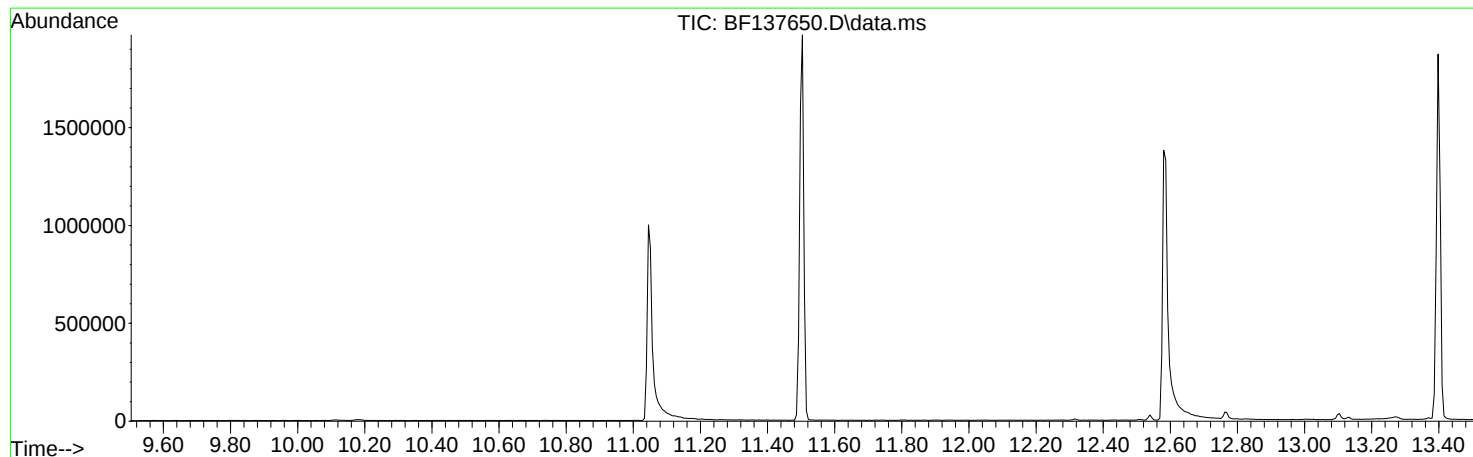




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	55199	PASS
68	69	0.00	2	1.4	774	PASS
69	198	0.00	100	35.4	56352	PASS
70	69	0.00	2	0.4	226	PASS
127	198	10	80	43.4	69160	PASS
197	198	0.00	2	0.6	1023	PASS
198	198	100	100	100.0	159397	PASS
199	198	5	9	6.7	10641	PASS
275	198	10	60	27.2	43376	PASS
365	198	1	100	3.5	5614	PASS
441	198	0.01	100	17.0	27048	PASS
442	442	50	100	100.0	178003	PASS
443	442	15	24	19.2	34197	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
 Data File : BF137650.D
 Acq On : 20 Mar 2024 12:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 21 02:13:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 14 14:45:20 2024
 Response via : Initial Calibration

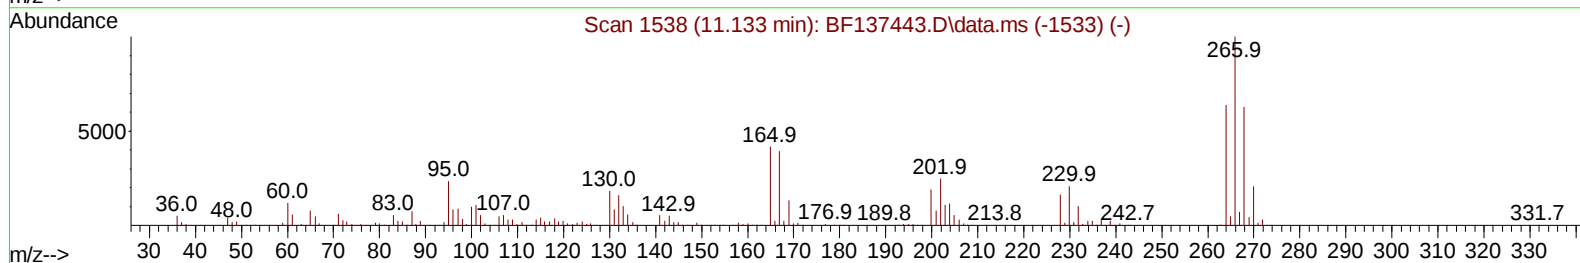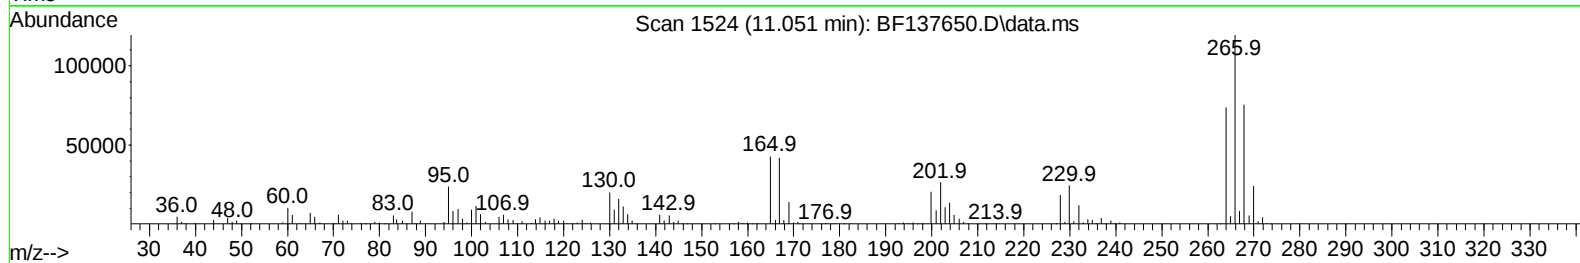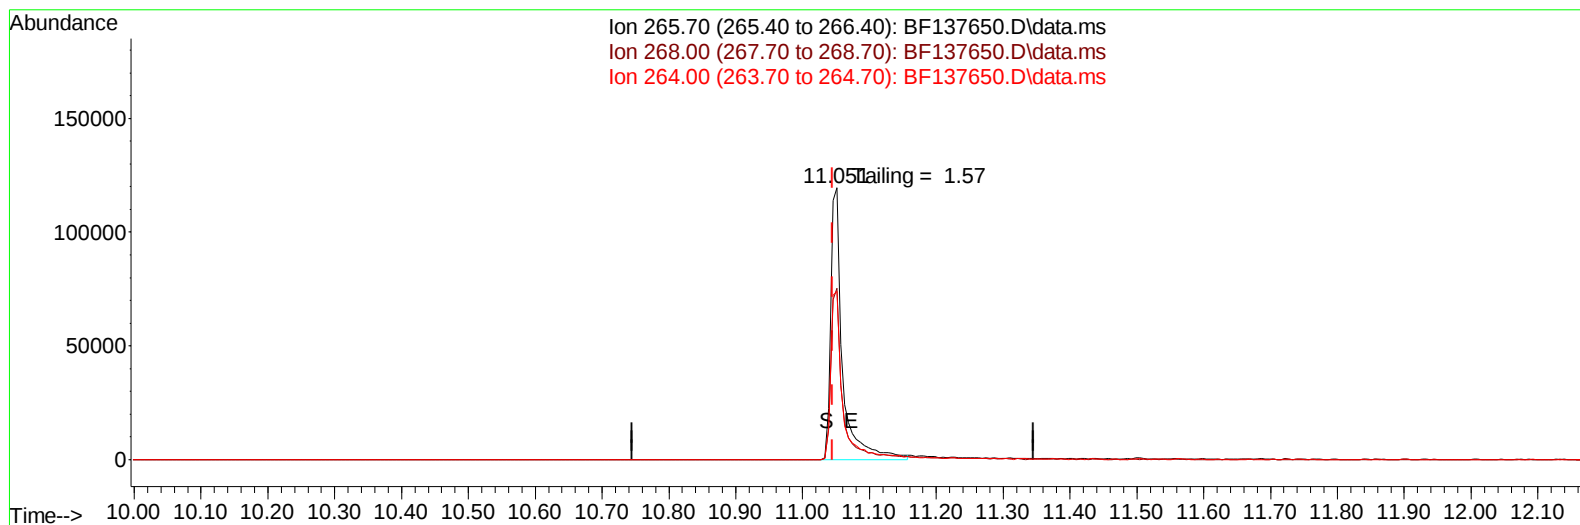

TIC: BF137650.D\data.ms

(70) Pentachlorophenol (C)

11.051min (+ 0.006) 28678.84 ng




response 147618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.20
264.00	63.60	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032024\
Data File : BF137650.D
Acq On : 20 Mar 2024 12:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 21 02:13:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

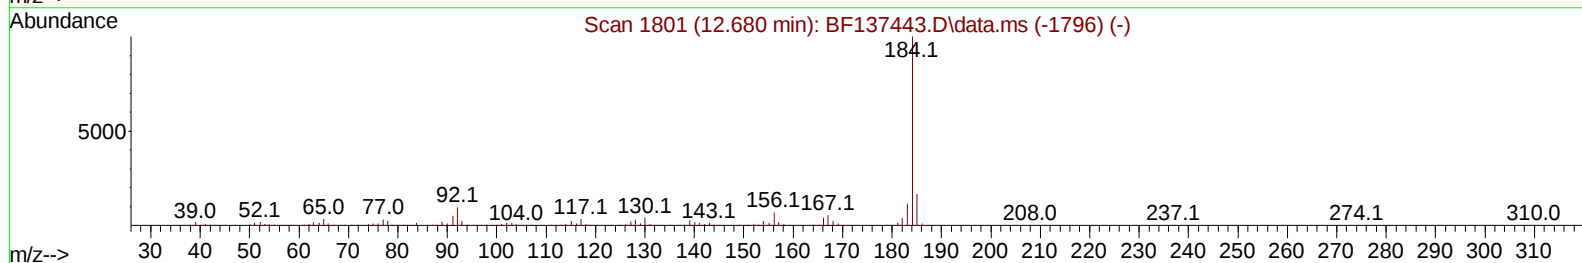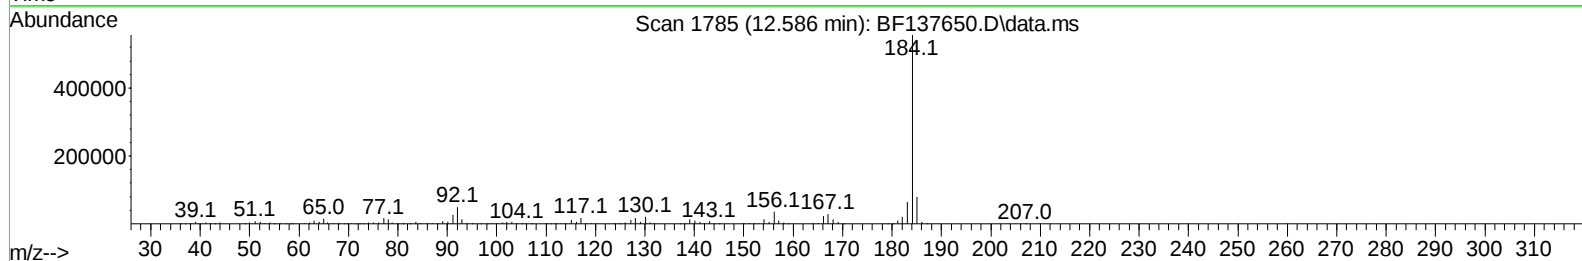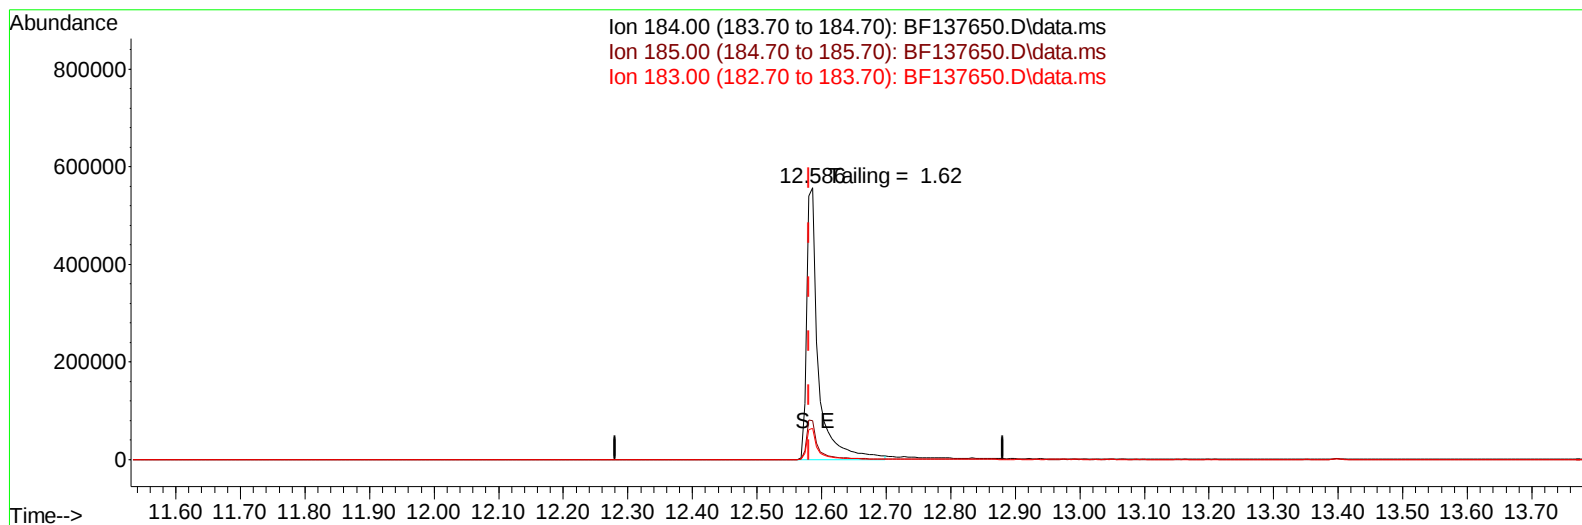

TIC: BF137650.D\data.ms

(77) Benzidine

12.586min (+ 0.006) 0.00 ng

response 716021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.40
183.00	11.60	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/20/2024	BNA_F	<u>BF137650.D</u>
Compound Name	Response	Retention Time
DDT	298907	13.398
DDD	9297	13.104
DDE	4489	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13786	312693	4.41

Instrument :
BNA_F
ClientSampleId :
DFTPP