
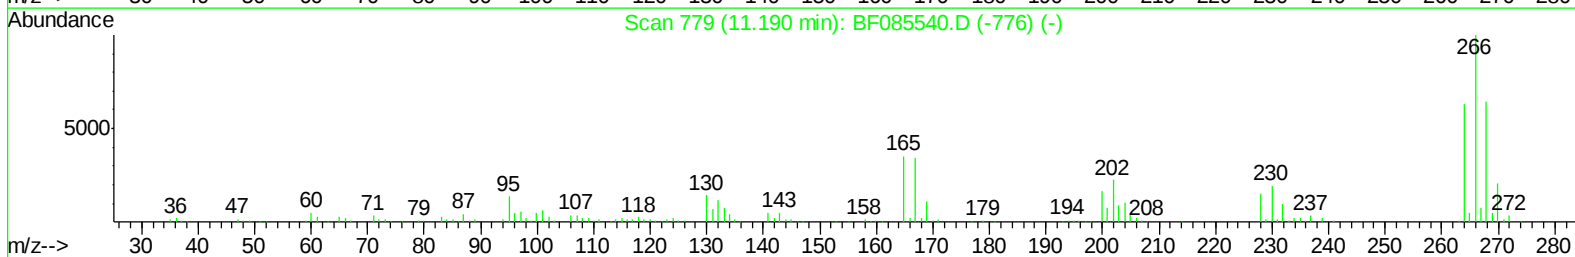
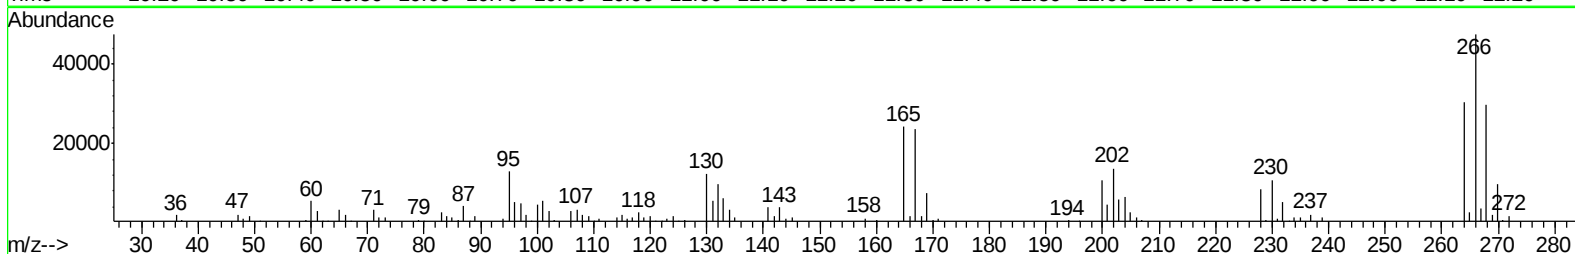


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032116\
Data File : BF085641.D
Acq On : 22 Mar 2016 2:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:54:32 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

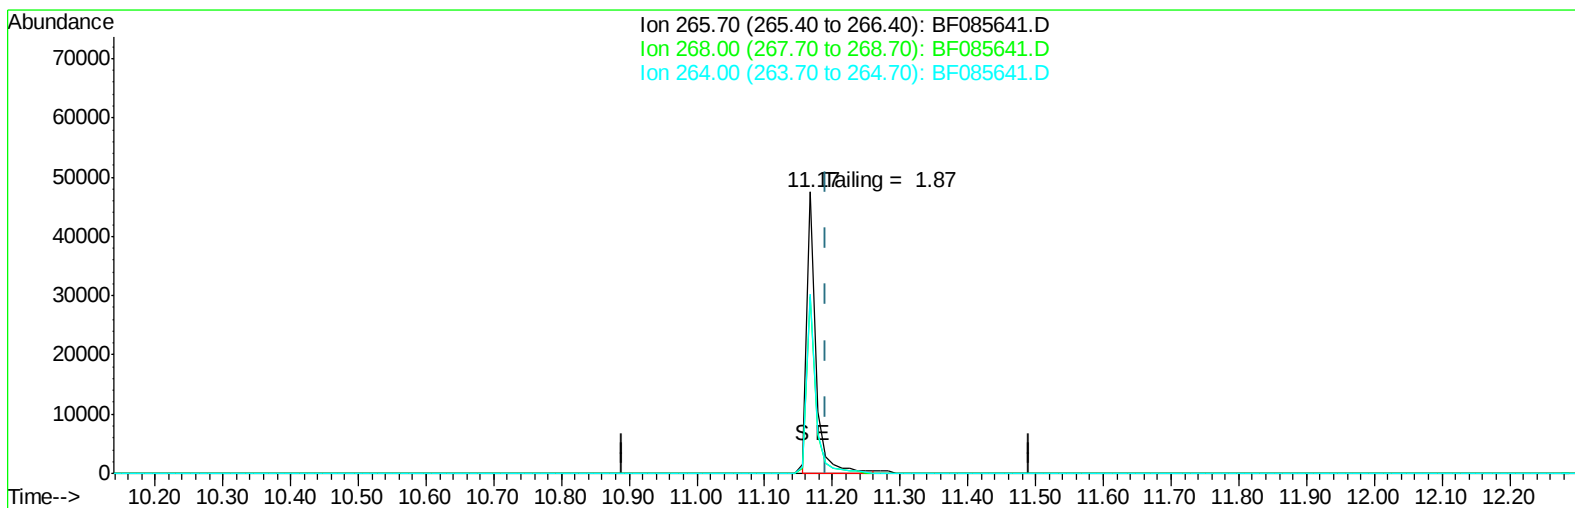

TIC: BF085641.D

(69) Pentachlorophenol (C)




11.168min (-0.023) 27361.44ng

response 46192

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.90
264.00	63.30	63.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032116\
Data File : BF085641.D
Acq On : 22 Mar 2016 2:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:54:32 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

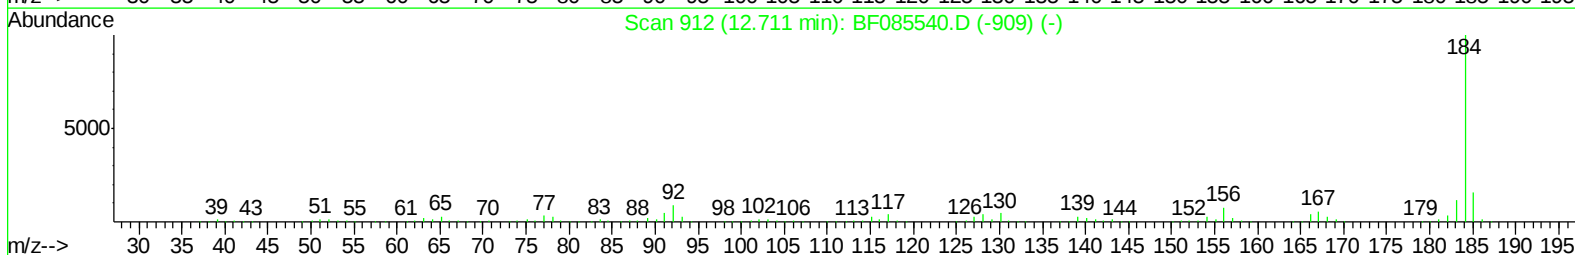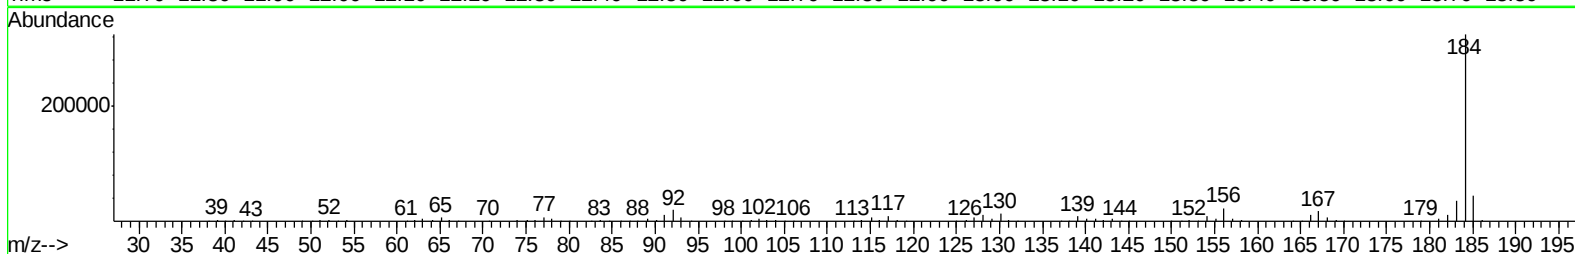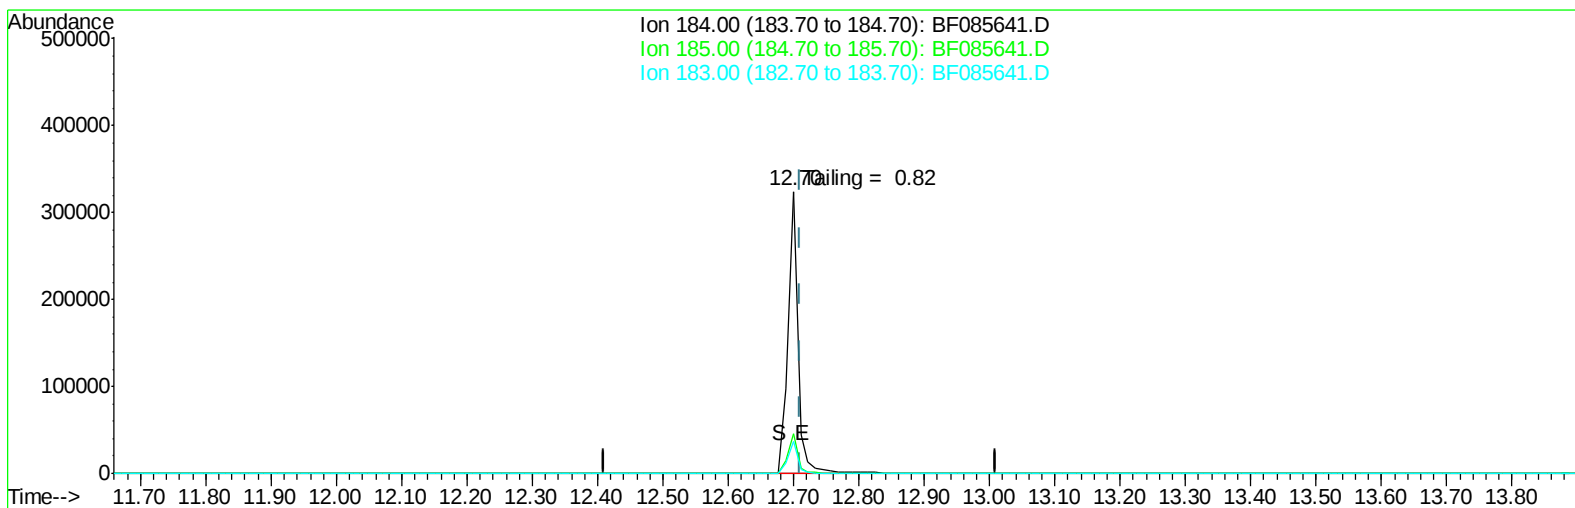

TIC: BF085641.D

(76) Benzidine

12.699min (-0.011) 0.00ng

response 346555

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.91
183.00	11.80	11.38
0.00	0.00	0.00