


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032116\
Data File : BF085616.D
Acq On : 21 Mar 2016 11:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 18 23:31:39 2016

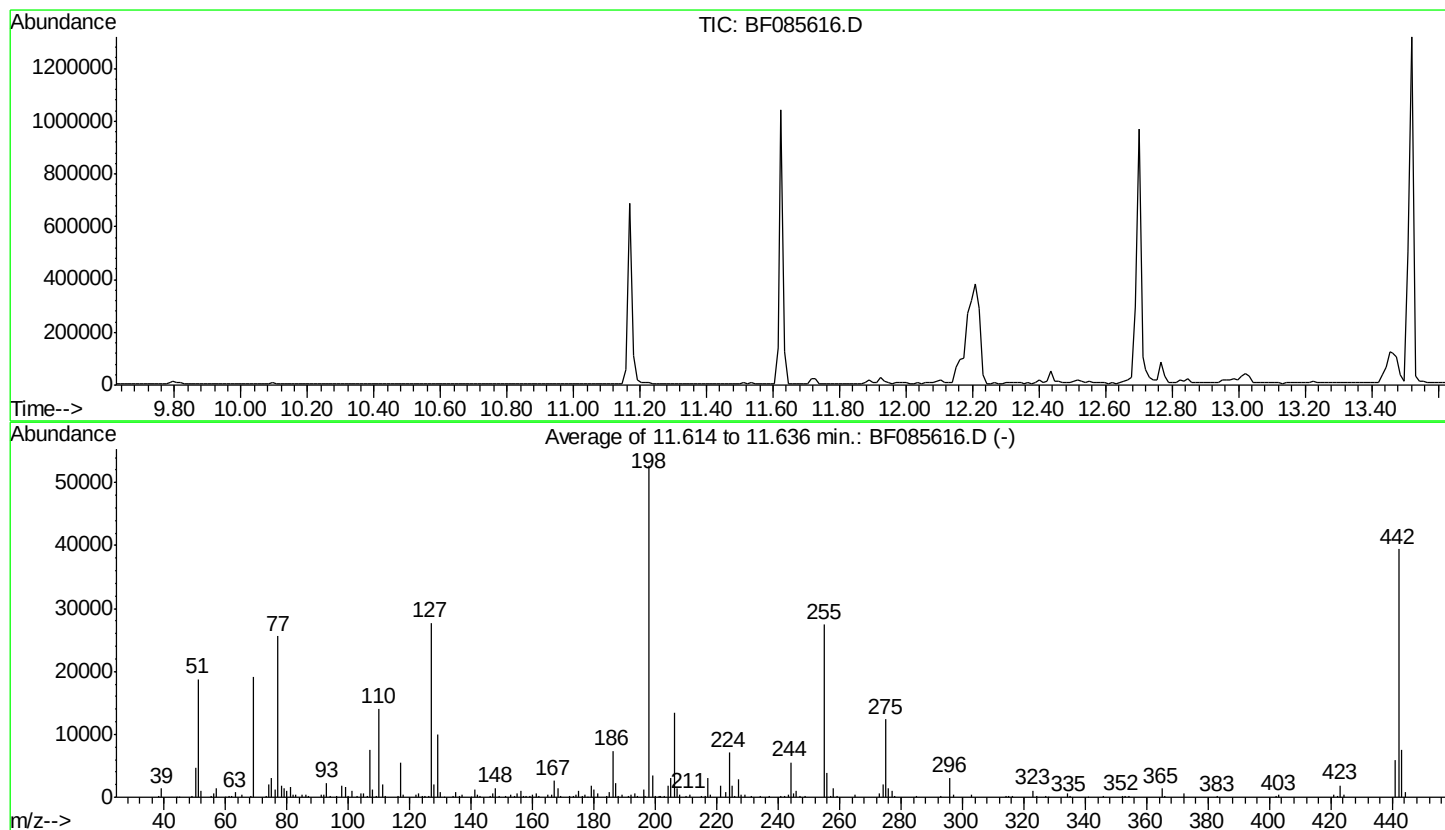

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	18760	PASS
68	69	0.00	2	1.3	258	PASS
69	198	0.00	100	36.5	19226	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	27730	PASS
197	198	0.00	2	0.5	278	PASS
198	198	100	100	100.0	52693	PASS
199	198	5	9	6.6	3474	PASS
275	198	10	60	23.5	12376	PASS
365	198	1	100	2.6	1385	PASS
441	442	0.01	24	15.1	5952	PASS
442	198	50	100	74.8	39419	PASS
443	442	15	24	19.0	7497	PASS