
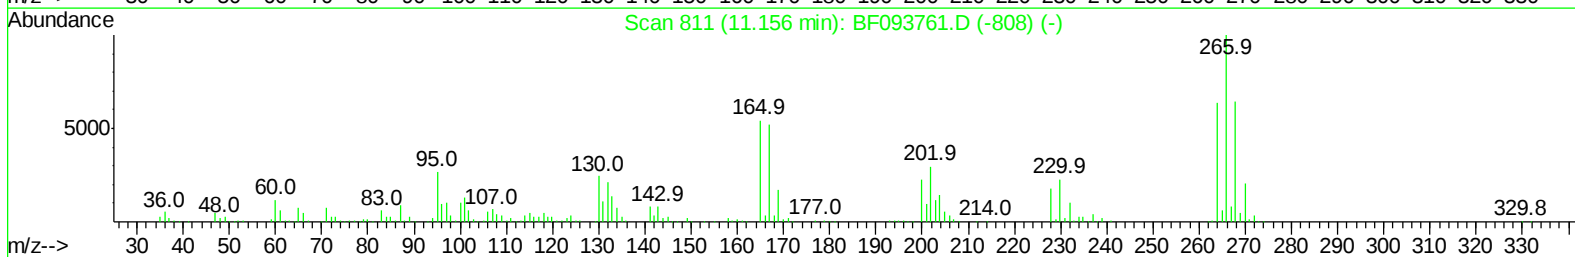
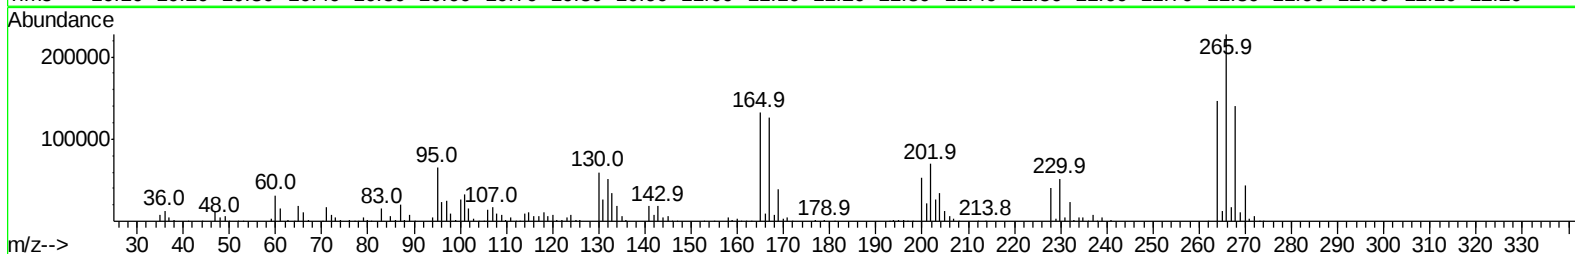


Data Path : Z:\HPCHEM1\BNA F\Data\BF032117\
Data File : BF093791.D
Acq On : 21 Mar 2017 11:45
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 18:53:44 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 14:38:20 2017
Response via : Initial Calibration

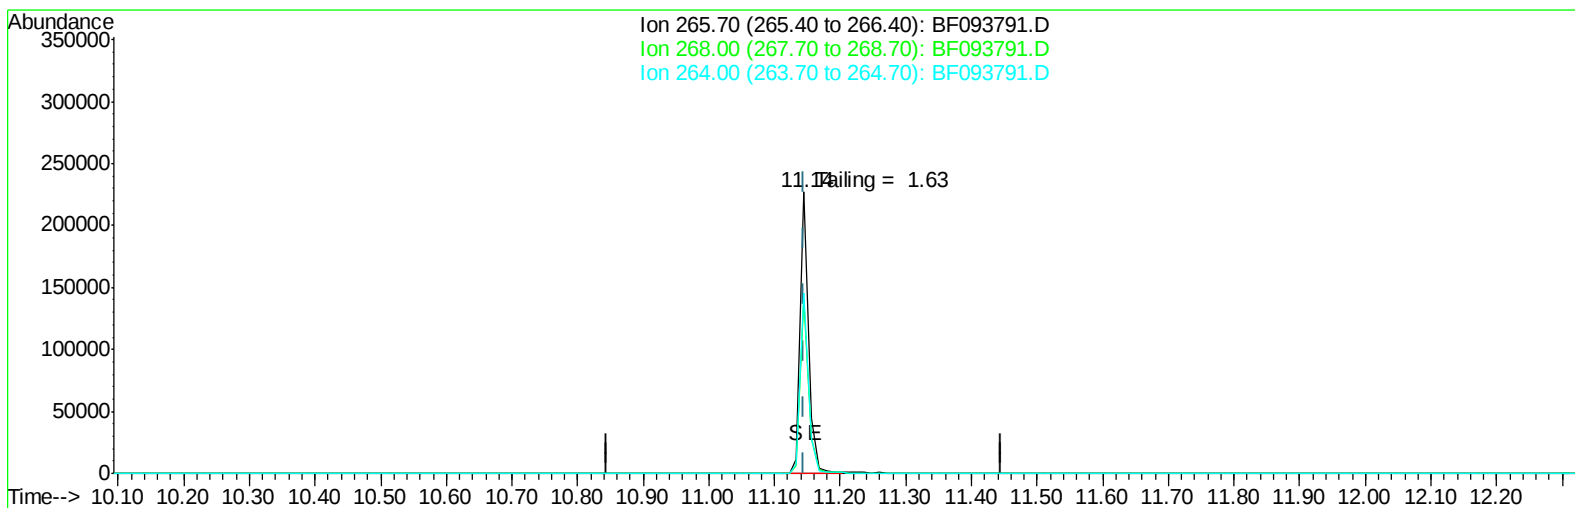

TIC: BF093791.D

(69) Pentachlorophenol (C)




11.145min (-0.000) 0.00ng

response 203634

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.83
264.00	64.60	64.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032117\
Data File : BF093791.D
Acq On : 21 Mar 2017 11:45
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 18:53:44 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 14:38:20 2017
Response via : Initial Calibration

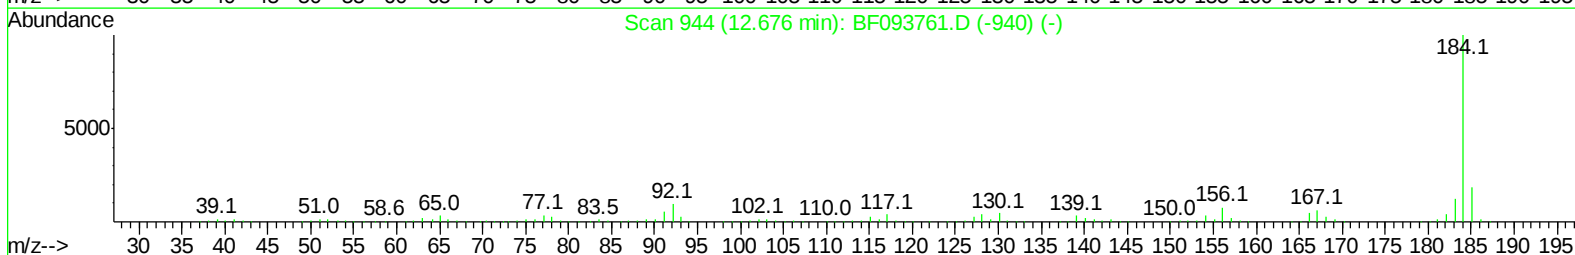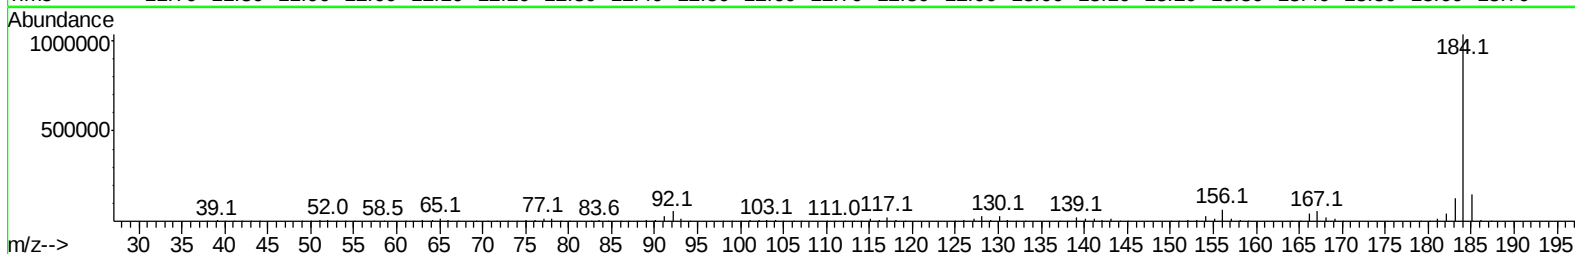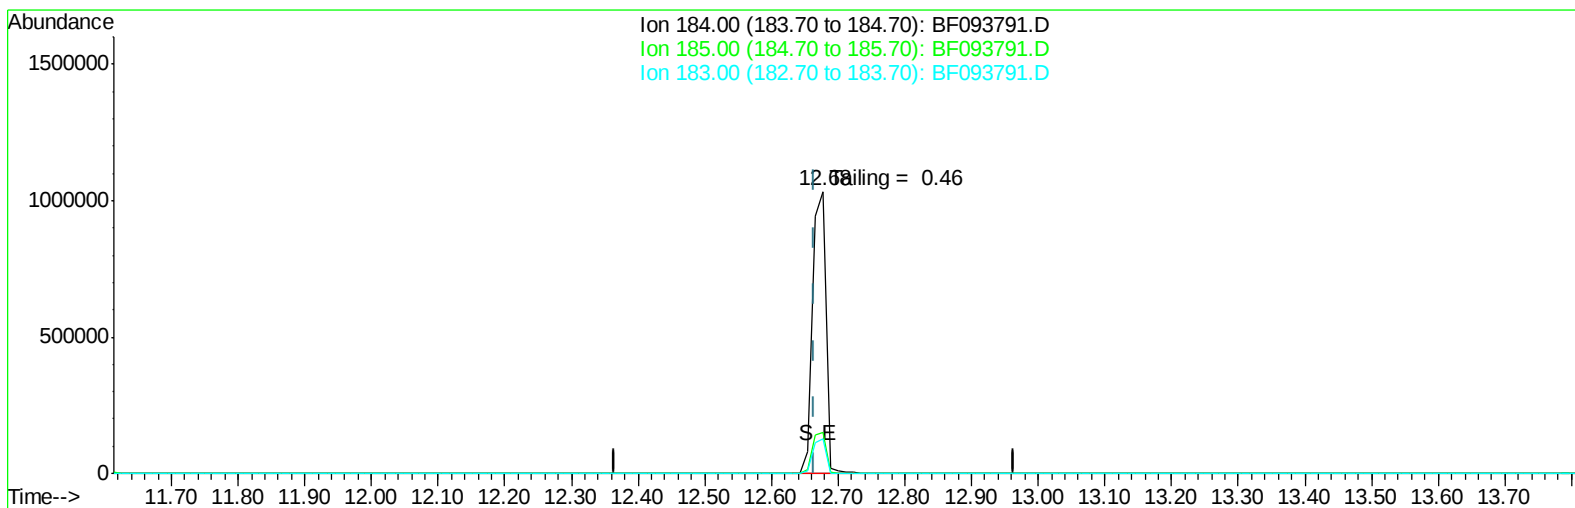

TIC: BF093791.D

(76) Benzidine

12.677min (+0.011) 0.00ng

response 1440003

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.37#
183.00	12.20	12.10
0.00	0.00	0.00