

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032117\
 Data File : BF093807.D
 Acq On : 21 Mar 2017 19:22
 Operator : SJ/MA
 Sample : I2332-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-SF-01-002-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.070	12	16	23	rVB	34460	56648	2.41%	0.244%
2	4.984	269	271	274	rBV	254364	283255	12.07%	1.220%
3	5.419	306	309	311	rBV	2006407	1809261	77.09%	7.791%
4	6.447	397	399	402	rBV	1725565	1763624	75.15%	7.595%
5	6.584	409	411	414	rBV	1641459	1866389	79.53%	8.037%
6	6.824	430	432	434	rBV	1494127	1238659	52.78%	5.334%
7	6.984	443	446	448	rBV	1656378	1547242	65.93%	6.663%
8	7.385	478	481	483	rBV	1365022	1263373	53.83%	5.440%
9	8.116	542	545	547	rBV	1217085	1677993	71.50%	7.226%
10	9.190	636	639	641	rBV	2334062	2346797	100.00%	10.106%
11	9.579	671	673	675	rBV	170634	136636	5.82%	0.588%
12	9.865	695	698	700	rBV	1744809	1774477	75.61%	7.641%
13	10.311	733	737	738	rBV	42267	45043	1.92%	0.194%
14	10.642	764	766	768	rBV	1220081	1104601	47.07%	4.757%
15	10.779	776	778	781	rBV	63835	68106	2.90%	0.293%
16	11.225	815	817	819	rBV	51467	50359	2.15%	0.217%
17	11.339	824	827	829	rVV	1990967	1758544	74.93%	7.573%
18	11.408	831	833	837	rVB	21032	26678	1.14%	0.115%
19	11.648	852	854	857	rBV	25531	27633	1.18%	0.119%
20	11.876	872	874	875	rBV2	18535	26998	1.15%	0.116%
21	12.539	930	932	934	rVB	104190	99033	4.22%	0.426%
22	12.768	949	952	955	rBV	102015	103208	4.40%	0.444%
23	12.917	963	965	968	rVB	1443643	1683456	71.73%	7.249%
24	13.831	1042	1045	1048	rBV	33083	47996	2.05%	0.207%
25	13.968	1054	1057	1059	rBV	962460	1188541	50.65%	5.118%
26	14.460	1097	1100	1107	rBV6	11303	33848	1.44%	0.146%
27	14.974	1142	1145	1150	rVB	30045	65566	2.79%	0.282%
28	15.305	1172	1174	1177	rVB	29475	32479	1.38%	0.140%
29	15.374	1177	1180	1182	rBV	802448	1045527	44.55%	4.502%
30	15.843	1218	1221	1223	rBV2	14309	25880	1.10%	0.111%
31	16.311	1260	1262	1267	rVB4	10422	24243	1.03%	0.104%


Sum of corrected areas: 23222093

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032117\
Data File : BF093807.D
Acq On : 21 Mar 2017 19:22
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-01-002-B

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

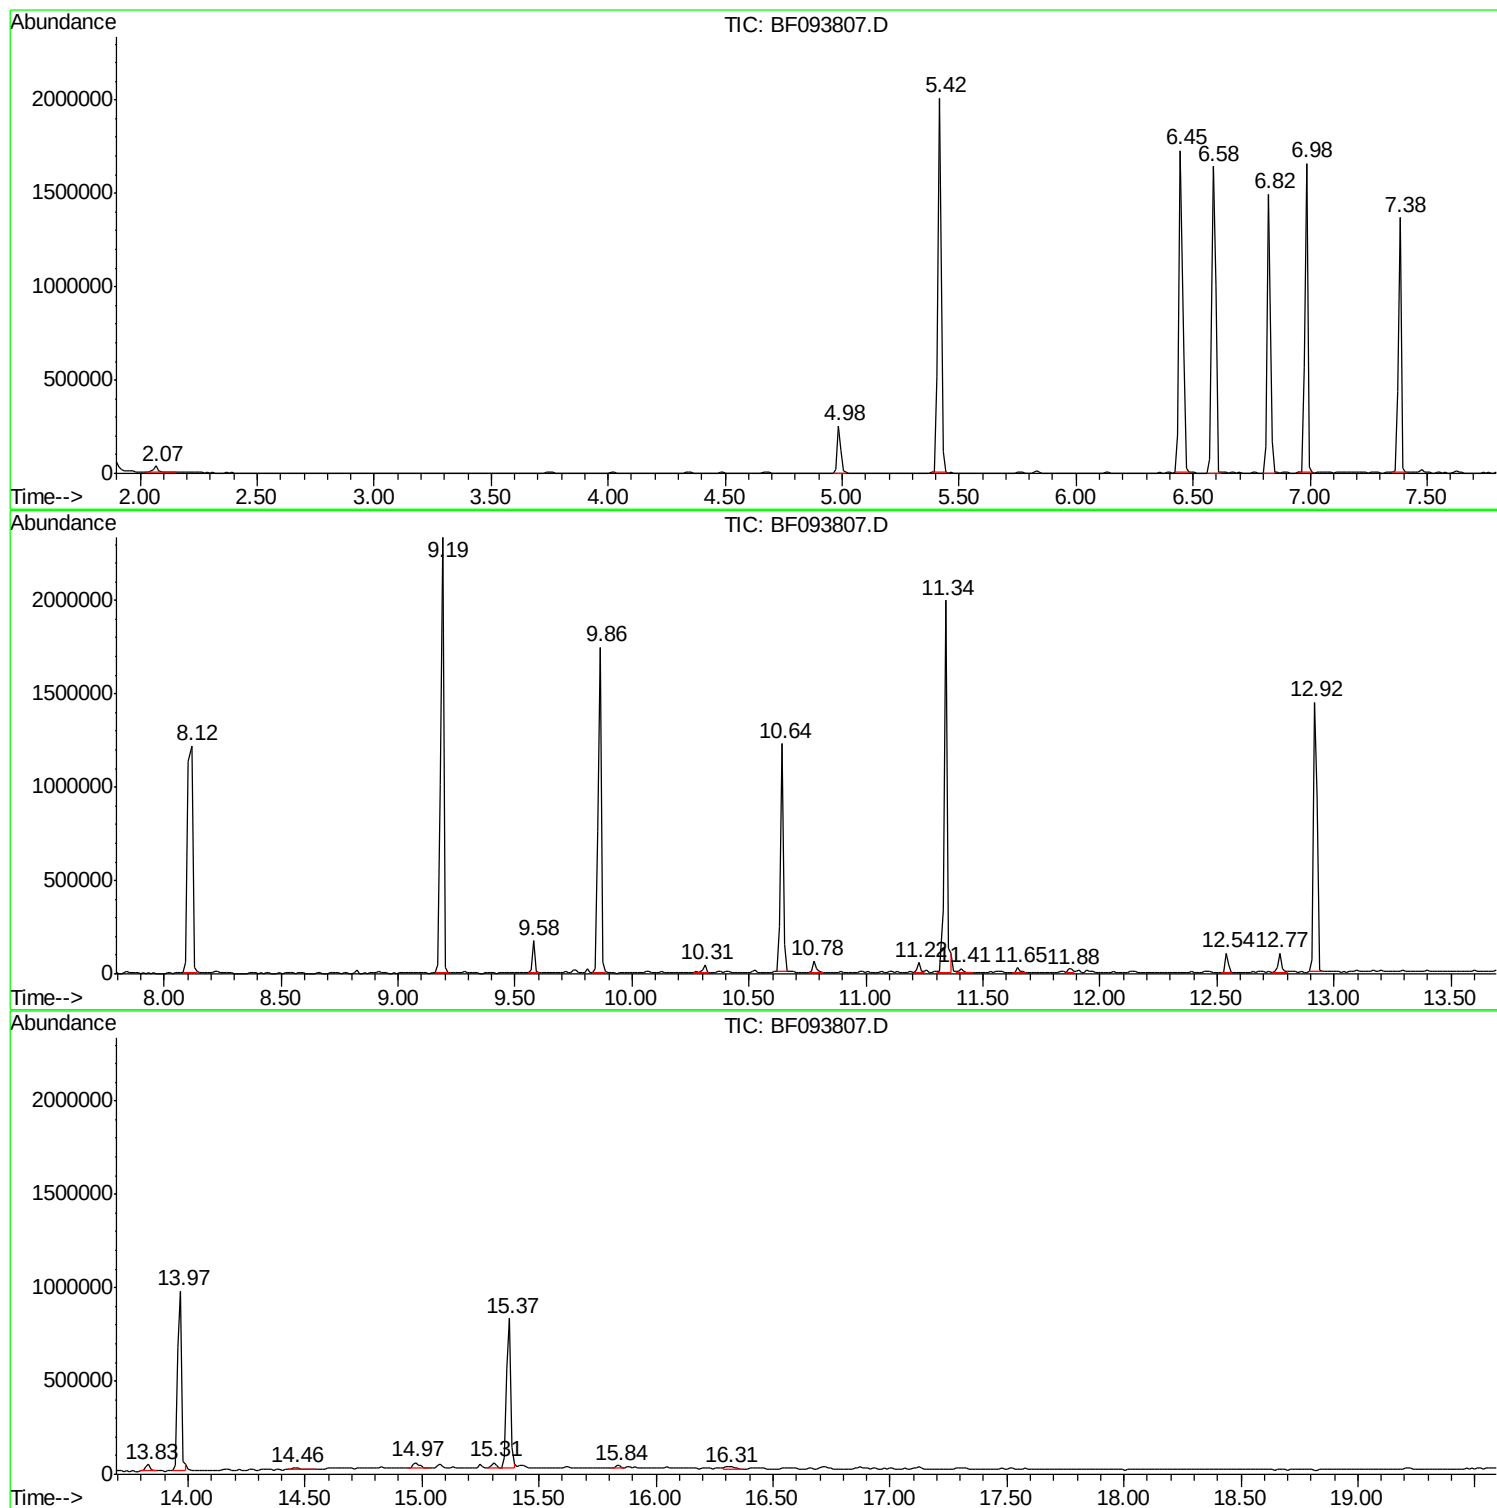

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032117\
Data File : BF093807.D
Acq On : 21 Mar 2017 19:22
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 17 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
FK-SF-01-002-B

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.	
4.98	4.57 ng	283255	1,4-Dichlorobenzene-d4	6.82	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10

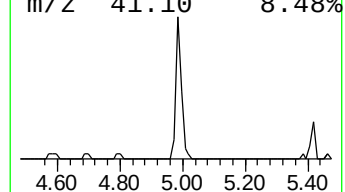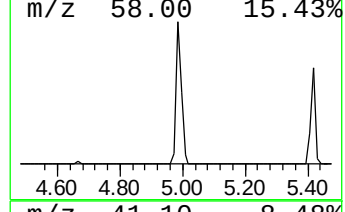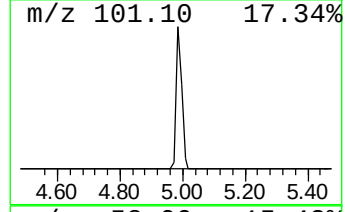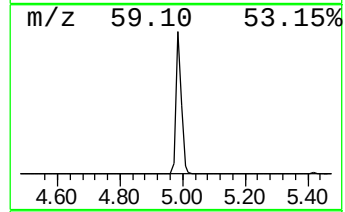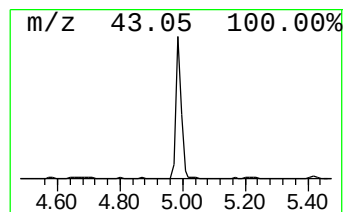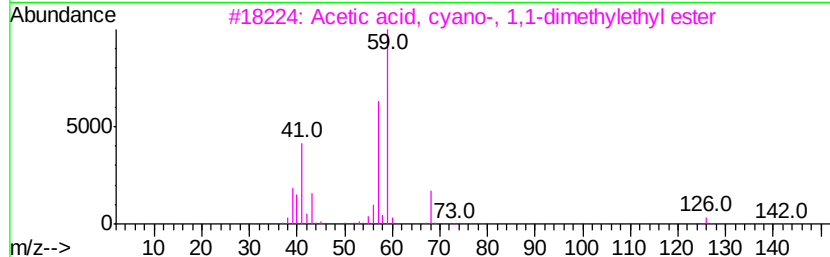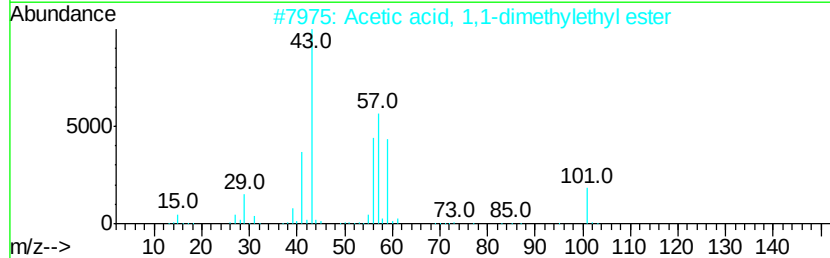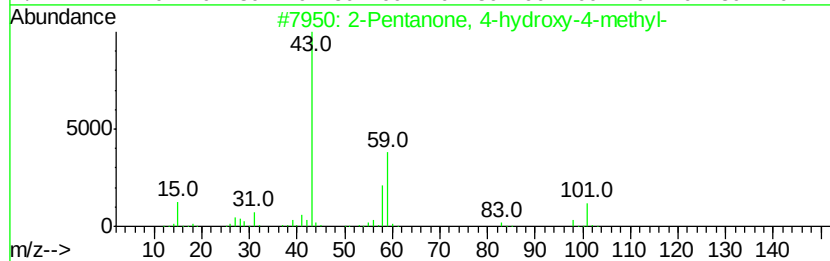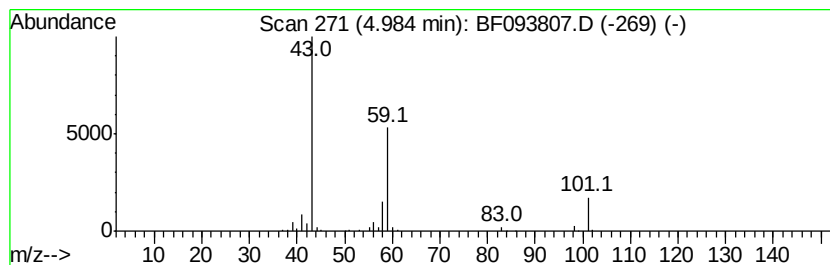

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032117\
Data File : BF093807.D
Acq On : 21 Mar 2017 19:22
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-01-002-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.58	30.14 ng	1866390	1,4-Dichlorobenzene-d4	6.82

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3		Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2	5		Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	10
4			Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

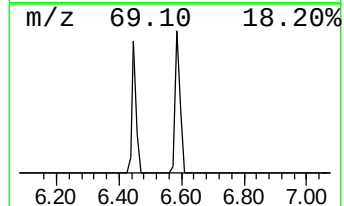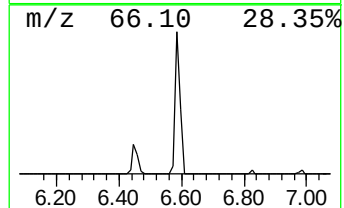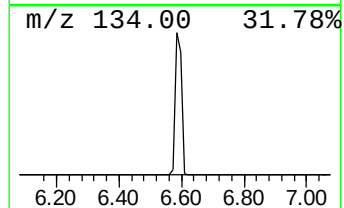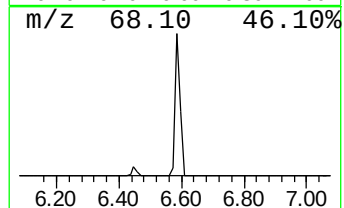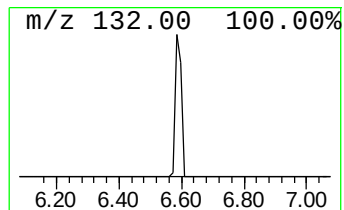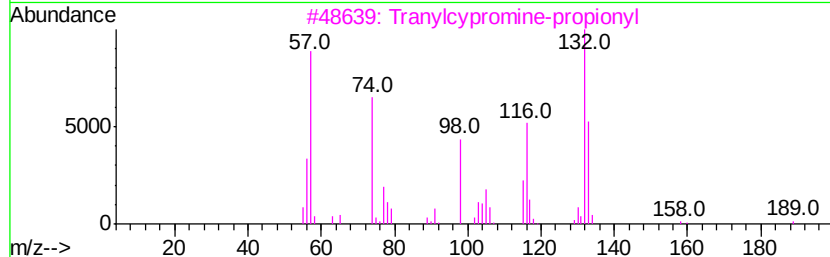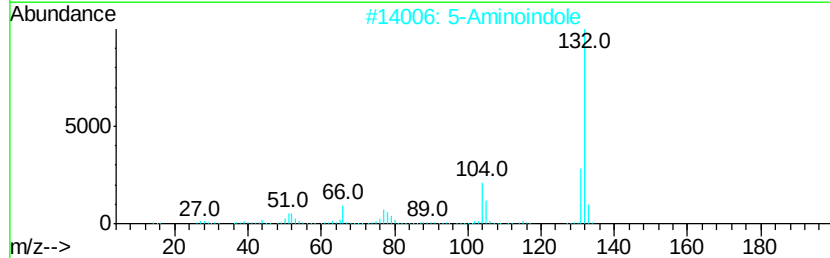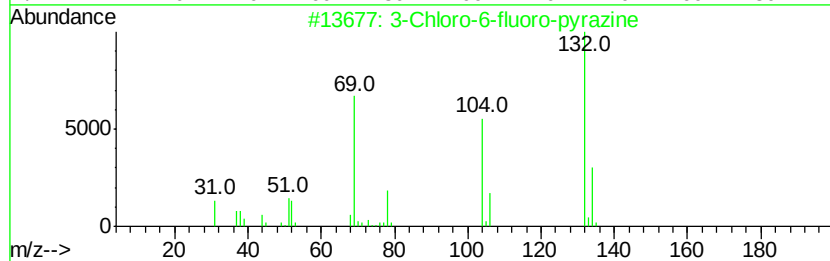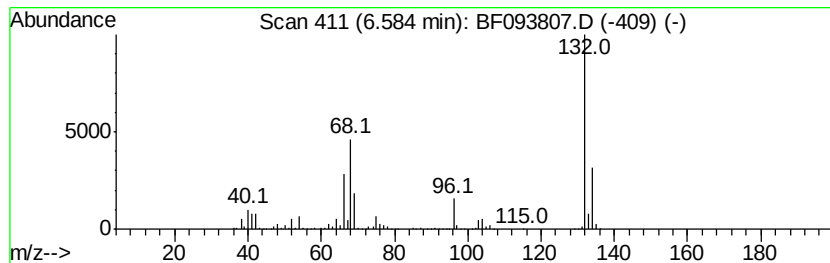

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032117\
Data File : BF093807.D
Acq On : 21 Mar 2017 19:22
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-01-002-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.98	4.6	ng	283255	1	6.82	1238660	20.0
unknown6.58	6.58	30.1	ng	1866390	1	6.82	1238660	20.0