


Data Path : Z:\HPCHEM1\BNA F\Data\BF032117\
 Data File : BF093791.D
 Acq On : 21 Mar 2017 11:45
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 21 14:38:20 2017

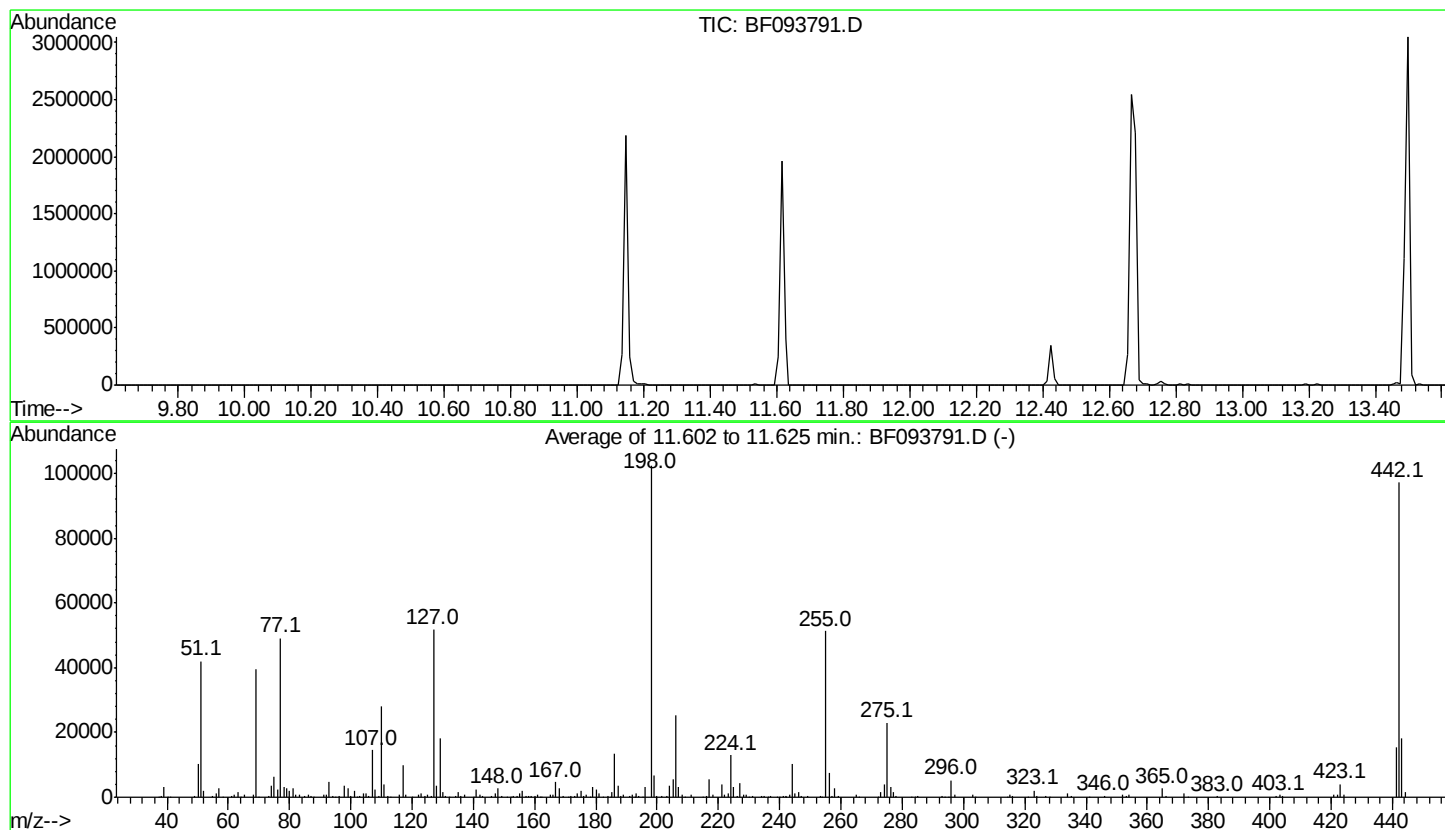

AutoFind: Scans 850, 851, 852; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	42111	PASS
68	69	0.00	2	1.6	635	PASS
69	198	0.00	100	38.5	39446	PASS
70	69	0.00	2	0.5	196	PASS
127	198	10	80	50.5	51741	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102394	PASS
199	198	5	9	6.7	6816	PASS
275	198	10	60	22.4	22965	PASS
365	198	1	100	2.5	2604	PASS
441	442	0.01	24	15.9	15409	PASS
442	198	50	100	94.8	97056	PASS
443	442	15	24	18.7	18136	PASS