


Data Path : Z:\HPCHEM1\BNA F\Data\BF032117\
 Data File : BF093815.D
 Acq On : 22 Mar 2017 4:32
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 21 14:38:20 2017

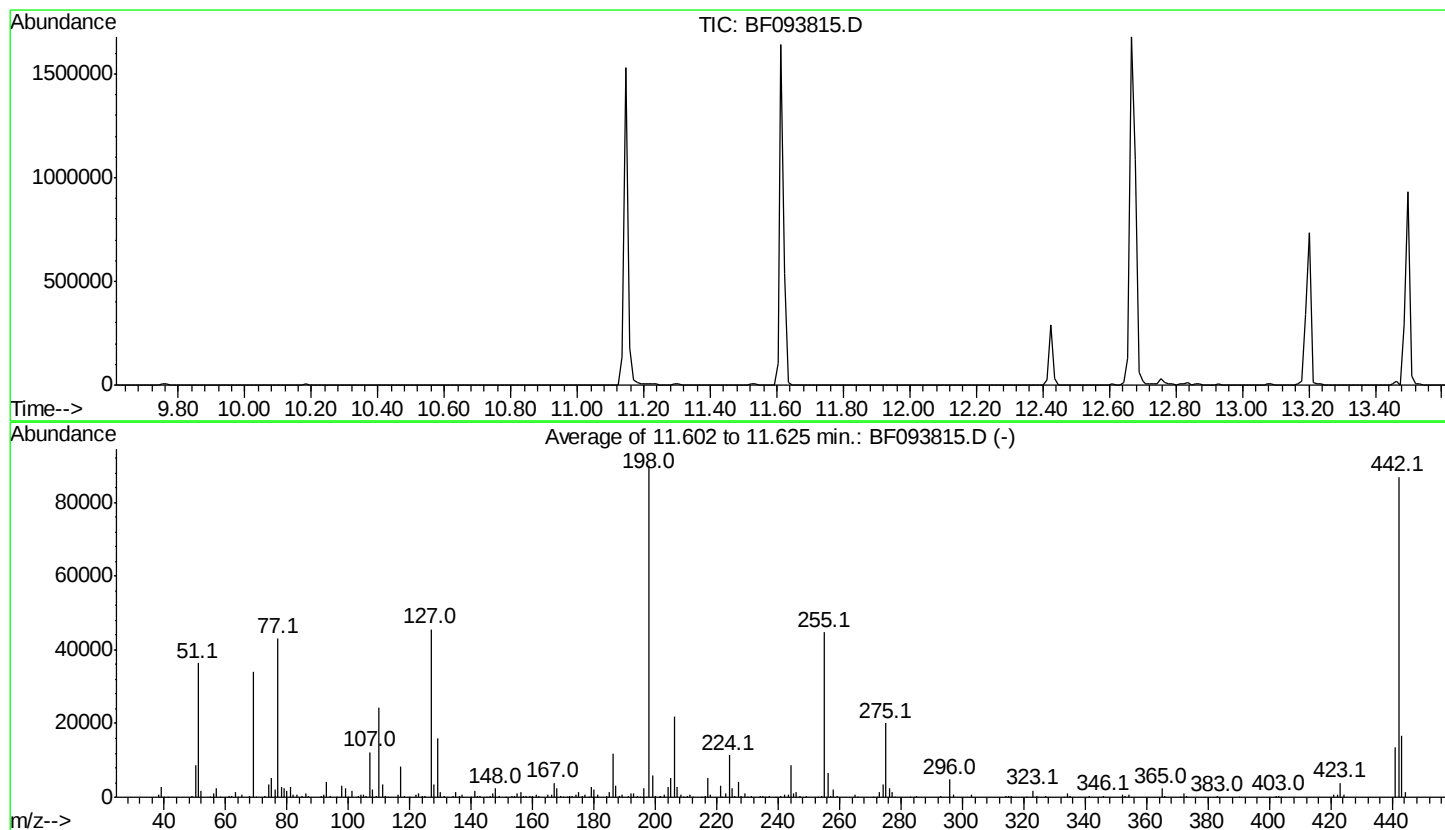

AutoFind: Scans 850, 851, 852; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	36353	PASS
68	69	0.00	2	1.4	484	PASS
69	198	0.00	100	37.7	33900	PASS
70	69	0.00	2	0.4	149	PASS
127	198	10	80	50.6	45553	PASS
197	198	0.00	2	0.2	166	PASS
198	198	100	100	100.0	90037	PASS
199	198	5	9	6.6	5960	PASS
275	198	10	60	22.3	20111	PASS
365	198	1	100	2.7	2399	PASS
441	442	0.01	24	15.7	13614	PASS
442	198	50	100	96.6	86950	PASS
443	442	15	24	19.1	16632	PASS