
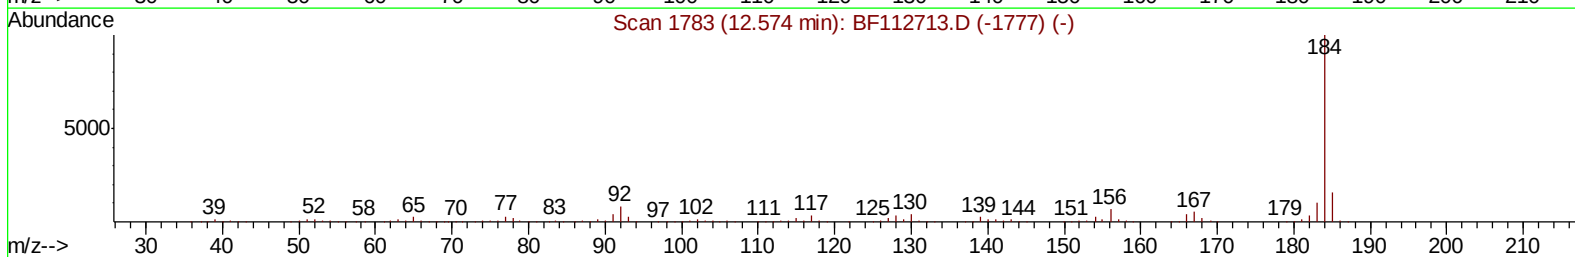
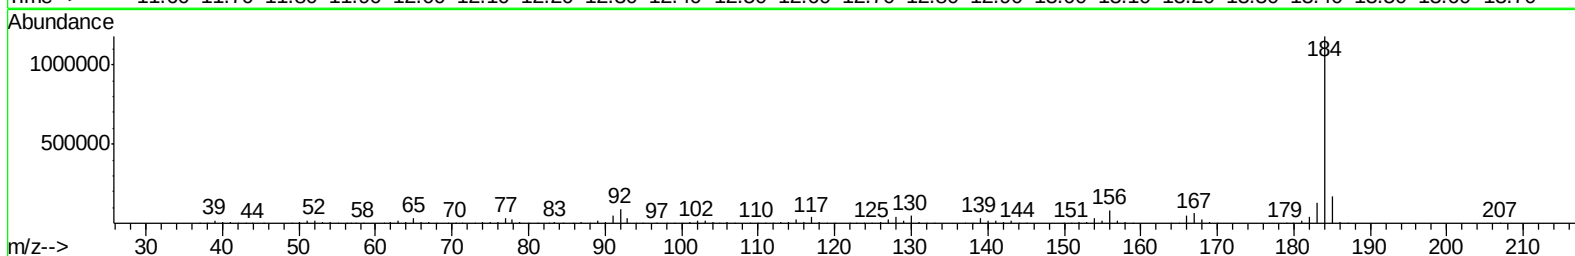


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
Data File : BF113198.D
Acq On : 21 Mar 2019 10:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 02:32:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

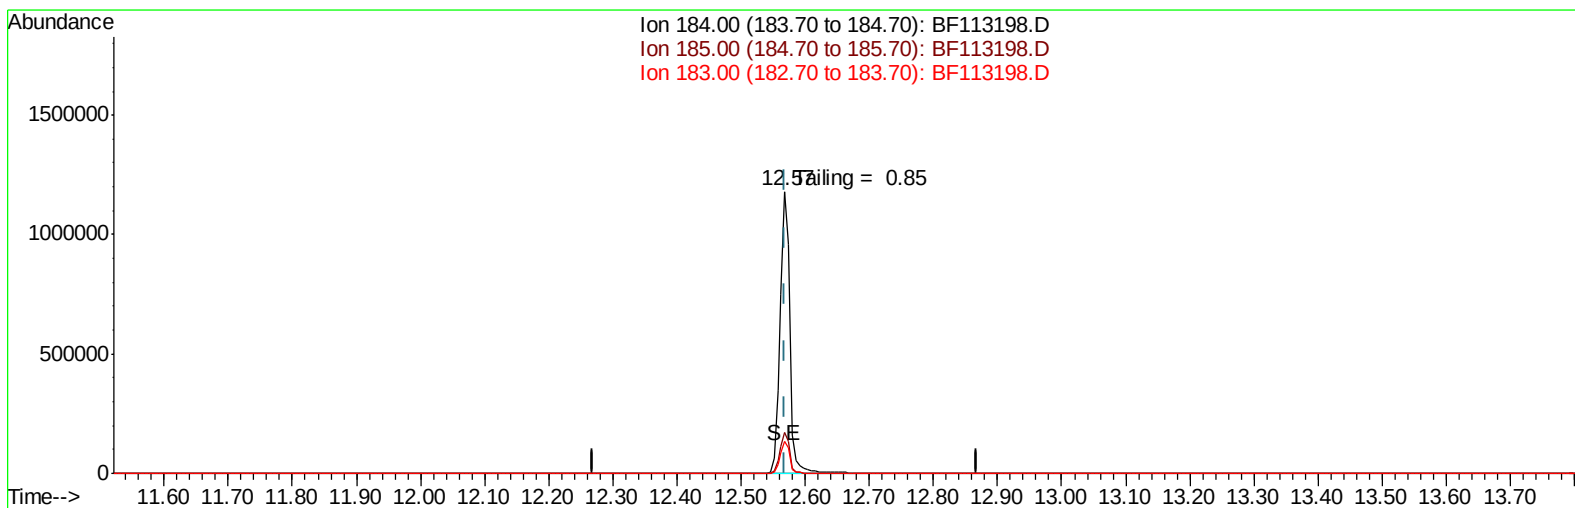

TIC: BF113198.D

(77) Benzidine




12.569min (-0.000) 68270.16ng

response 1299904

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.54
183.00	10.70	11.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
Data File : BF113198.D
Acq On : 21 Mar 2019 10:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 02:32:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

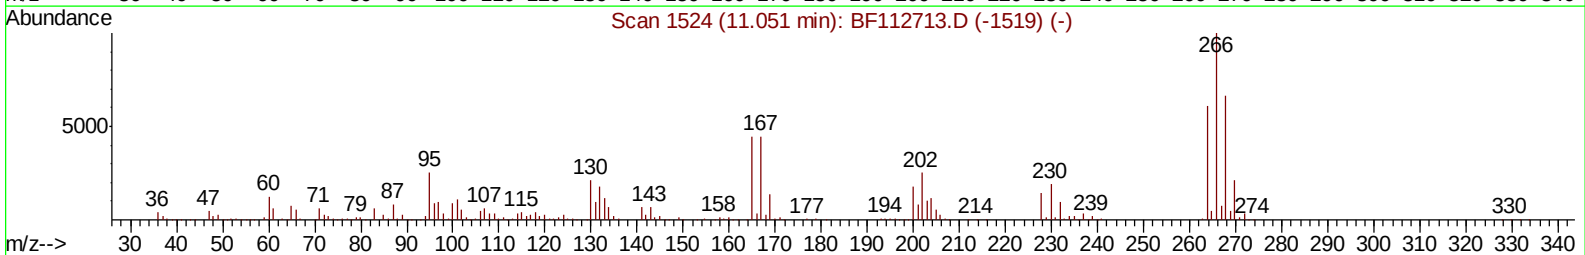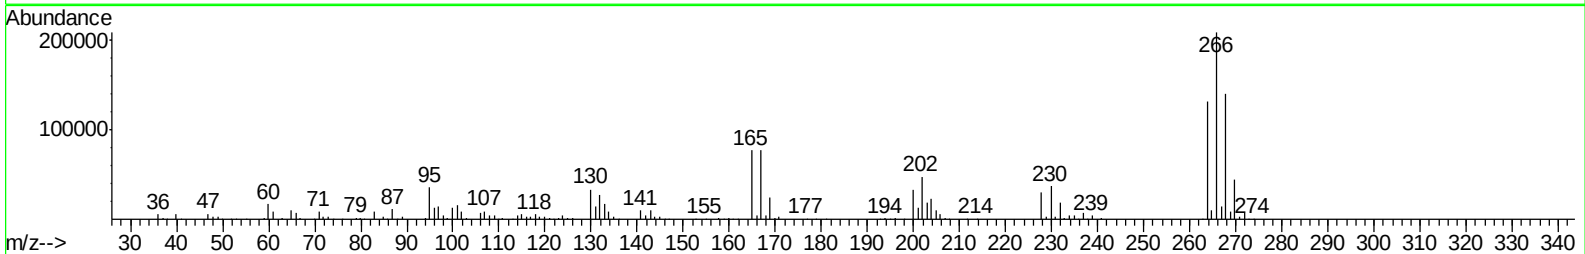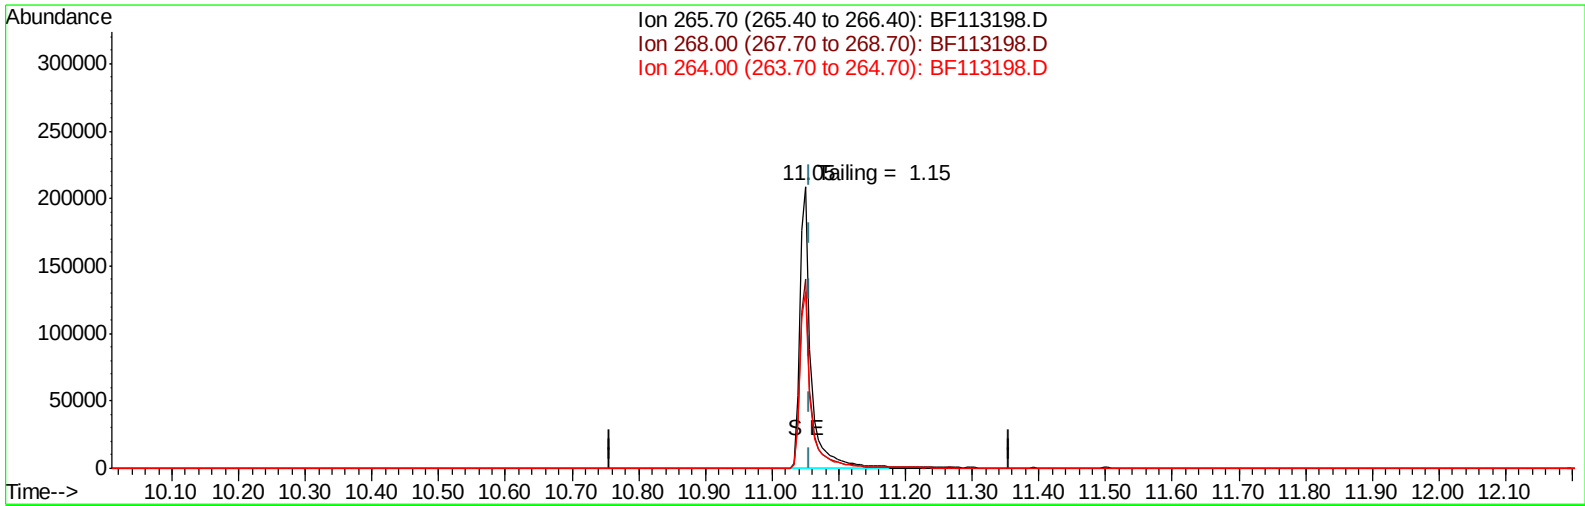

TIC: BF113198.D

(70) Pentachlorophenol (C)

11.051min (-0.006) 204642.98ng

response 241691

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.29
264.00	61.10	62.94
0.00	0.00	0.00