

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
 Data File : BF113216.D
 Acq On : 21 Mar 2019 18:52
 Operator : JU/SJ
 Sample : K2004-01 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-20(10-11)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	548	552	561	rBV	865389	857209	65.06%	5.728%
2	5.975	658	661	666	rBV2	12921	17525	1.33%	0.117%
3	6.163	688	693	696	rBV3	17987	22606	1.72%	0.151%
4	6.363	723	727	742	rBV	1062294	1068254	81.08%	7.138%
5	6.493	745	749	757	rVB	1222223	1061469	80.57%	7.093%
6	6.722	784	788	791	rBV	1191581	971926	73.77%	6.494%
7	6.875	811	814	823	rVB	915452	831862	63.14%	5.558%
8	7.281	873	883	890	rBV	615572	648981	49.26%	4.336%
9	7.516	916	923	924	rBV4	12739	19286	1.46%	0.129%
10	7.534	924	926	930	rVB4	20526	18421	1.40%	0.123%
11	7.628	937	942	944	rBV2	28713	33695	2.56%	0.225%
12	8.004	1002	1006	1014	rBV	1448740	1317477	100.00%	8.803%
13	8.075	1017	1018	1021	rVV	63555	59931	4.55%	0.400%
14	8.104	1021	1023	1031	rVB5	21603	41618	3.16%	0.278%
15	8.304	1051	1057	1060	rBV3	34809	43777	3.32%	0.293%
16	8.439	1077	1080	1085	rBV	52147	47094	3.57%	0.315%
17	8.604	1105	1108	1112	rBV3	17198	25347	1.92%	0.169%
18	8.704	1121	1125	1127	rVB2	28012	33850	2.57%	0.226%
19	8.916	1158	1161	1169	rVB3	35356	42504	3.23%	0.284%
20	9.034	1179	1181	1185	rBV	44838	37890	2.88%	0.253%
21	9.081	1185	1189	1199	rVV	1263411	1271850	96.54%	8.498%
22	9.475	1253	1256	1257	rBV	71881	65609	4.98%	0.438%
23	9.486	1257	1258	1261	rVB	75980	59061	4.48%	0.395%
24	9.757	1300	1304	1310	rVB	1404944	1275931	96.85%	8.526%
25	9.928	1328	1333	1336	rBV6	11928	18673	1.42%	0.125%
26	10.022	1347	1349	1356	rVB2	28153	28760	2.18%	0.192%
27	10.139	1364	1369	1372	rBV4	13895	18292	1.39%	0.122%
28	10.186	1372	1377	1379	rBV4	11113	16345	1.24%	0.109%
29	10.322	1394	1400	1402	rBV5	21344	36707	2.79%	0.245%
30	10.416	1410	1416	1419	rBV	42445	51148	3.88%	0.342%
31	10.539	1433	1437	1449	rBV	603347	640437	48.61%	4.279%
32	10.681	1457	1461	1468	rVB3	48432	67805	5.15%	0.453%
33	10.992	1511	1514	1517	rBV5	18524	28482	2.16%	0.190%
34	11.086	1526	1530	1533	rBV4	14661	25339	1.92%	0.169%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
Data File : BF113216.D
Acq On : 21 Mar 2019 18:52
Operator : JU/SJ
Sample : K2004-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-20(10-11)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.145	1536	1540	1544	rVB4	41394	52926	4.02%	0.354%
36	11.192	1546	1548	1551	rBV3	15439	23022	1.75%	0.154%
37	11.233	1551	1555	1566	rVV	1140286	1153688	87.57%	7.709%
38	11.428	1586	1588	1592	rBV4	25804	31575	2.40%	0.211%
39	11.492	1597	1599	1602	rVB2	28947	33697	2.56%	0.225%
40	11.586	1613	1615	1617	rBV3	19245	17371	1.32%	0.116%
41	11.769	1643	1646	1651	rBV6	50349	80085	6.08%	0.535%
42	11.880	1663	1665	1669	rVB5	30862	34896	2.65%	0.233%
43	11.980	1679	1682	1684	rBV3	49114	44932	3.41%	0.300%
44	12.004	1684	1686	1691	rVB2	44509	41245	3.13%	0.276%
45	12.180	1714	1716	1719	rVB4	42507	38210	2.90%	0.255%
46	12.816	1820	1824	1827	rBV	973779	831052	63.08%	5.553%
47	13.869	1999	2003	2006	rBV	1095620	1010488	76.70%	6.752%
48	15.280	2239	2243	2247	rBV	638718	767478	58.25%	5.128%


Sum of corrected areas: 14965826

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
Data File : BF113216.D
Acq On : 21 Mar 2019 18:52
Operator : JU/SJ
Sample : K2004-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SB-20(10-11)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

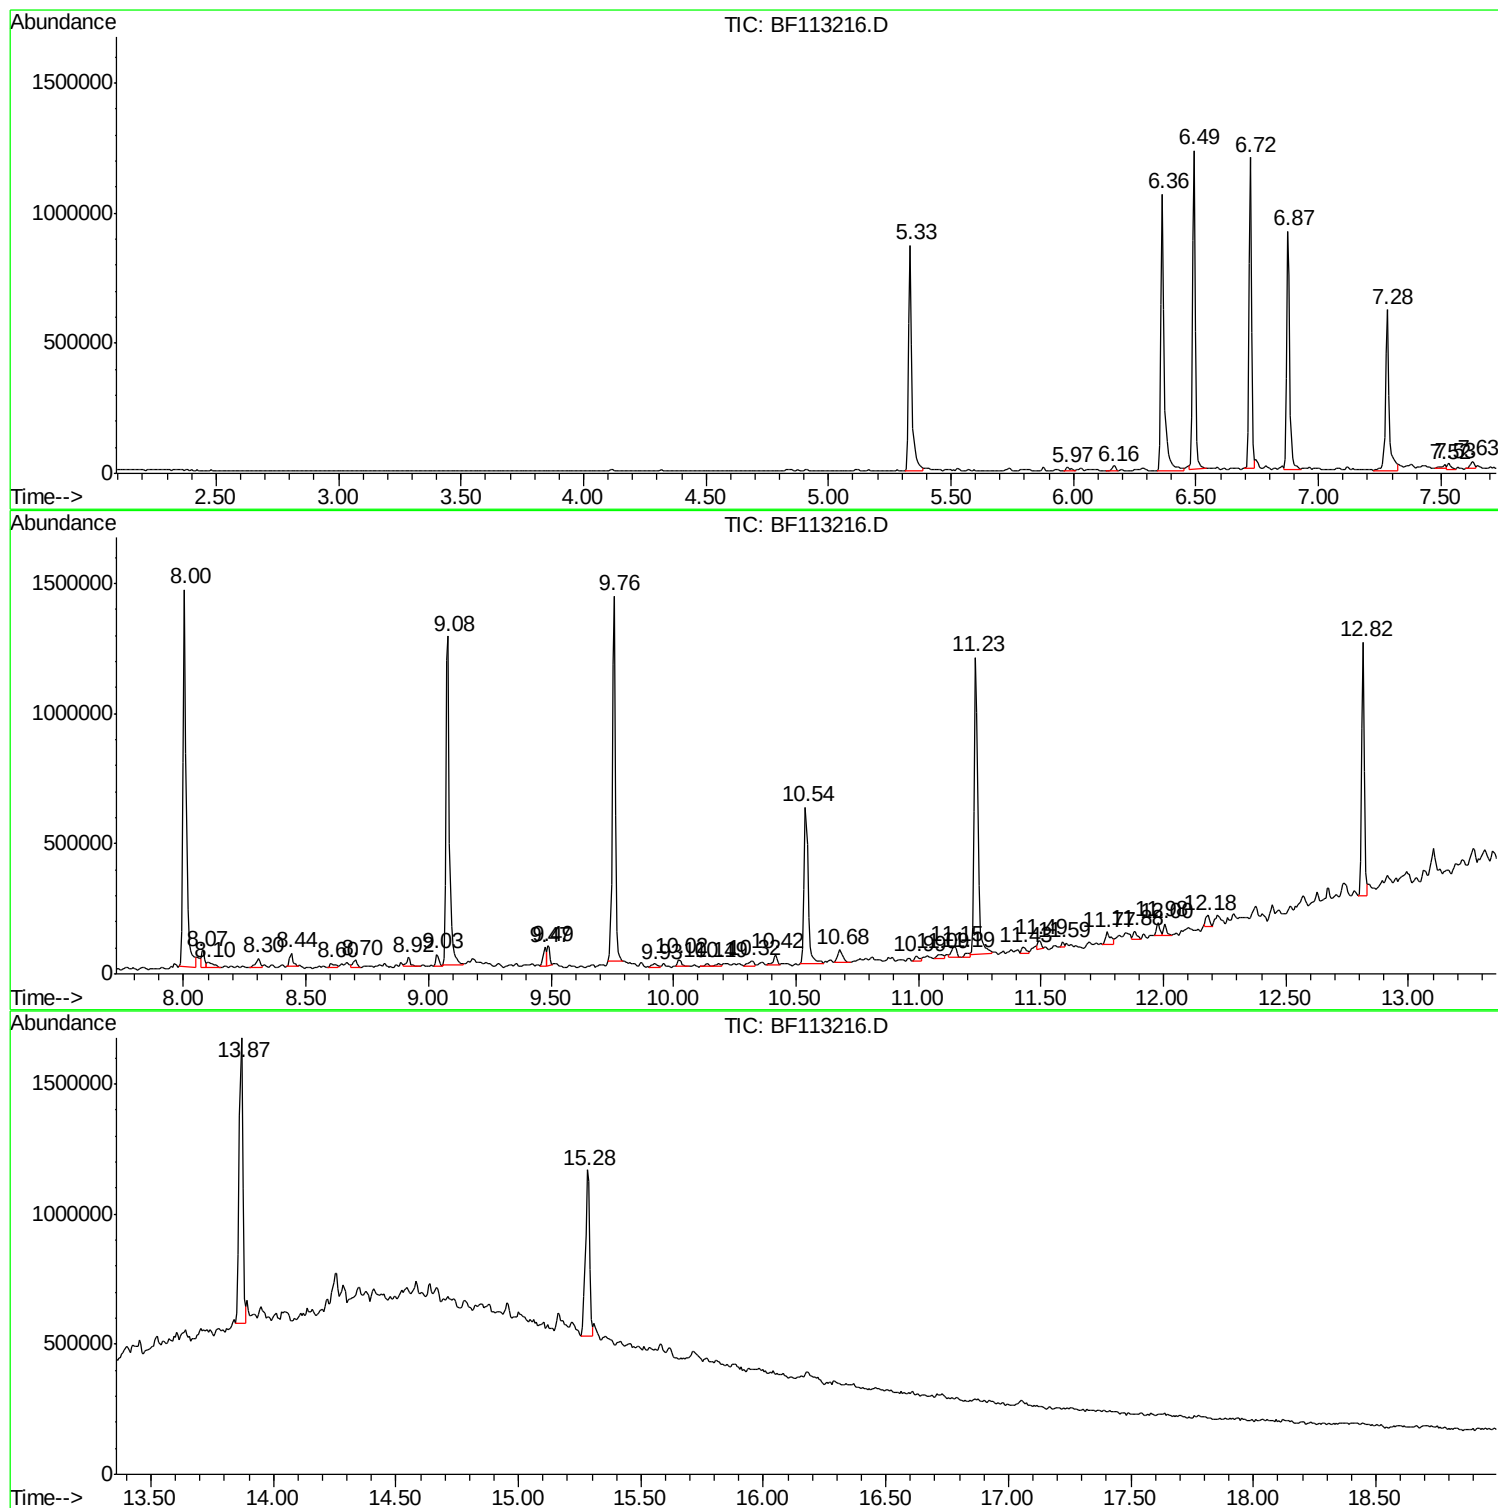

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
Data File : BF113216.D
Acq On : 21 Mar 2019 18:52
Operator : JU/SJ
Sample : K2004-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-20(10-11)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.49 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.49	21.84 ng	1061470	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

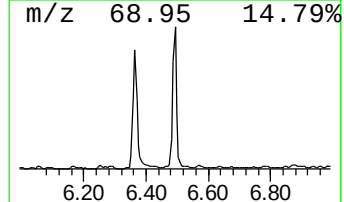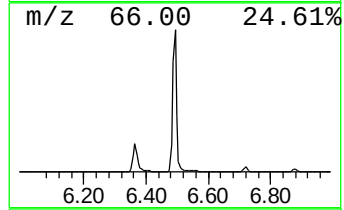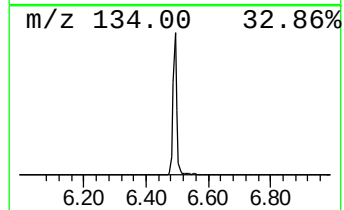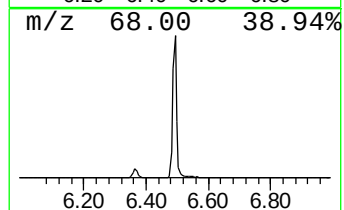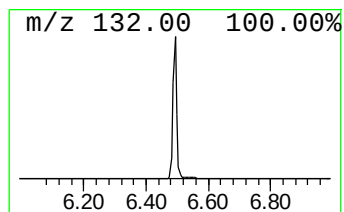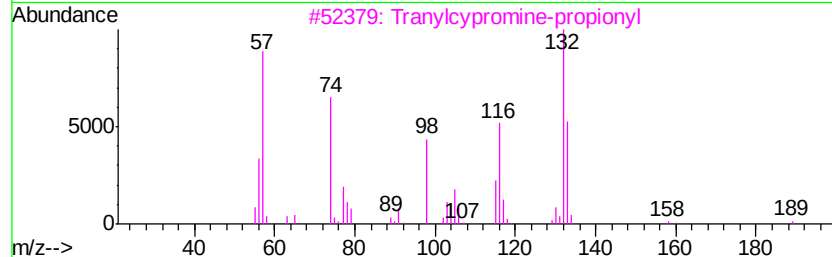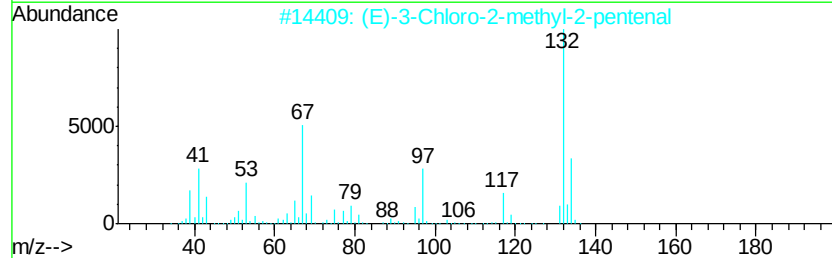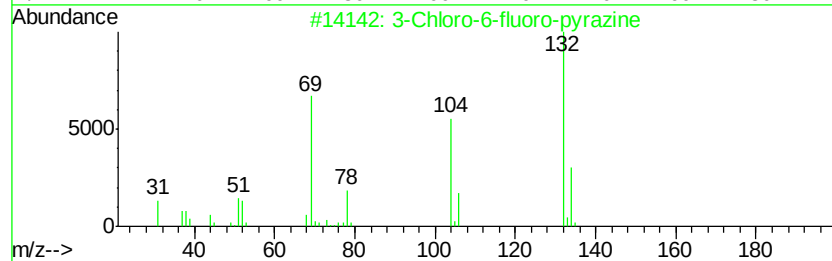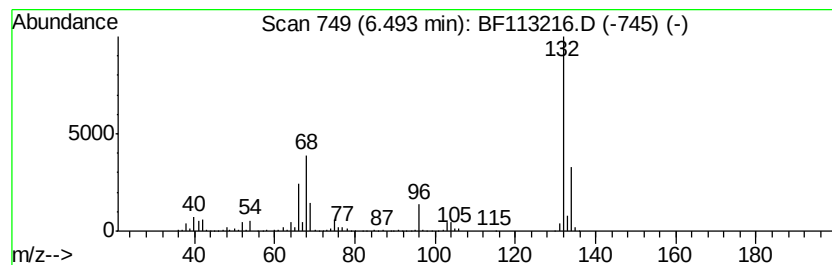

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
Data File : BF113216.D
Acq On : 21 Mar 2019 18:52
Operator : JU/SJ
Sample : K2004-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-20(10-11)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.49	6.49	21.8	ng	1061470	1	6.72	971926	20.0