


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032119\
 Data File : BF113198.D
 Acq On : 21 Mar 2019 10:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

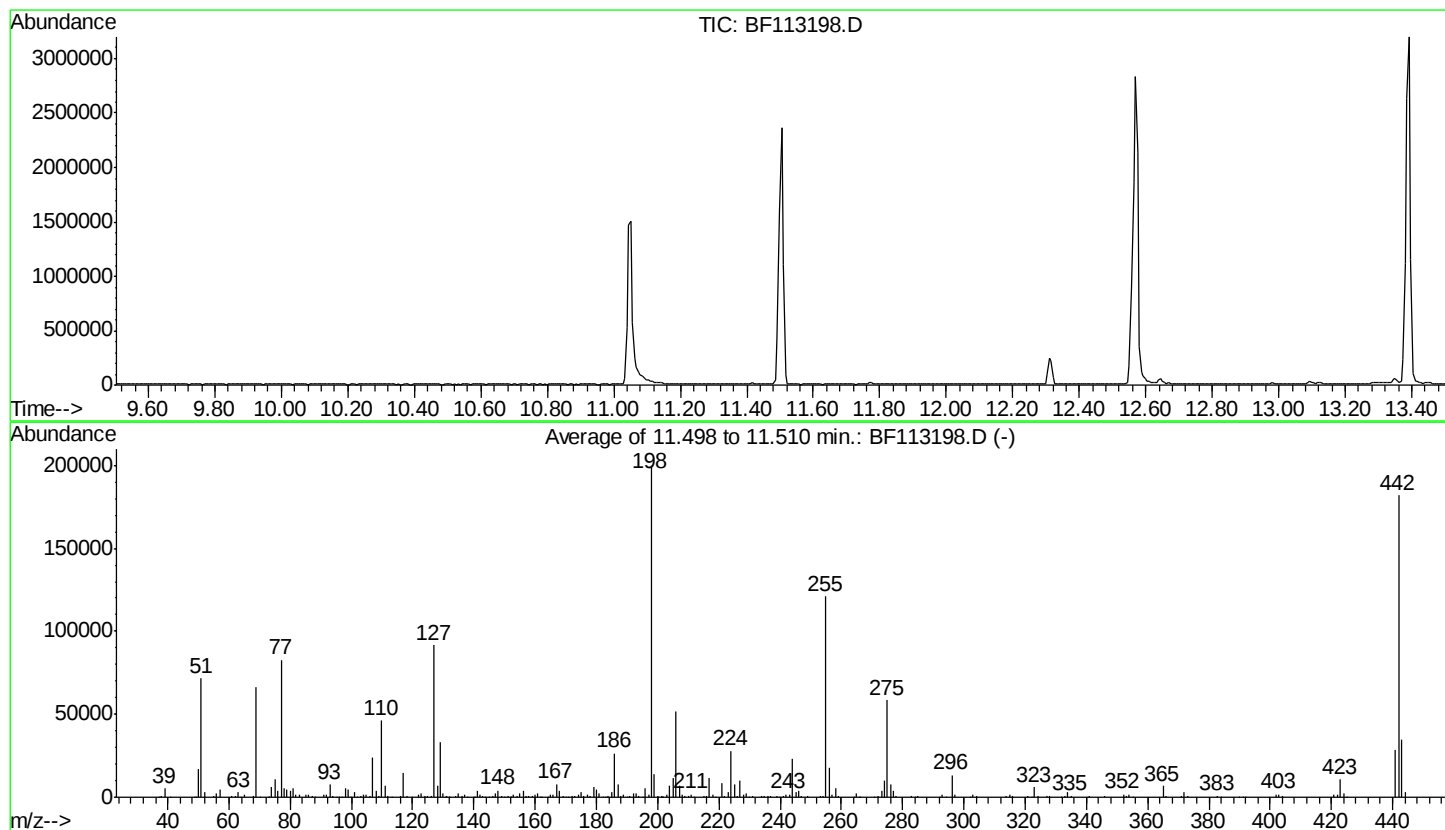

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	71549	PASS
68	69	0.00	2	1.6	1075	PASS
69	198	0.00	100	33.2	66333	PASS
70	69	0.00	2	0.4	248	PASS
127	198	10	80	45.9	91666	PASS
197	198	0.00	2	0.6	1245	PASS
198	198	100	100	100.0	199869	PASS
199	198	5	9	6.8	13592	PASS
275	198	10	60	29.2	58298	PASS
365	198	1	100	3.4	6753	PASS
441	198	0.01	100	14.3	28641	PASS
442	198	50	100	91.0	181837	PASS
443	442	15	24	19.1	34746	PASS