
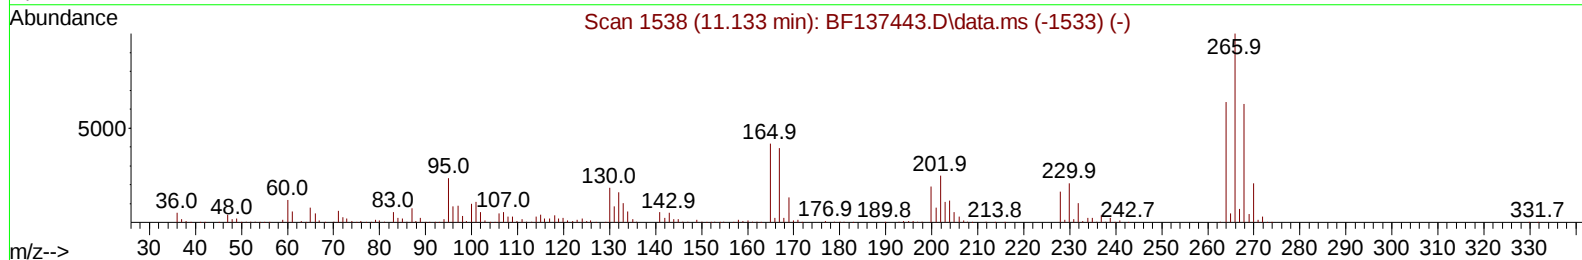
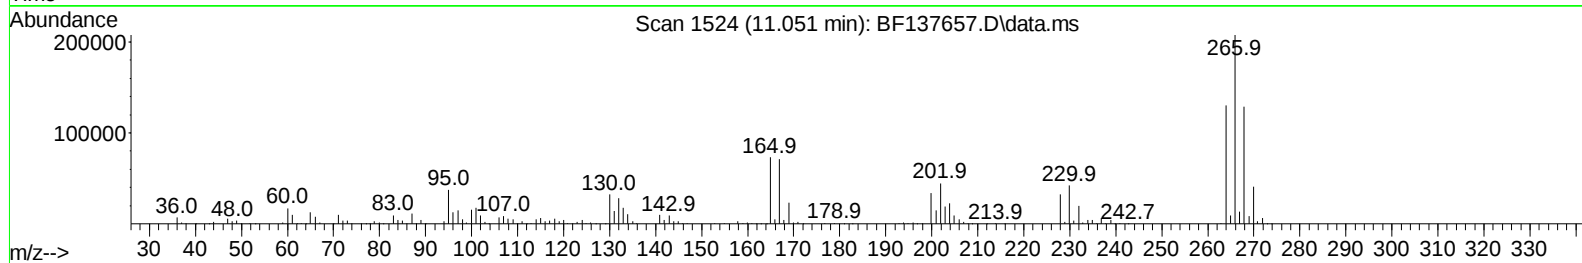


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137657.D
Acq On : 21 Mar 2024 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 17:22:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

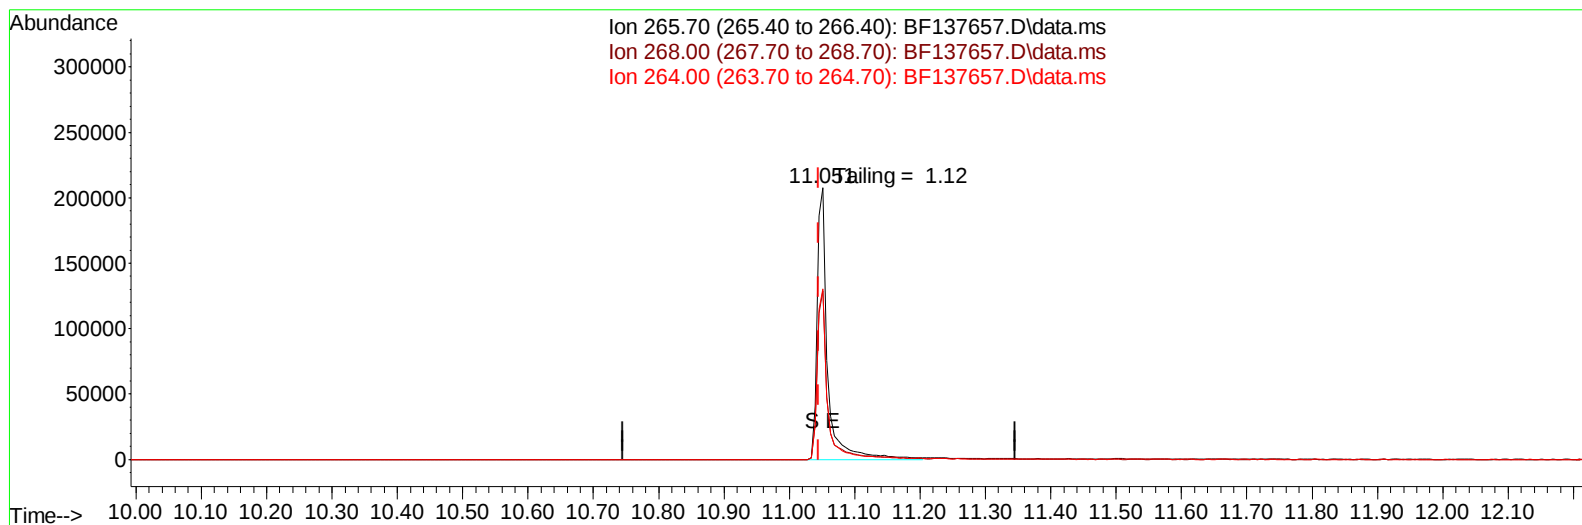

TIC: BF137657.D\data.ms

(70) Pentachlorophenol (C)




11.051min (+ 0.006) 38120.36 ng

response 232975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.11
264.00	63.60	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137657.D
Acq On : 21 Mar 2024 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 17:22:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

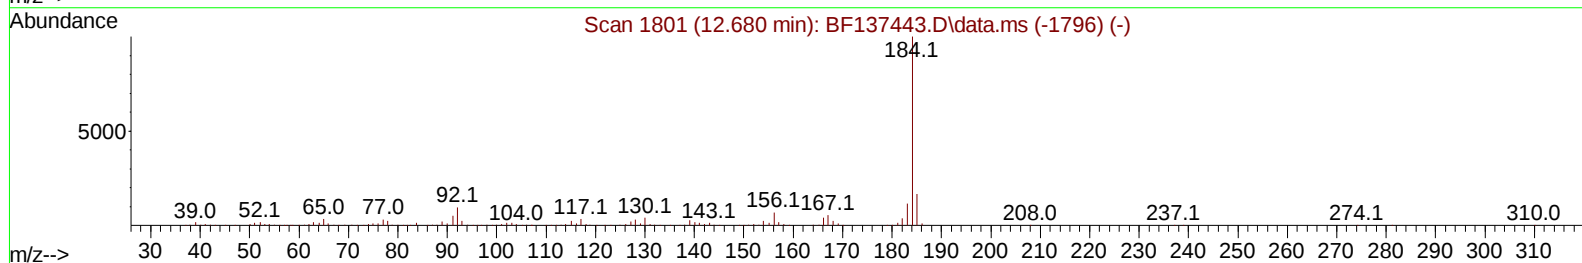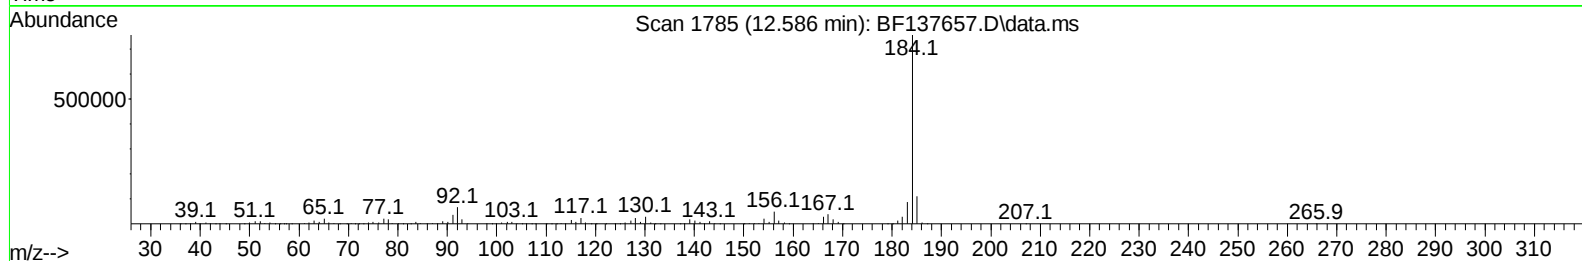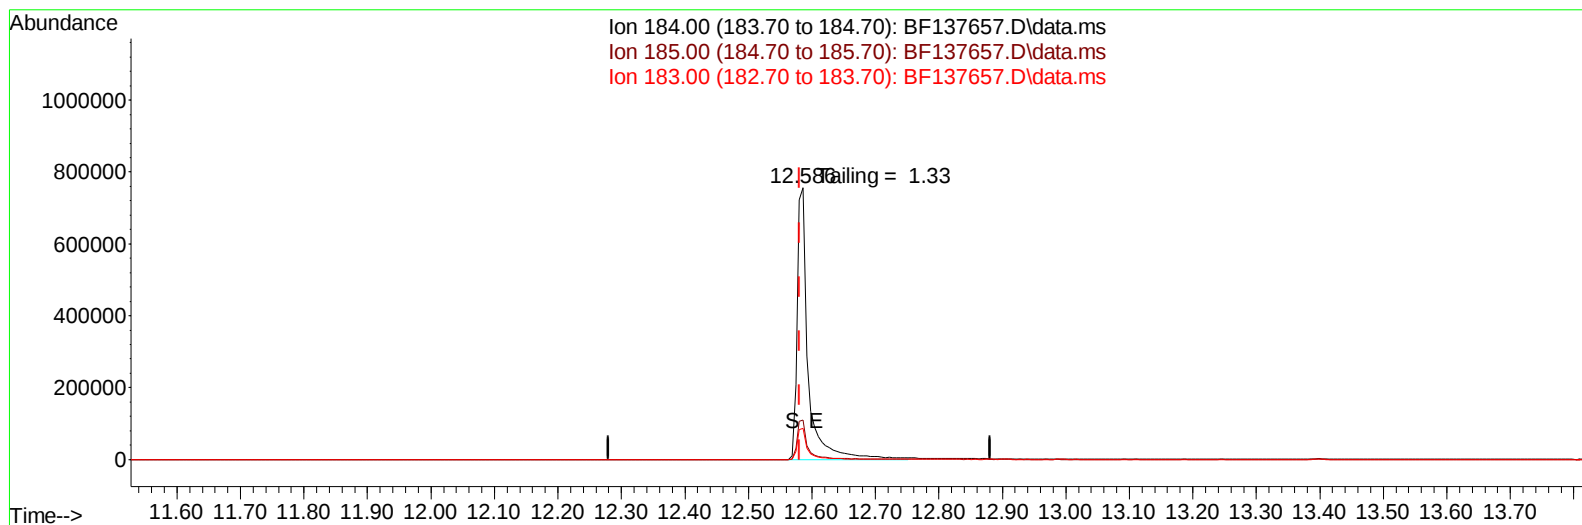

TIC: BF137657.D\data.ms

(77) Benzidine**12.586min (+ 0.006) 0.00 ng****response 936102**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.45
183.00	11.60	11.56
0.00	0.00	0.00