

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
 Data File : BF137660.D
 Acq On : 21 Mar 2024 14:51
 Operator : CG\JU
 Sample : PB159709BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159709BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	485	489	499	rBV	60817	100902	1.47%	0.237%
2	5.345	550	554	569	rBV	4914842	5889188	85.84%	13.850%
3	6.369	723	728	731	rBV	4955853	5835914	85.06%	13.724%
4	6.722	785	788	810	rBV	1278952	1301166	18.97%	3.060%
5	7.292	880	885	888	rBV	3642586	3882823	56.59%	9.131%
6	8.004	1003	1006	1028	rBV	1783149	1770823	25.81%	4.164%
7	9.086	1185	1190	1193	rBV	6887187	6860738	100.00%	16.134%
8	9.757	1300	1304	1319	rBV	2219926	1989232	28.99%	4.678%
9	10.551	1434	1439	1464	rBV	3727833	3783862	55.15%	8.899%
10	11.239	1553	1556	1578	rBV	1902618	1933184	28.18%	4.546%
11	12.833	1822	1827	1830	rBV	6785115	6525549	95.11%	15.346%
12	13.874	2001	2004	2019	rBV	1172331	1315146	19.17%	3.093%
13	15.298	2242	2246	2264	rBV	763402	1168718	17.03%	2.748%
14	15.745	2317	2322	2330	rVB	55237	83449	1.22%	0.196%
15	16.221	2398	2403	2411	rBV3	43660	81505	1.19%	0.192%




Sum of corrected areas: 42522199

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137660.D
Acq On : 21 Mar 2024 14:51
Operator : CG\JU
Sample : PB159709BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

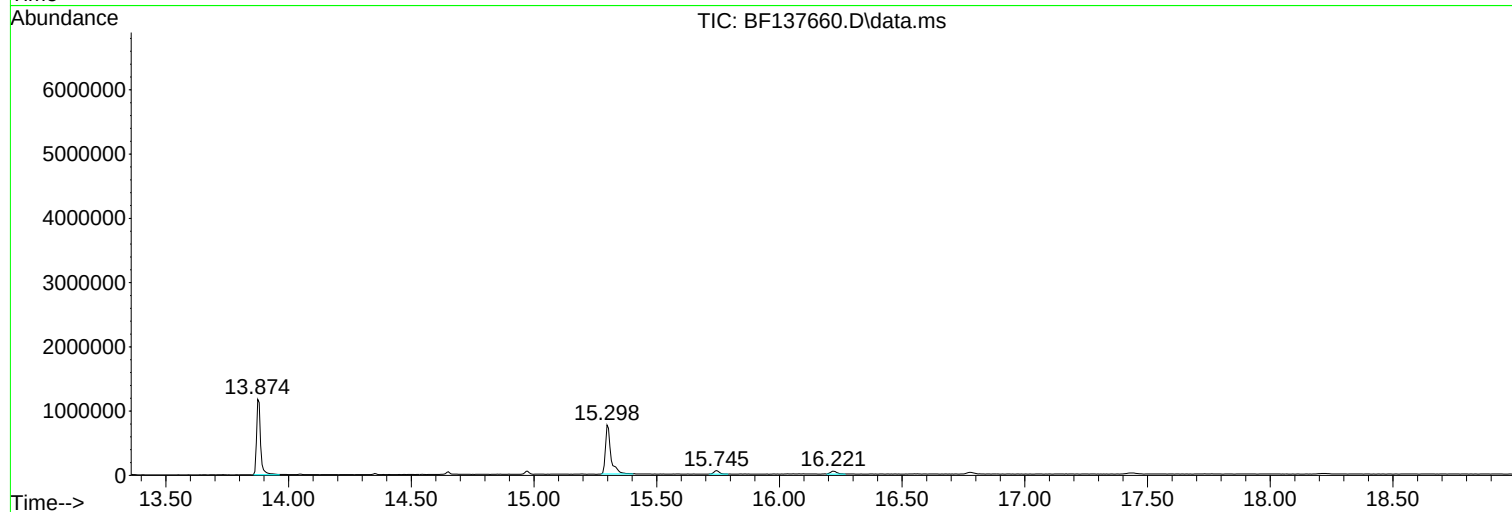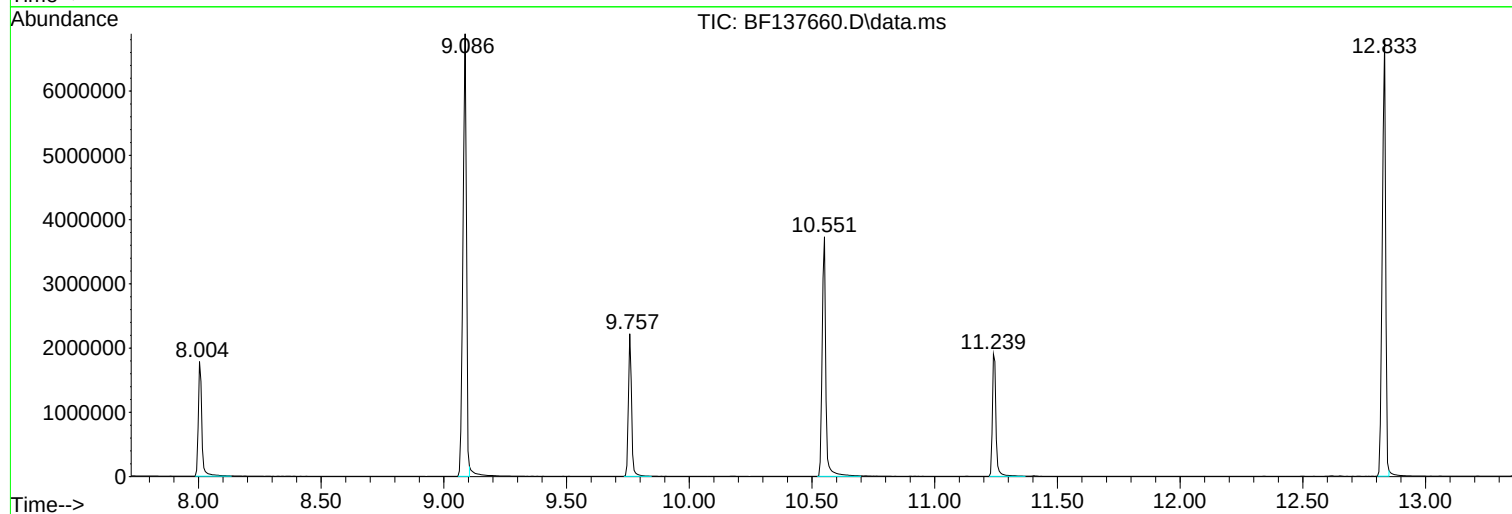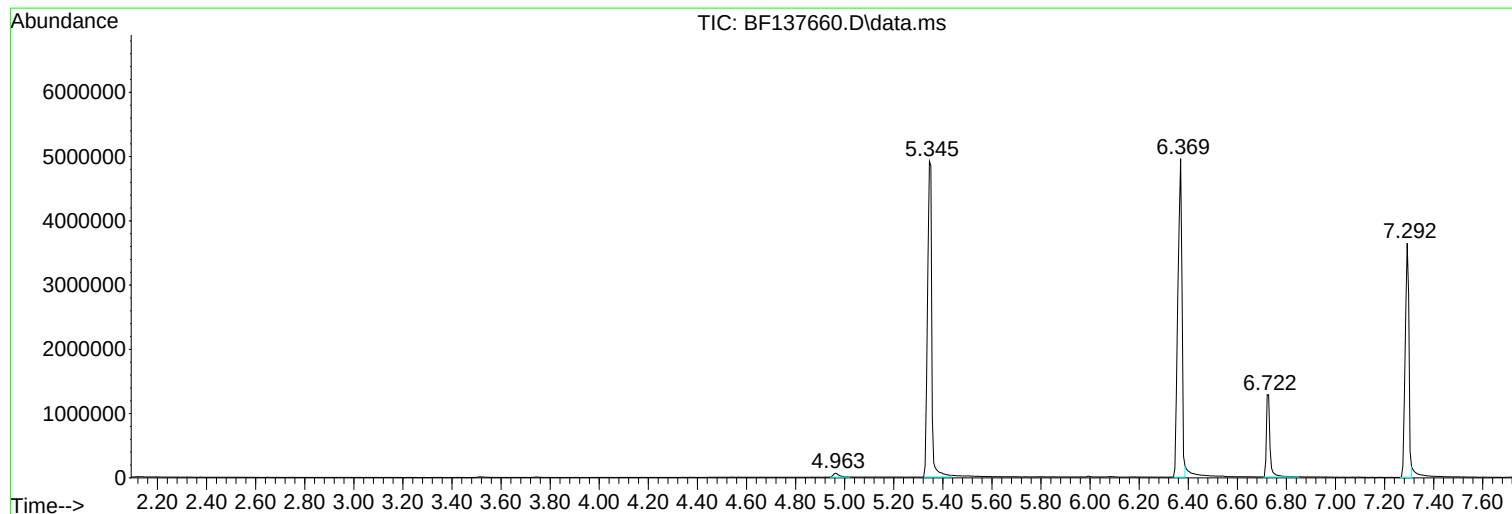

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137660.D
Acq On : 21 Mar 2024 14:51
Operator : CG\JU
Sample : PB159709BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137660.D
Acq On : 21 Mar 2024 14:51
Operator : CG\JU
Sample : PB159709BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------