

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
 Data File : BF137671.D
 Acq On : 21 Mar 2024 20:25
 Operator : CG\JU
 Sample : P1815-01 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-032024

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	549	552	566	rBV	84121	157946	14.32%	2.023%
2	6.369	725	728	742	rBV	74742	160230	14.53%	2.052%
3	6.722	785	788	805	rBV	802667	849244	77.01%	10.876%
4	7.298	883	886	895	rBV	41291	82796	7.51%	1.060%
5	8.004	1003	1006	1021	rBV	1069529	1050739	95.28%	13.457%
6	9.080	1186	1189	1201	rBV	223274	243644	22.09%	3.120%
7	9.204	1206	1210	1213	rVV2	15289	15748	1.43%	0.202%
8	9.622	1278	1281	1286	rBV	19197	20553	1.86%	0.263%
9	9.757	1301	1304	1321	rVB	1254623	1052449	95.44%	13.479%
10	10.551	1435	1439	1449	rBV	59915	85872	7.79%	1.100%
11	10.663	1455	1458	1464	rVB3	15067	20373	1.85%	0.261%
12	11.145	1536	1540	1545	rVB4	12640	15866	1.44%	0.203%
13	11.239	1553	1556	1559	rBV	1085377	937069	84.97%	12.001%
14	11.321	1567	1570	1574	rVB	16381	15776	1.43%	0.202%
15	11.745	1638	1642	1645	rBV2	21777	25364	2.30%	0.325%
16	11.774	1645	1647	1652	rVB	22005	24045	2.18%	0.308%
17	11.851	1658	1660	1663	rBV2	28331	34148	3.10%	0.437%
18	11.880	1663	1665	1670	rVB3	17920	18507	1.68%	0.237%
19	12.045	1689	1693	1695	rBV5	12061	17592	1.60%	0.225%
20	12.221	1720	1723	1724	rBV3	12134	12419	1.13%	0.159%
21	12.292	1732	1735	1738	rBV	30641	33525	3.04%	0.429%
22	12.327	1738	1741	1743	rVV4	29755	35394	3.21%	0.453%
23	12.380	1747	1750	1753	rBV5	15881	19206	1.74%	0.246%
24	12.451	1759	1762	1767	rBV	177550	164443	14.91%	2.106%
25	12.610	1786	1789	1791	rBV3	14754	16550	1.50%	0.212%
26	12.680	1796	1801	1804	rBV	205104	225180	20.42%	2.884%
27	12.739	1809	1811	1815	rVB3	15208	15837	1.44%	0.203%
28	12.821	1822	1825	1834	rBV	265915	274088	24.85%	3.510%
29	12.898	1836	1838	1845	rVV6	19114	35038	3.18%	0.449%
30	13.063	1863	1866	1867	rBV2	24866	24765	2.25%	0.317%
31	13.110	1872	1874	1878	rBV	29906	34354	3.12%	0.440%
32	13.204	1888	1890	1893	rBV2	18952	13722	1.24%	0.176%
33	13.233	1893	1895	1897	rBV	20175	18617	1.69%	0.238%
34	13.874	2000	2004	2008	rBV	1037374	1102759	100.00%	14.123%
35	14.898	2175	2178	2184	rVB	88061	138055	12.52%	1.768%
36	15.298	2243	2246	2251	rBV	544759	664676	60.27%	8.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137671.D
Acq On : 21 Mar 2024 20:25
Operator : CG\JU
Sample : P1815-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-032024

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.956	2355	2358	2366	rVB3	95223	151677	13.75%	1.943%
----	--------	------	------	------	------	-------	--------	--------	--------



Sum of corrected areas: 7808266

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137671.D
Acq On : 21 Mar 2024 20:25
Operator : CG\JU
Sample : P1815-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-032024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

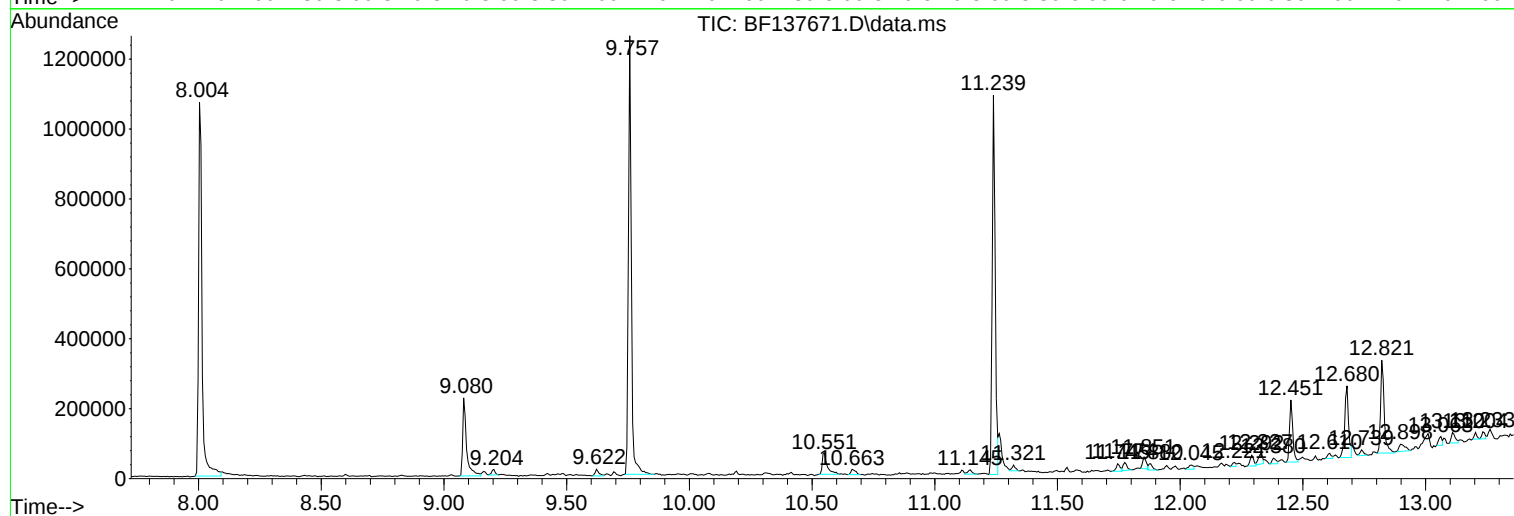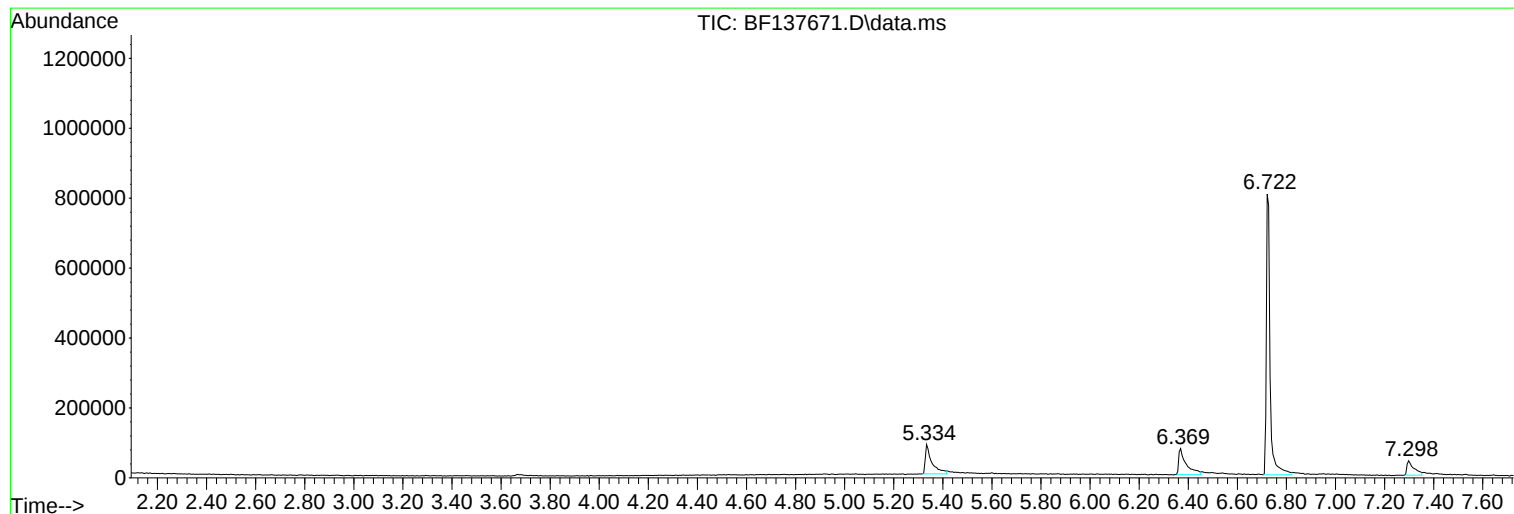

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137671.D
Acq On : 21 Mar 2024 20:25
Operator : CG\JU
Sample : P1815-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-032024










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 .beta.-iso-Methyl ionone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.956	4.56 ng	151677	Perylene-d12	15.298

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		.beta.-iso-Methyl ionone	206	C14H22O	1000285-40-2	68
2		Baccharane	414	C30H54	036441-74-4	68
3		28-Nor-17.beta.(H)-hopane	398	C29H50	036728-72-0	64
4		28-Nor-17.alpha.(H)-hopane	398	C29H50	053584-60-4	55
5		Damascone, .beta.-	192	C13H20O	023726-91-2	38

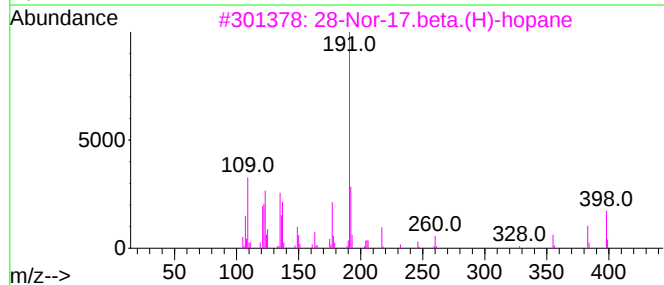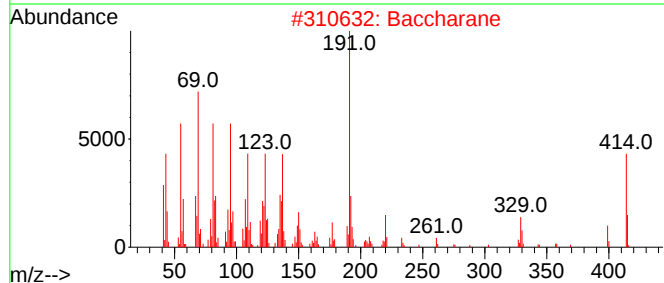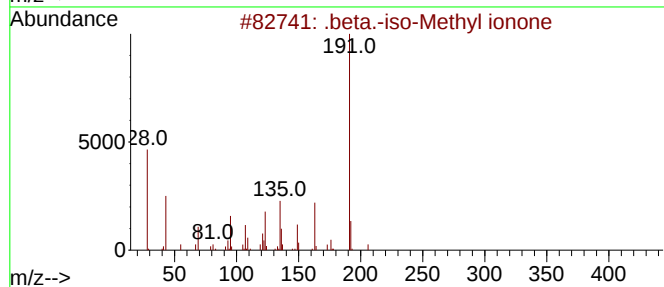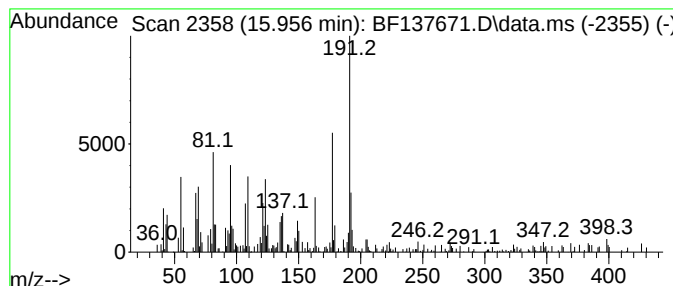

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137671.D
Acq On : 21 Mar 2024 20:25
Operator : CG\JU
Sample : P1815-01 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-032024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
.beta.-iso-Meth...	15.956	4.6	ng	151677	6	15.298	664676	20.0