
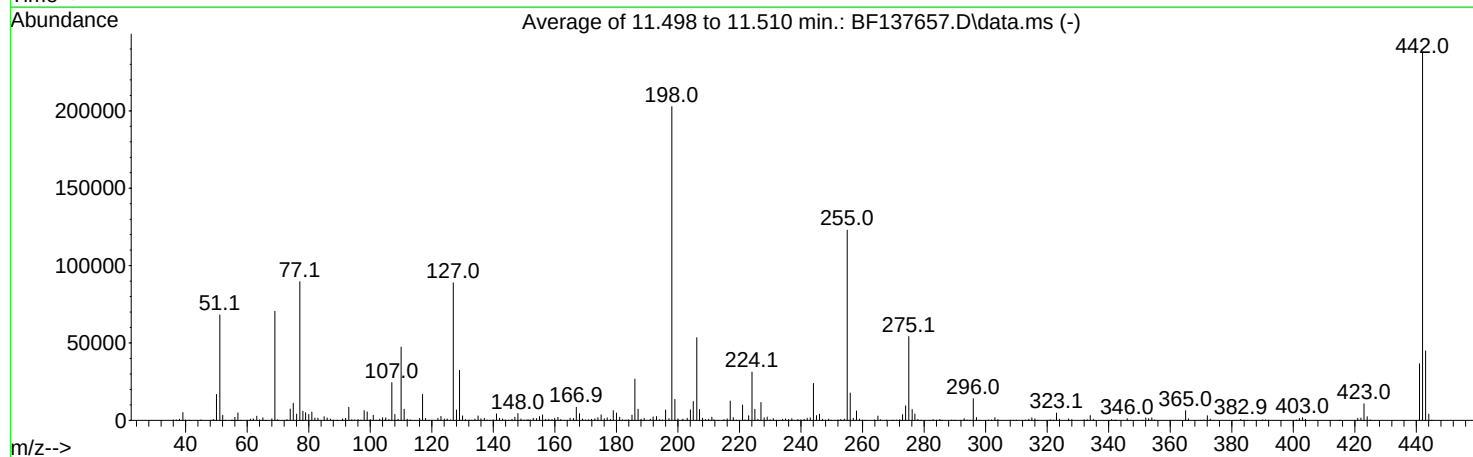


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137657.D
Acq On : 21 Mar 2024 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

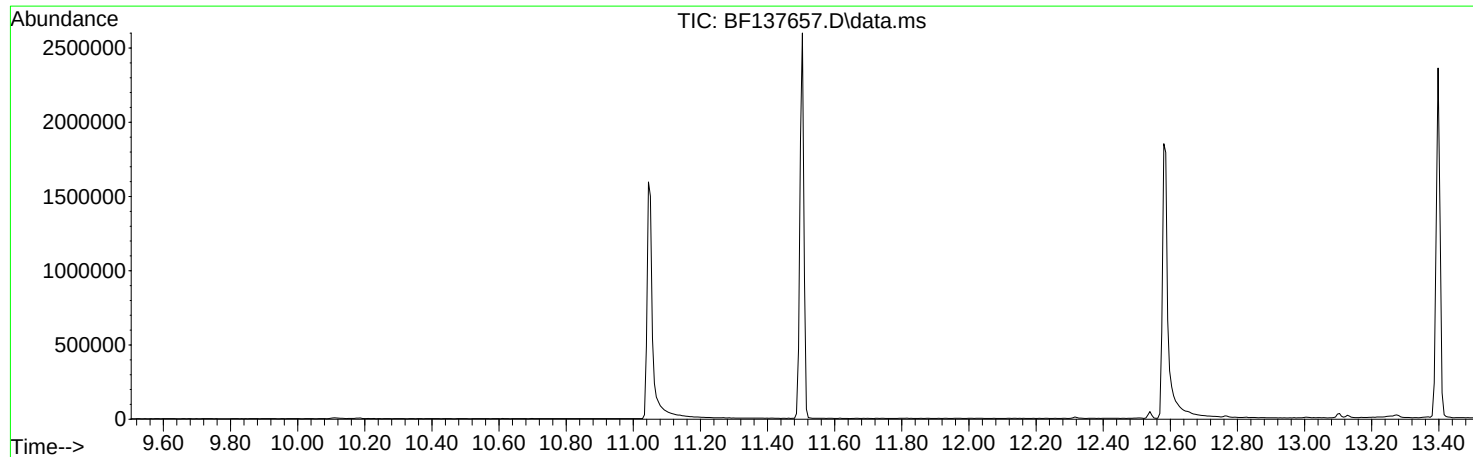




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	68101	PASS
68	69	0.00	2	1.5	1092	PASS
69	198	0.00	100	34.8	70536	PASS
70	69	0.00	2	0.6	436	PASS
127	198	10	80	43.8	88877	PASS
197	198	0.00	2	0.5	1102	PASS
198	198	100	100	100.0	202765	PASS
199	198	5	9	6.7	13522	PASS
275	198	10	60	26.7	54136	PASS
365	198	1	100	3.1	6351	PASS
441	198	0.01	100	18.1	36619	PASS
442	442	50	100	100.0	237696	PASS
443	442	15	24	18.9	44920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137657.D
Acq On : 21 Mar 2024 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 21 17:22:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

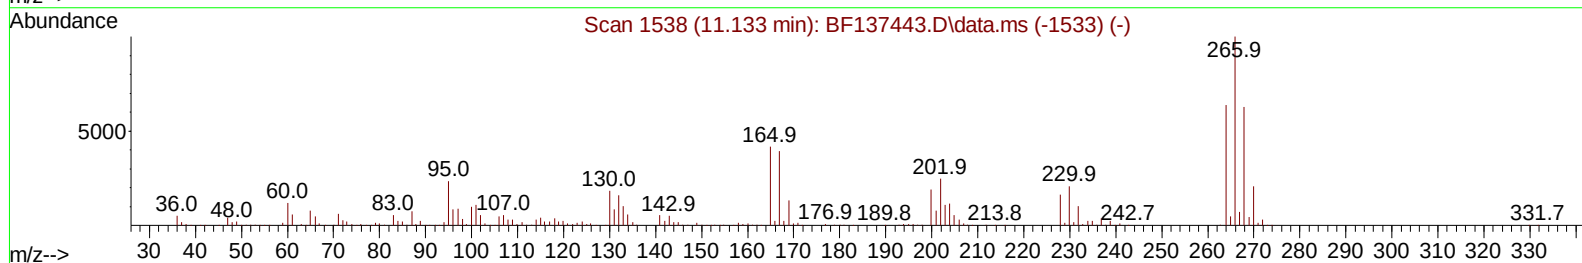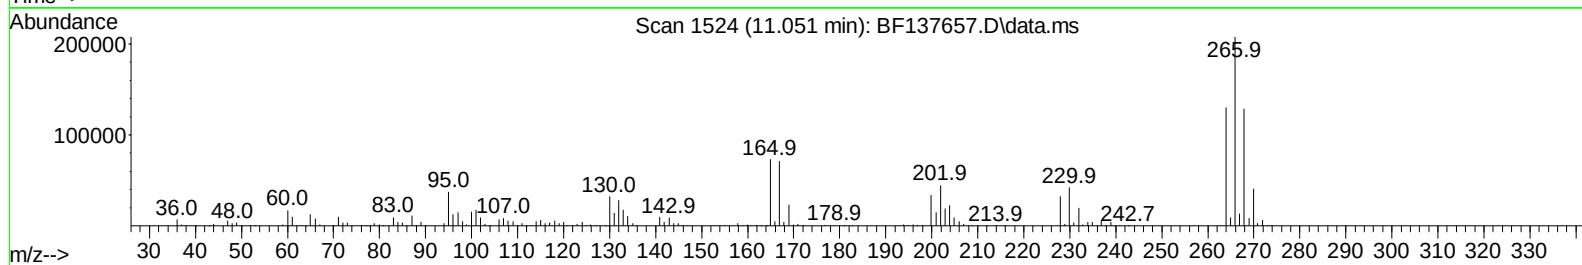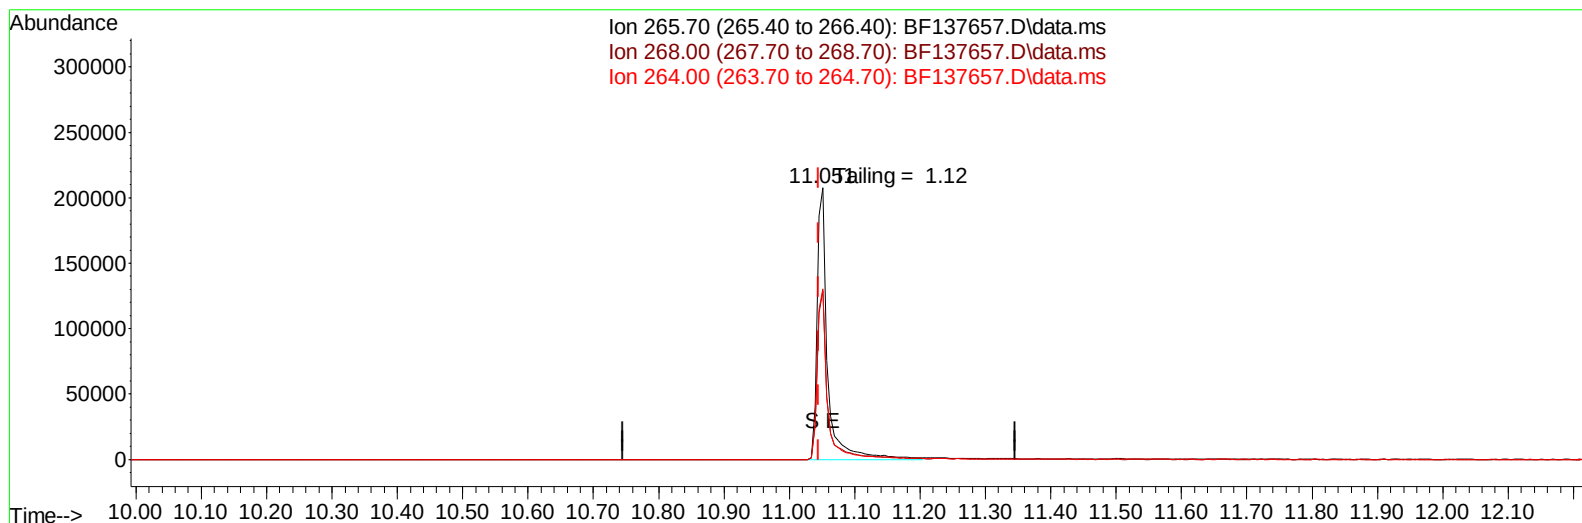

TIC: BF137657.D\data.ms

(70) Pentachlorophenol (C)

11.051min (+ 0.006) 38120.36 ng




response 232975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.11
264.00	63.60	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032124\
Data File : BF137657.D
Acq On : 21 Mar 2024 12:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 21 17:22:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

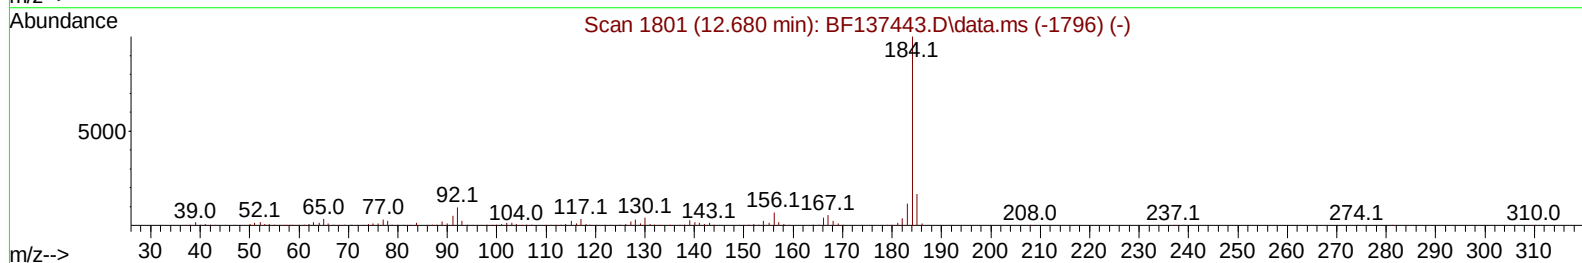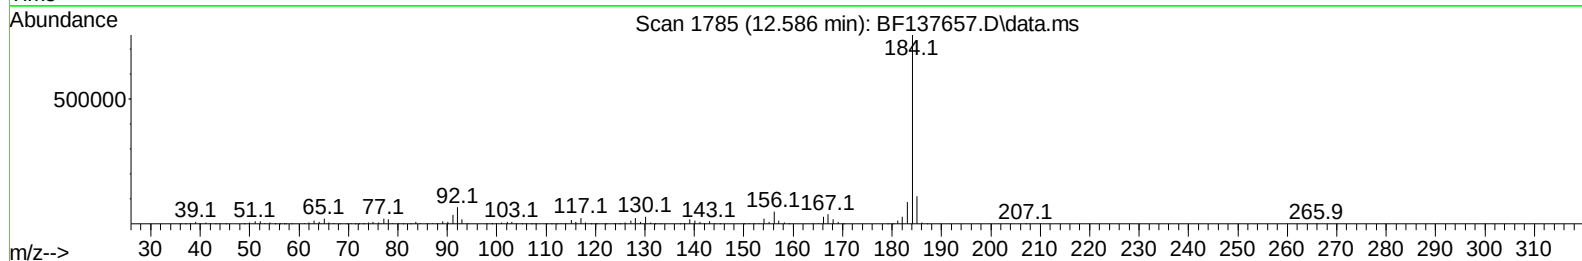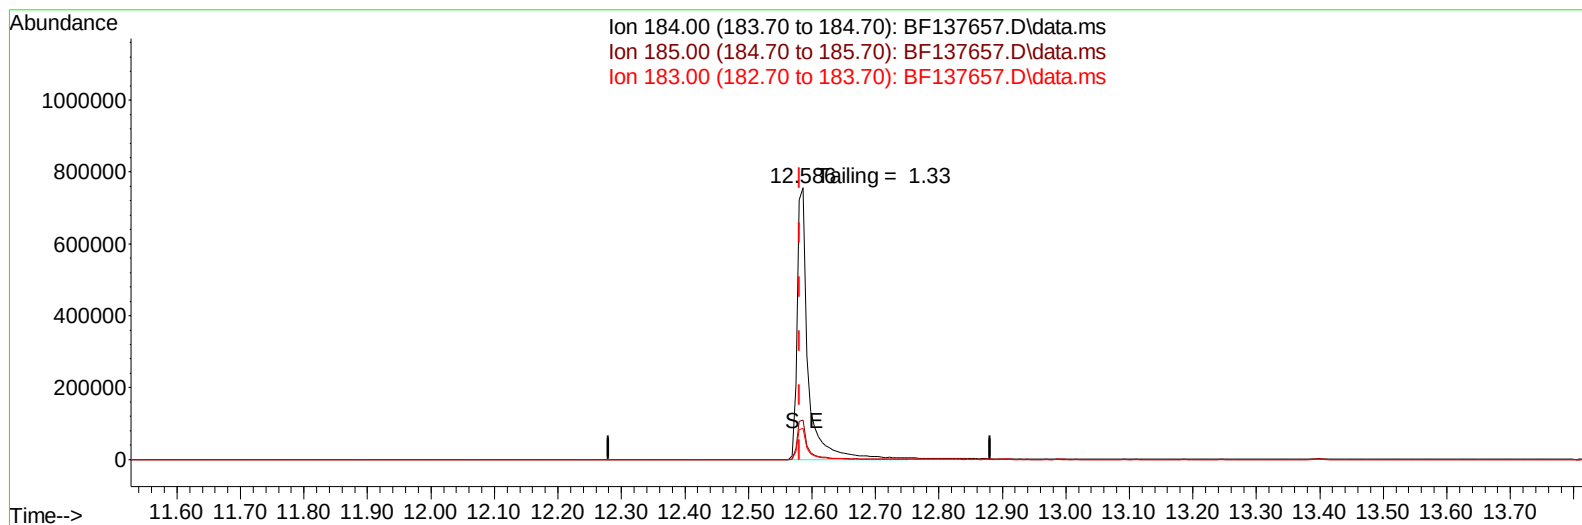

TIC: BF137657.D\data.ms

(77) Benzidine

12.586min (+ 0.006) 0.00 ng

response 936102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.45
183.00	11.60	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2024	BNA_F	<u>BF137657.D</u>
Compound Name	Response	Retention Time
DDT	298907	13.398
DDD	8456	13.104
DDE	1221	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9677	308584	3.14

Instrument :
BNA_F
ClientSampleId :
DFTPP