
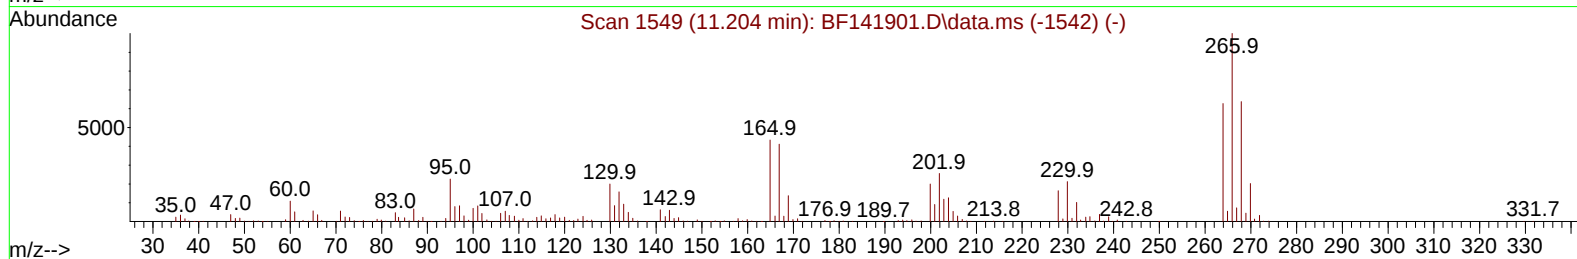
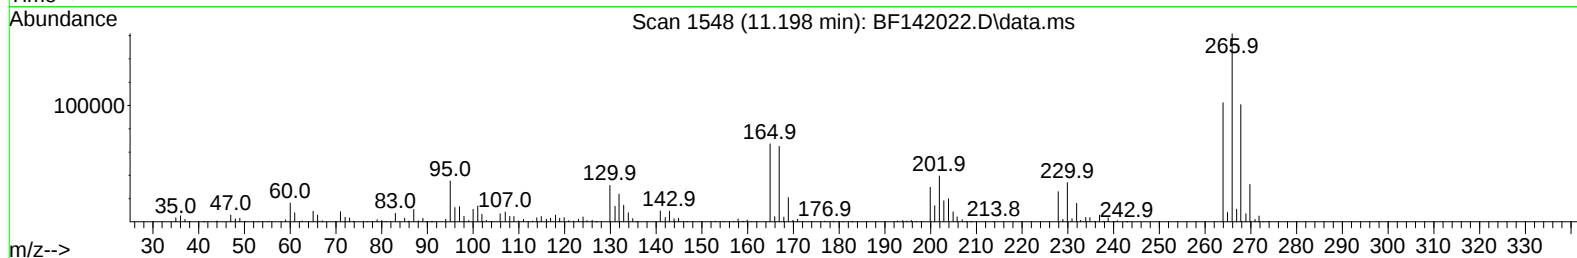


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032125\
Data File : BF142022.D
Acq On : 21 Mar 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 11:49:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

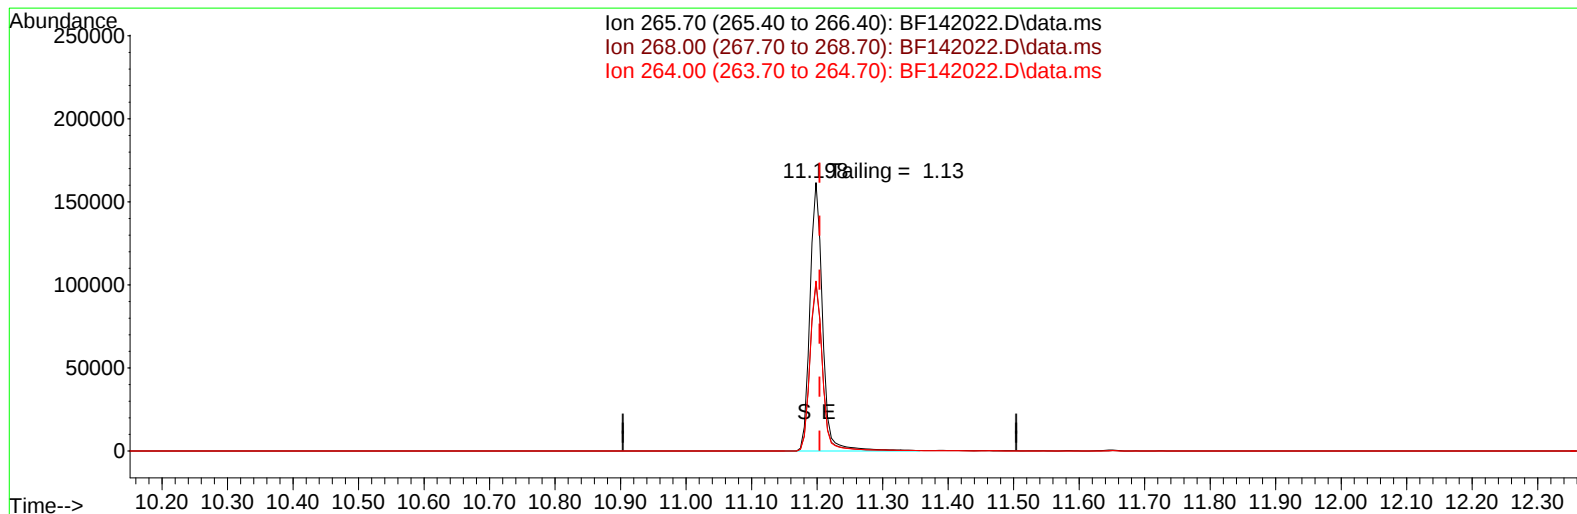

TIC: BF142022.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 12886.67 ng

response 215449

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.32
264.00	62.70	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032125\
Data File : BF142022.D
Acq On : 21 Mar 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 11:49:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

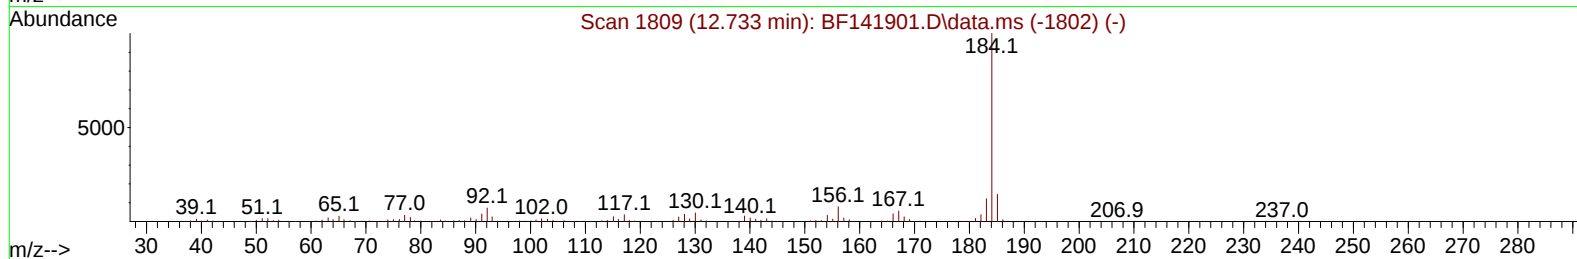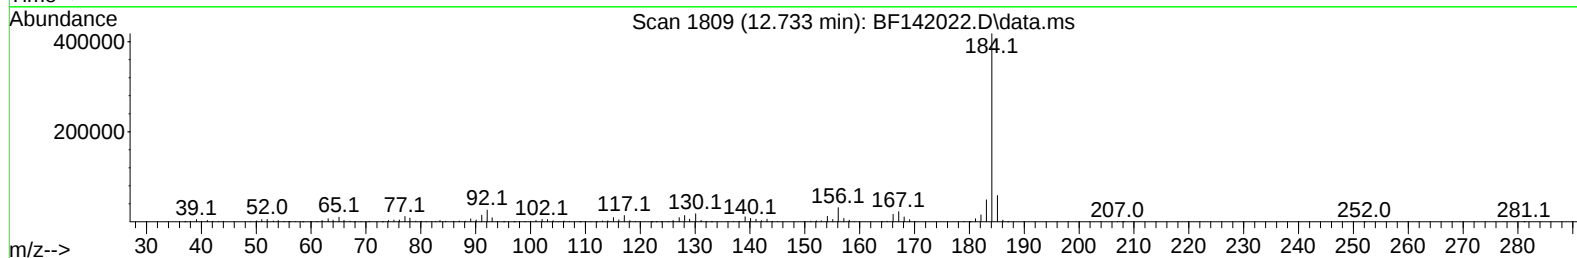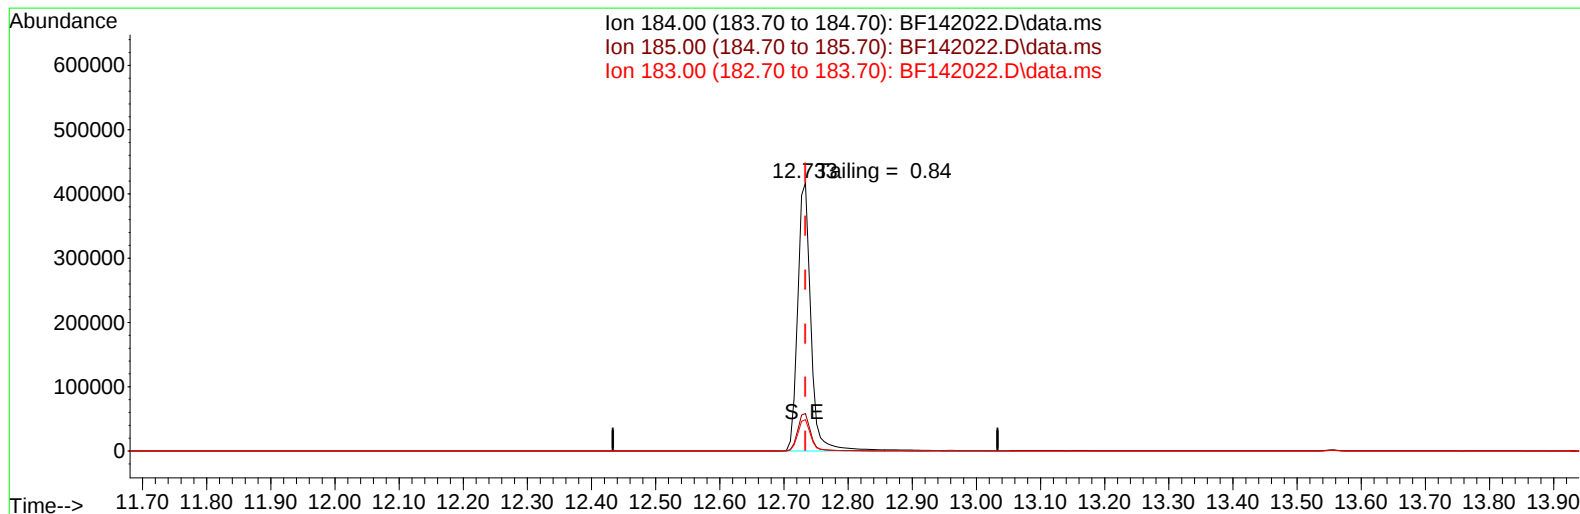

TIC: BF142022.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 26852.19 ng

response 603543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	12.10	11.72
0.00	0.00	0.00