
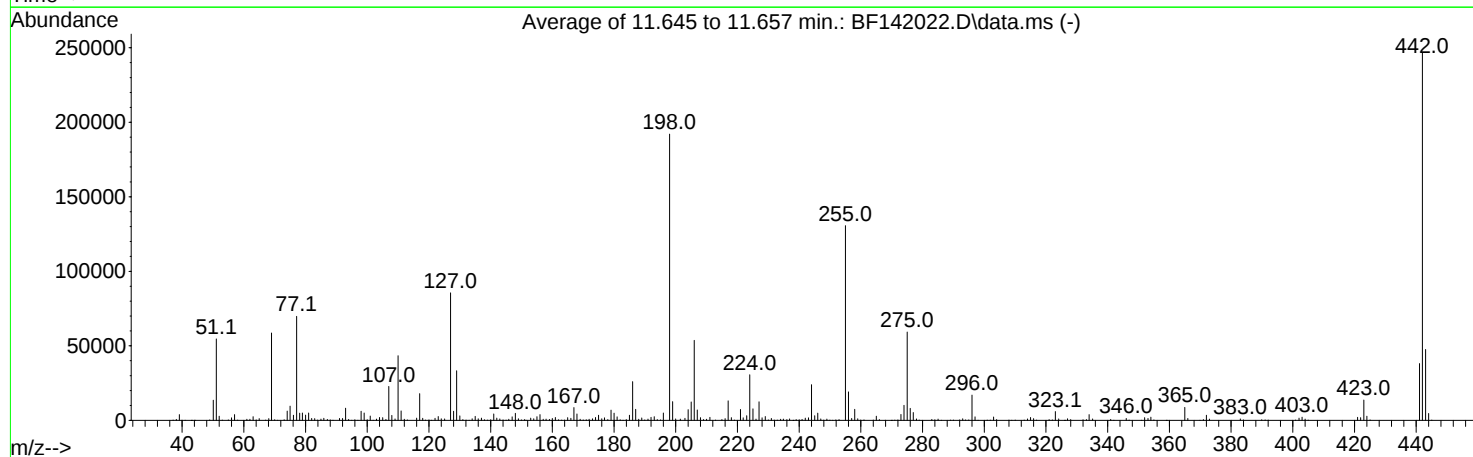


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032125\
Data File : BF142022.D
Acq On : 21 Mar 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

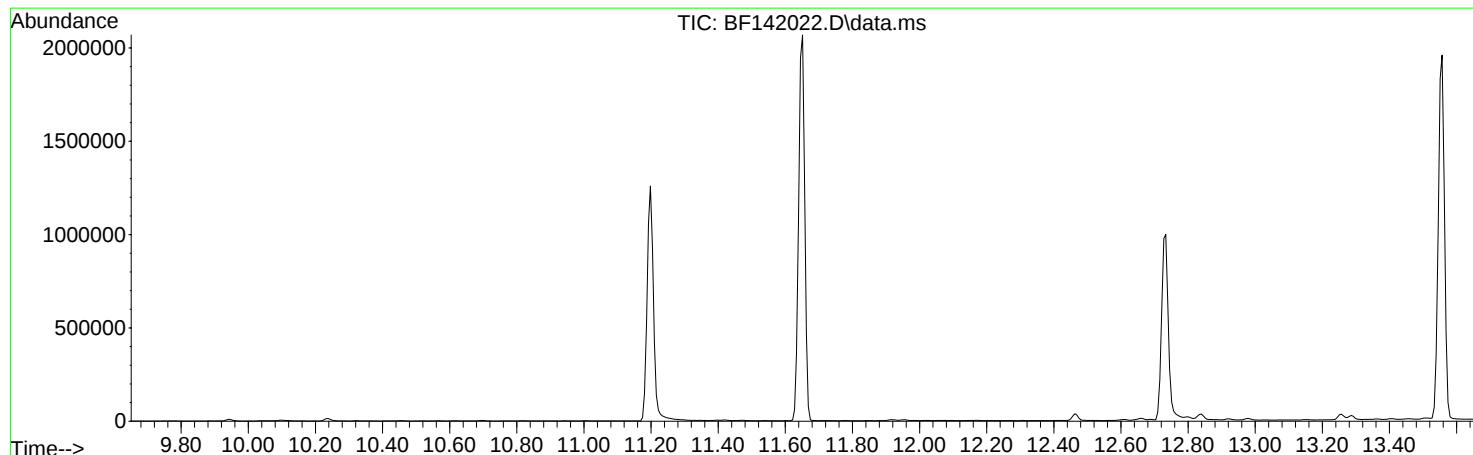

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	54696	PASS
68	69	0.00	2	1.9	1140	PASS
69	198	0.00	100	30.5	58637	PASS
70	69	0.00	2	0.7	384	PASS
127	198	10	80	44.5	85512	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	192043	PASS
199	198	5	9	6.5	12551	PASS
275	198	10	60	30.9	59285	PASS
365	198	1	100	4.6	8758	PASS
441	198	0.01	100	19.8	38109	PASS
442	442	50	100	100.0	246805	PASS
443	442	15	24	19.3	47605	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/21/2025	BNA_F	<u>BF142022.D</u>
Compound Name	Response	Retention Time
DDT	507083	13.557
DDD	15007	13.257
DDE	1598	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16605	523688	3.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032125\
Data File : BF142022.D
Acq On : 21 Mar 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 21 11:49:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

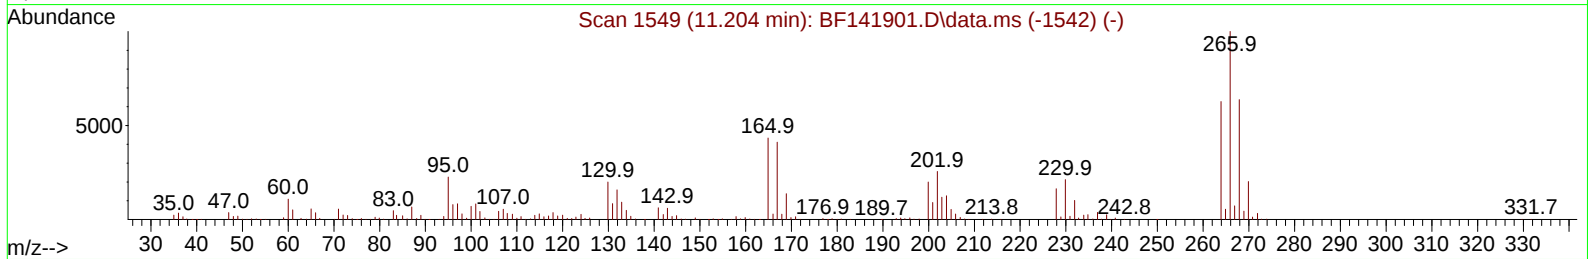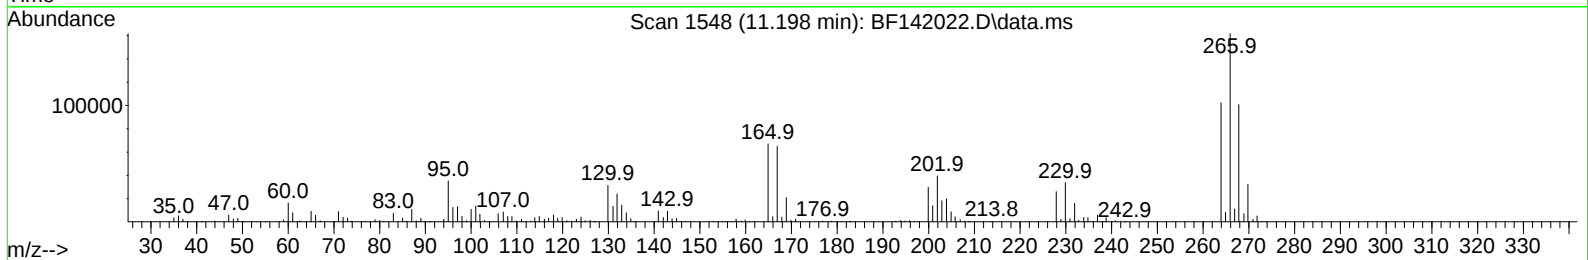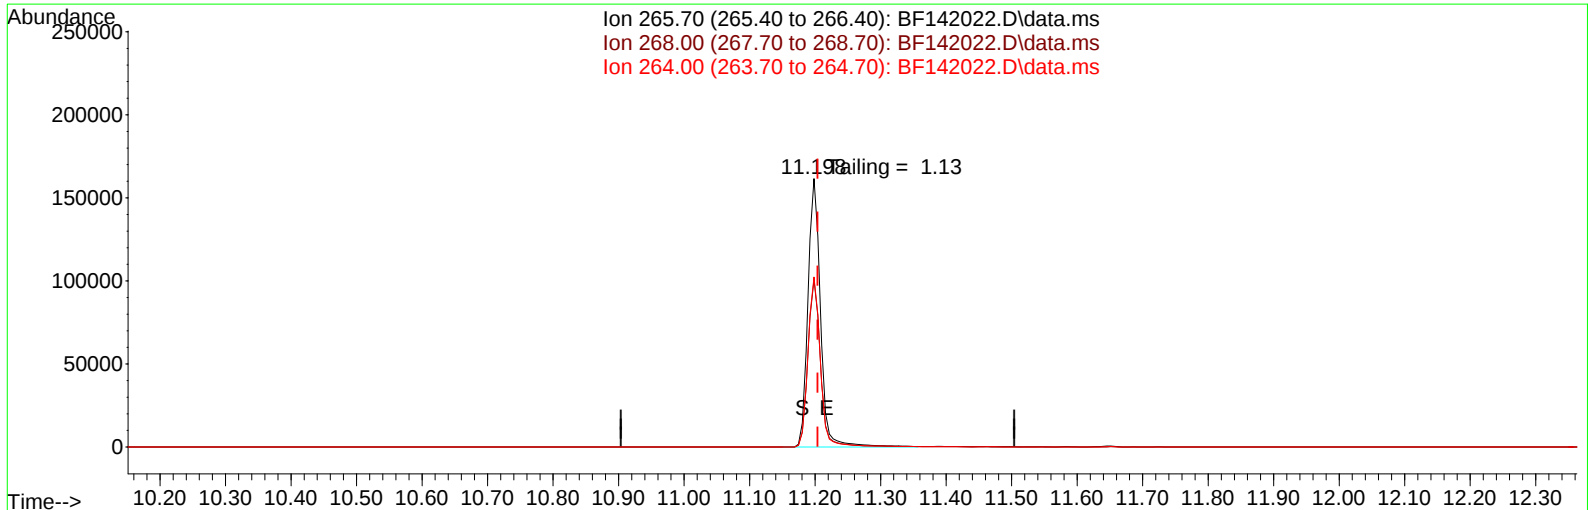

TIC: BF142022.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 12886.67 ng




response 215449

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.32
264.00	62.70	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032125\
Data File : BF142022.D
Acq On : 21 Mar 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 21 11:49:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

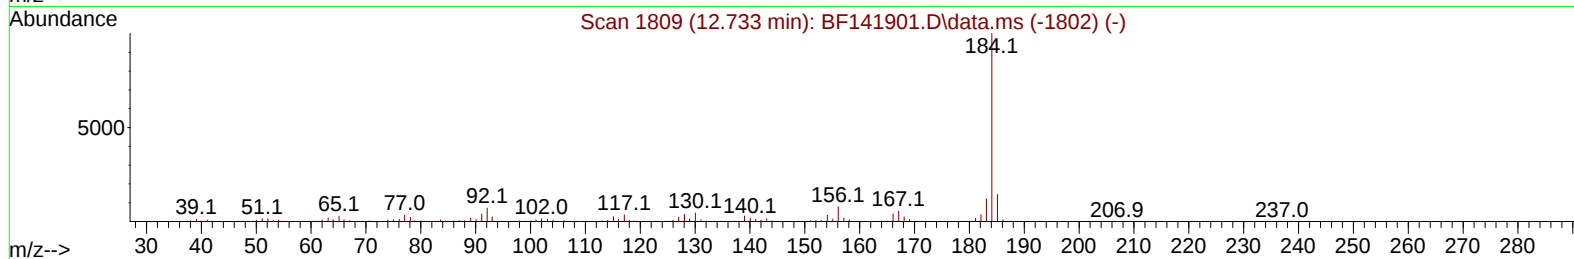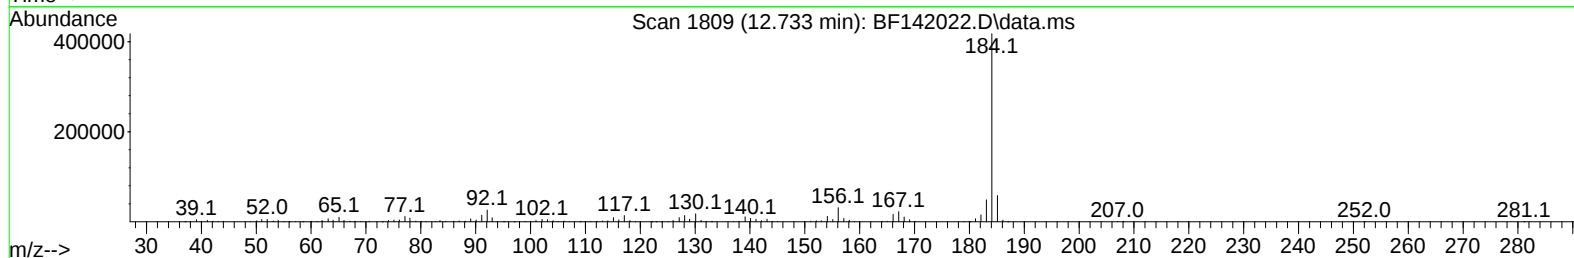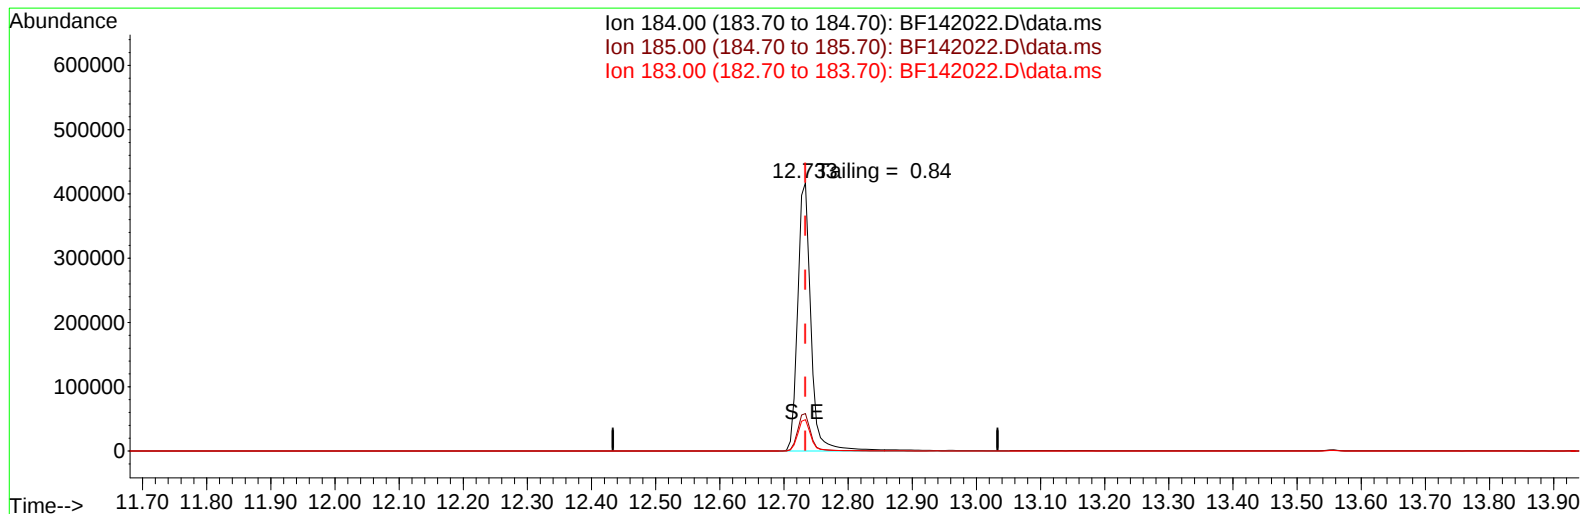

TIC: BF142022.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 26852.19 ng

response 603543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	12.10	11.72
0.00	0.00	0.00