
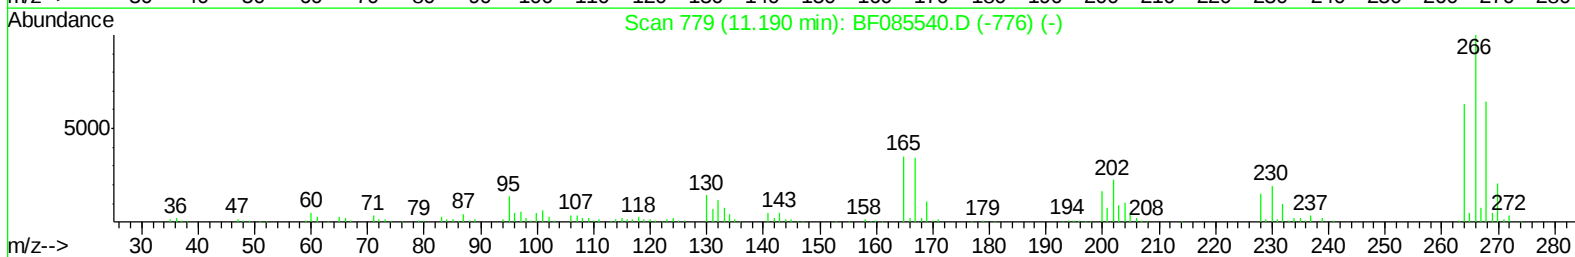
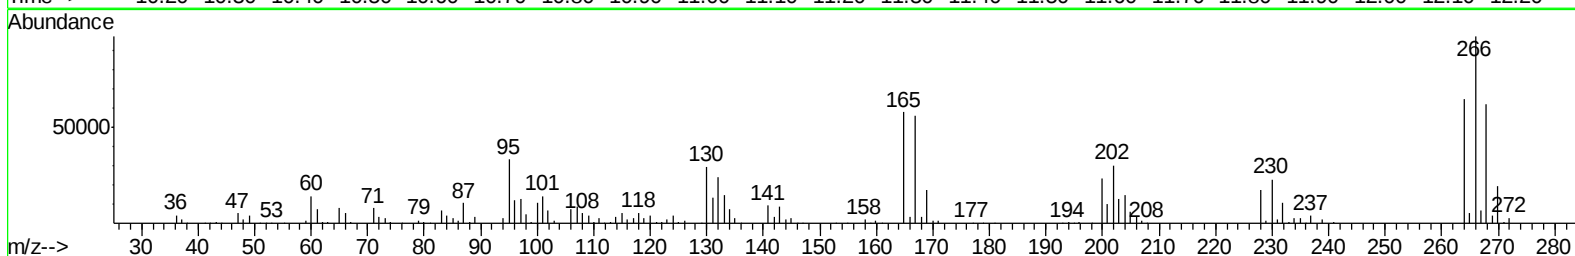


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:13:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

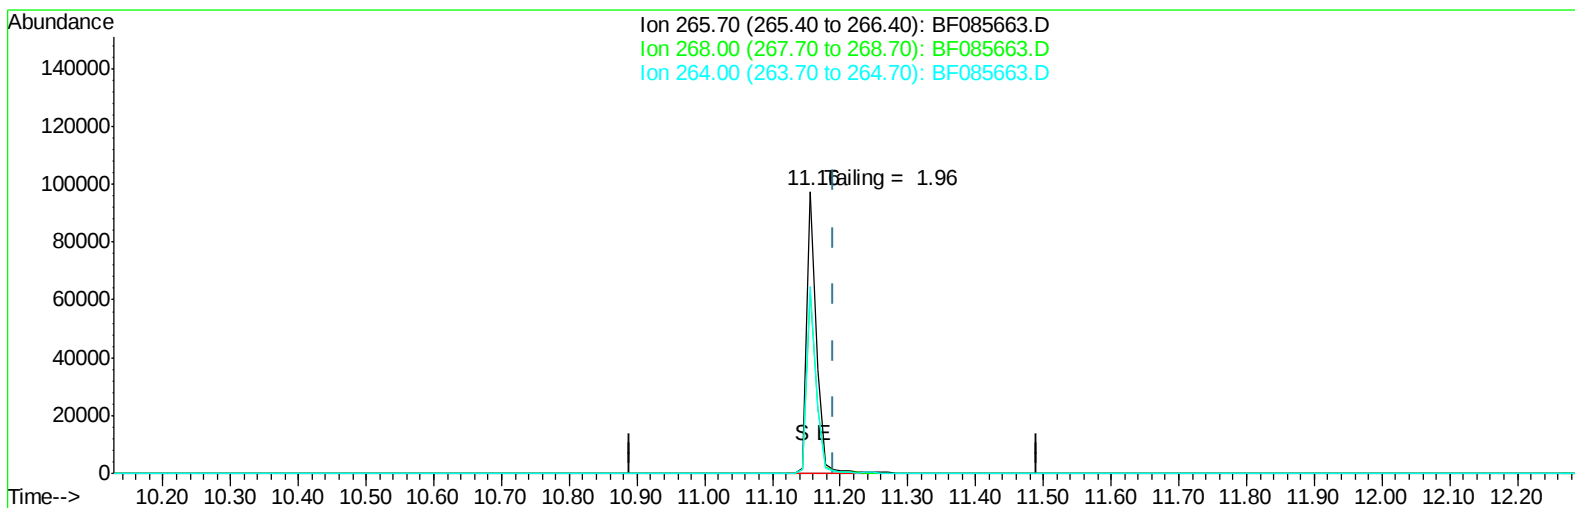

TIC: BF085663.D

(69) Pentachlorophenol (C)

11.156min (-0.034) 57113.51ng




response 98628

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.00
264.00	63.30	66.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:13:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

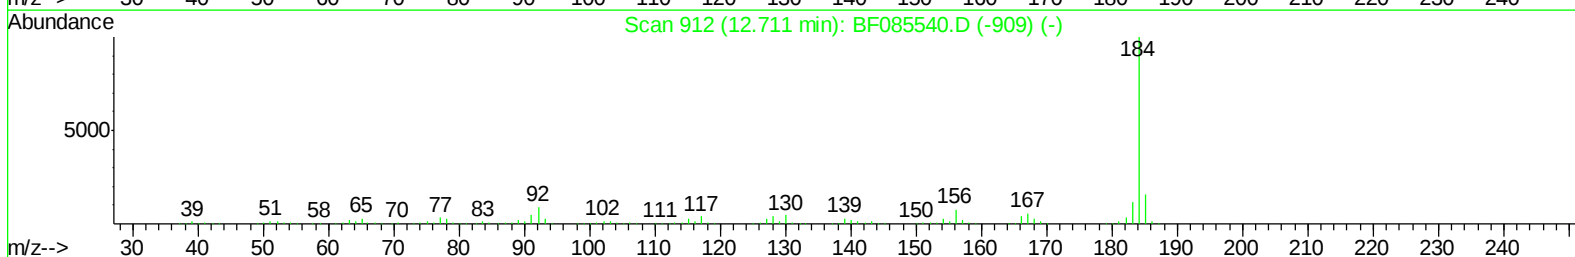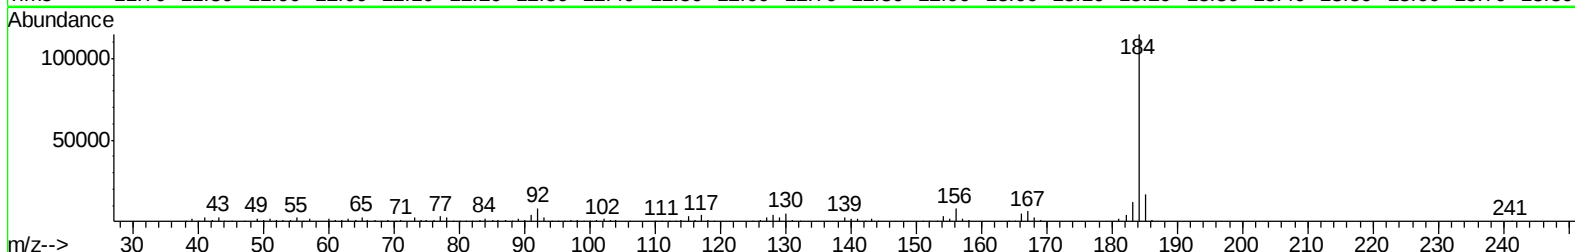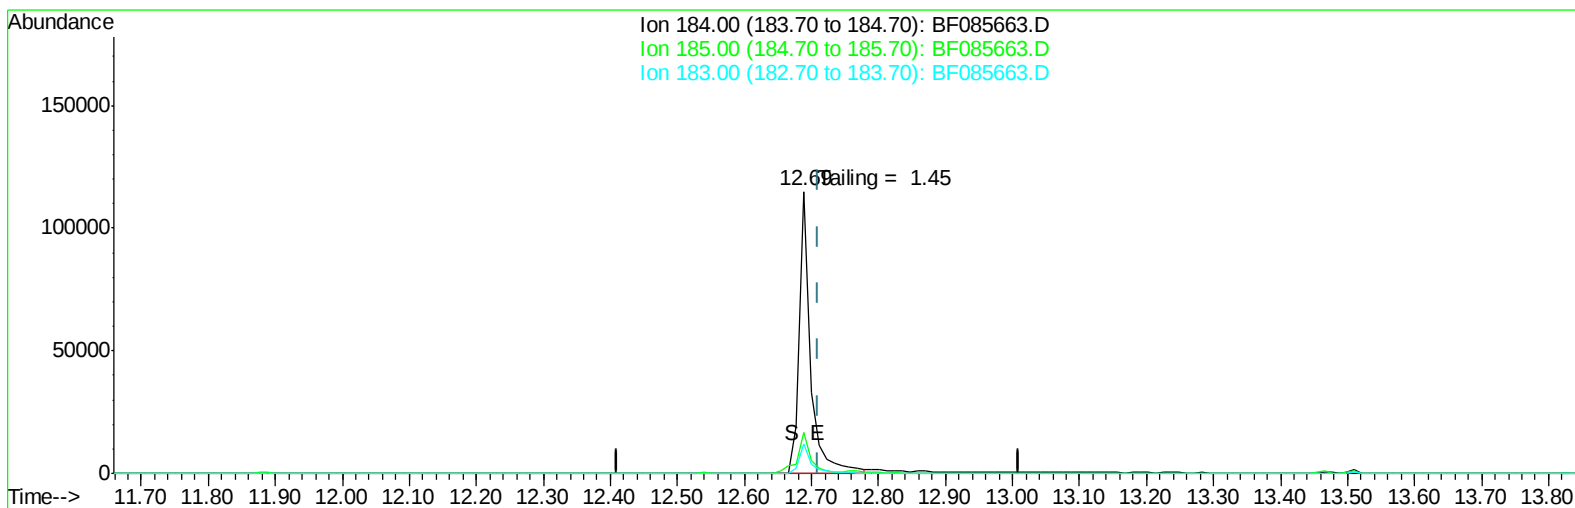

TIC: BF085663.D

(76) Benzidine

12.688min (-0.023) 16249.54ng




response 140437

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.80	10.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:13:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

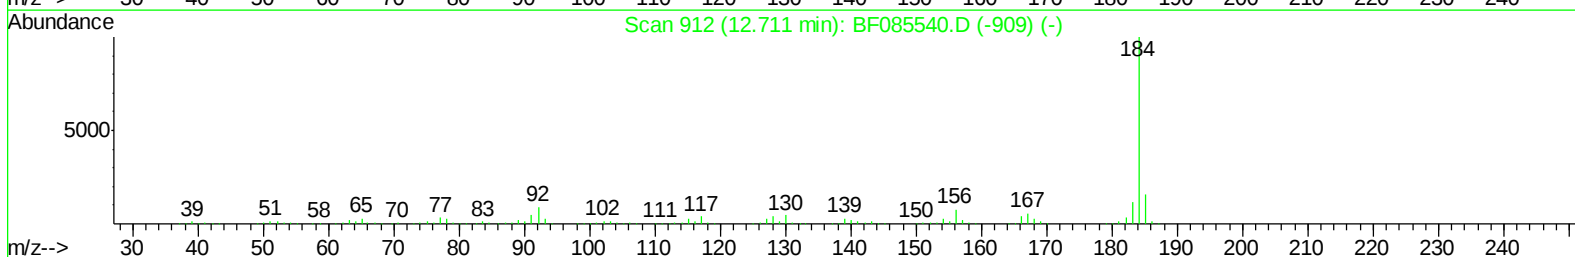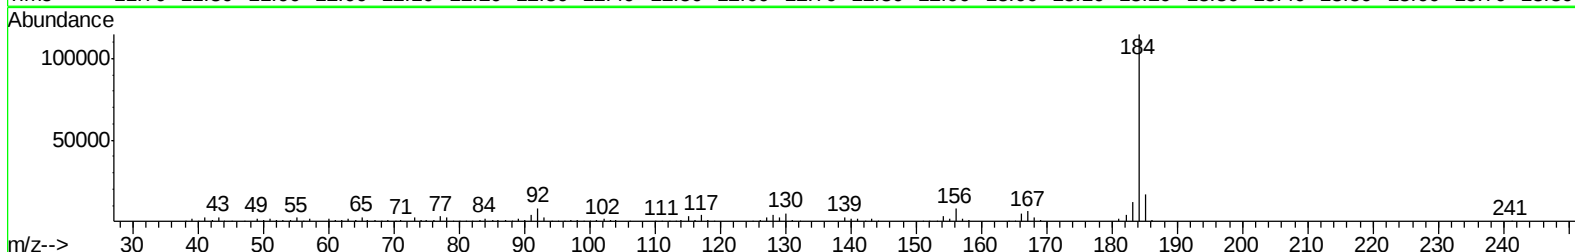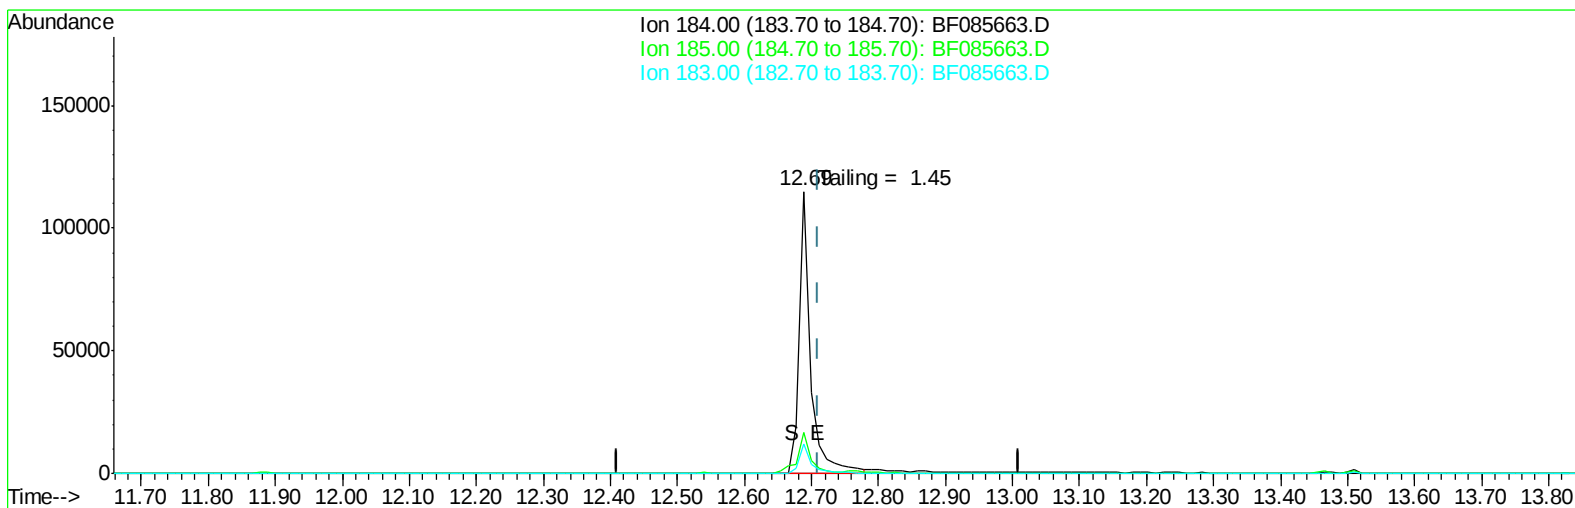

TIC: BF085663.D

(76) Benzidine

12.688min (-0.023) 16249.54ng




response 140437

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.80	10.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

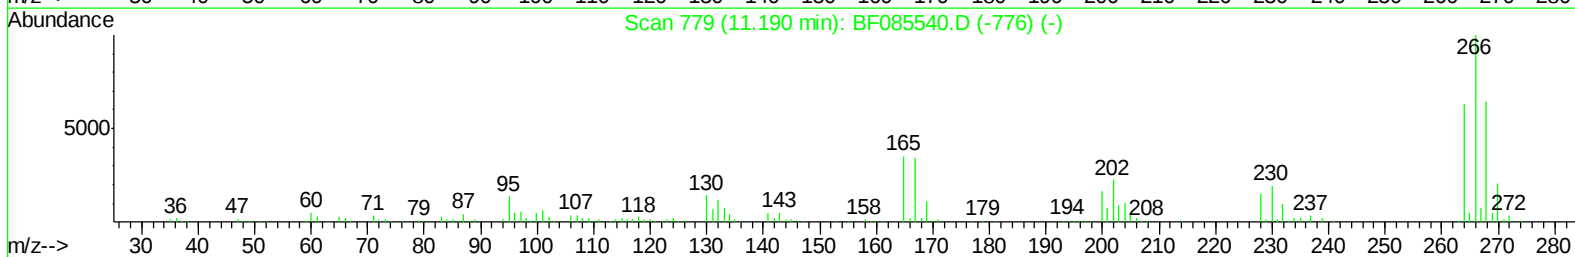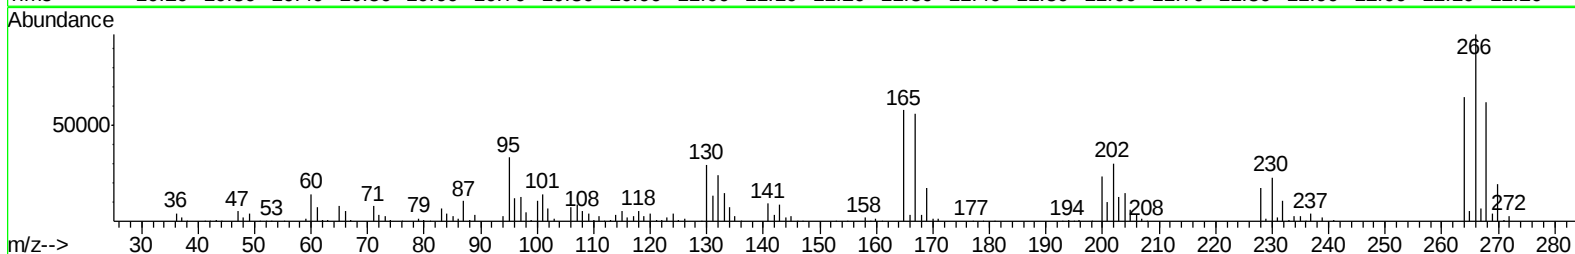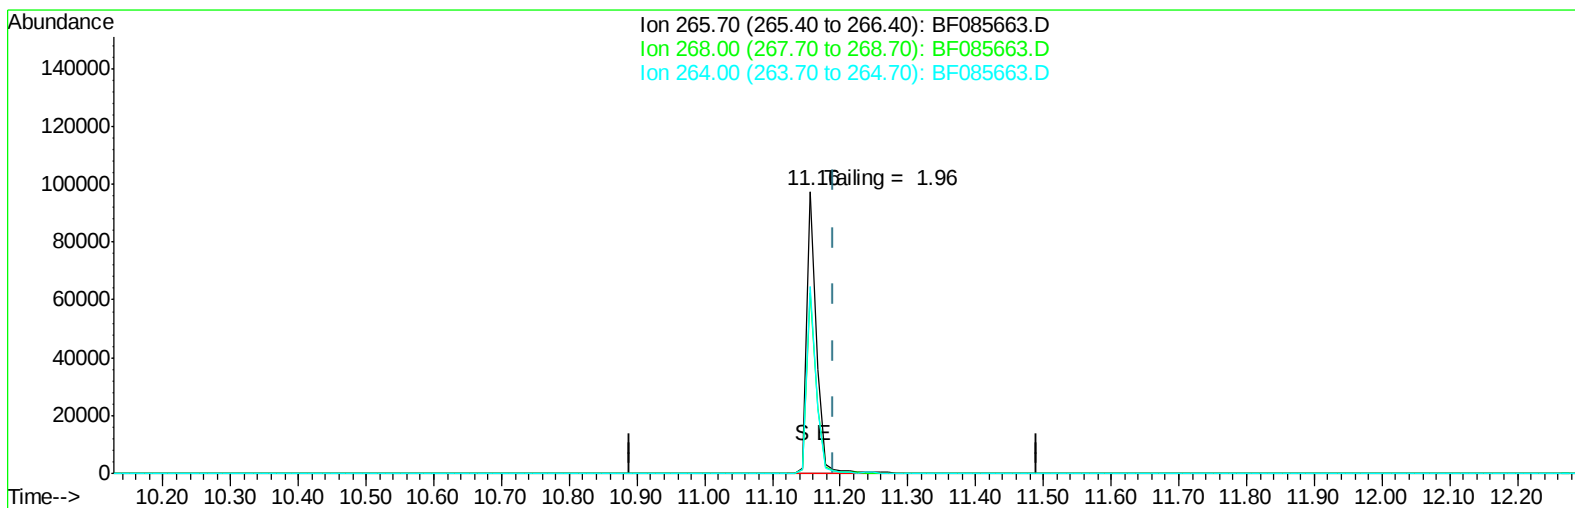

TIC: BF085663.D

(69) Pentachlorophenol (C)

11.156min (-0.034) 57113.51ng m




response 98628

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.00
264.00	63.30	66.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

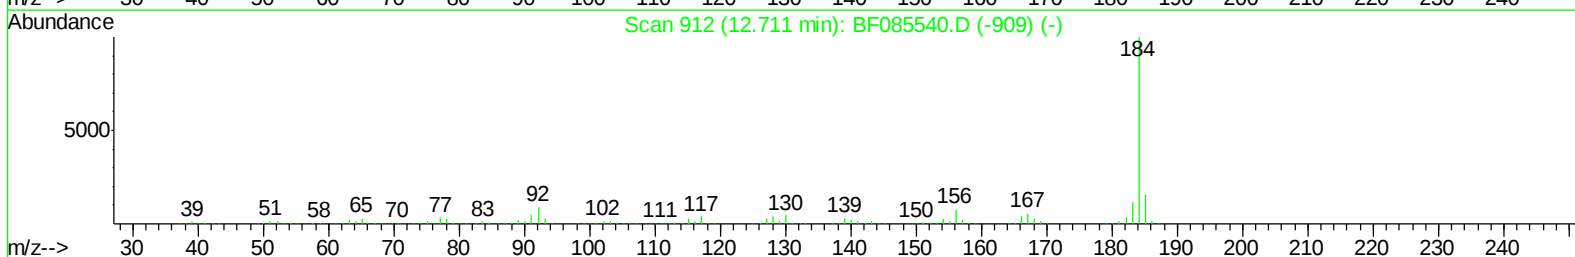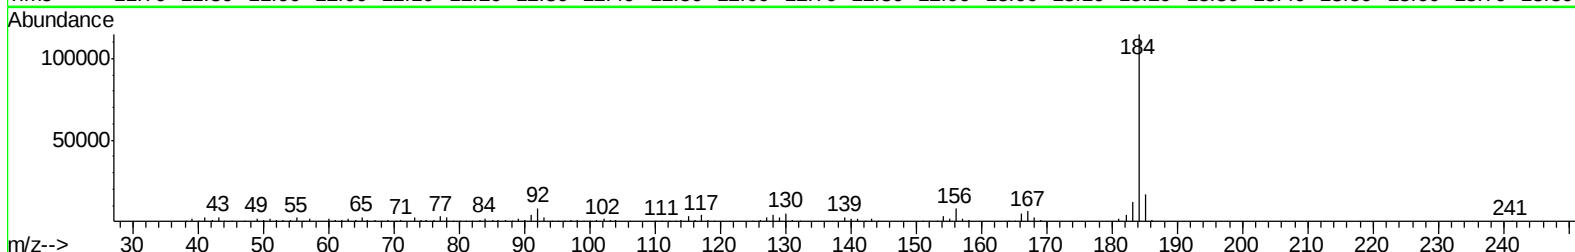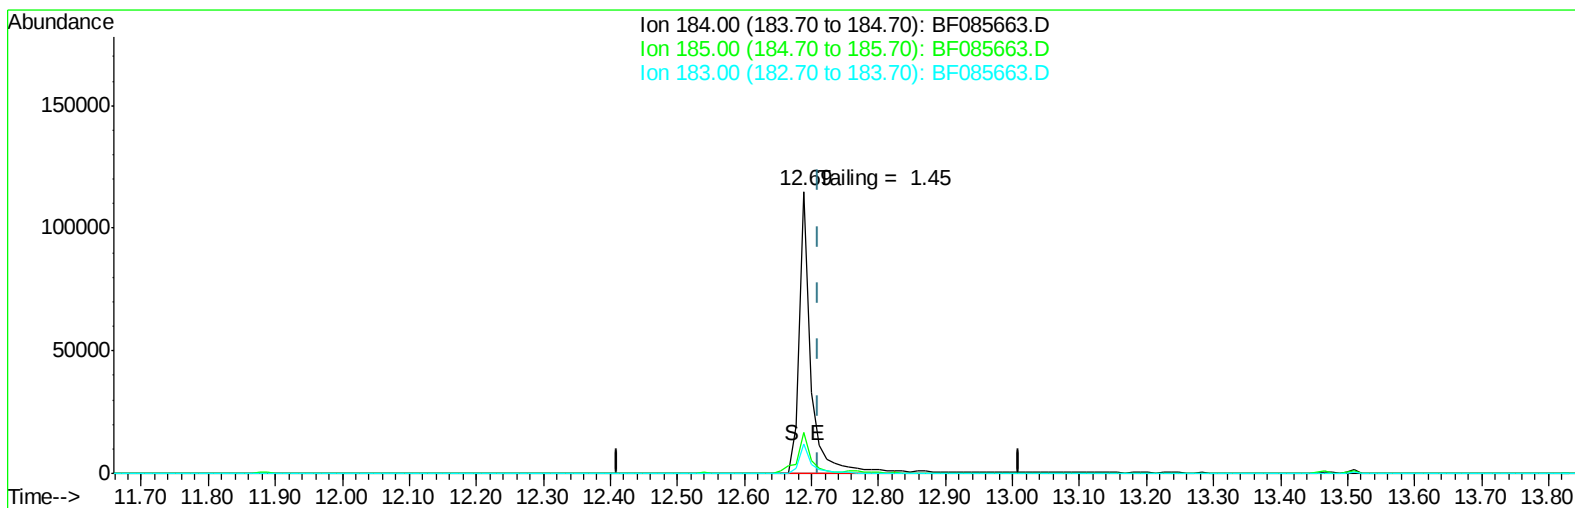

TIC: BF085663.D

(76) Benzidine

12.688min (-0.023) 16249.54ng




response 140437

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.80	10.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

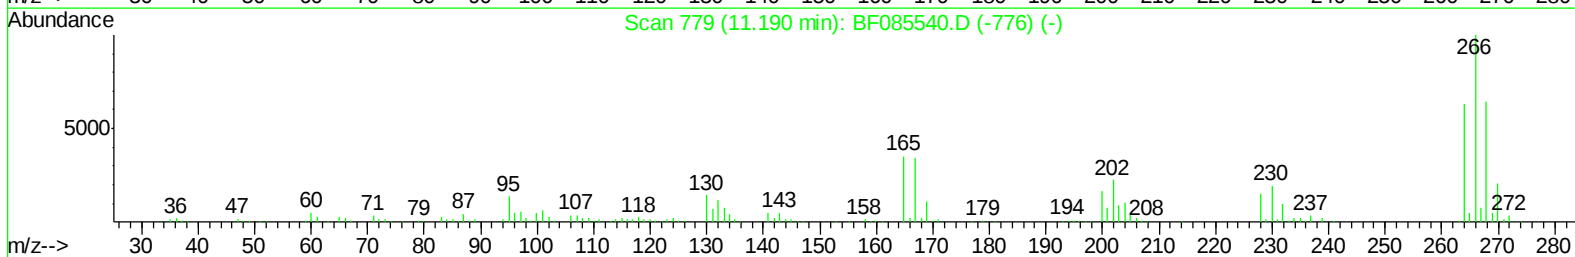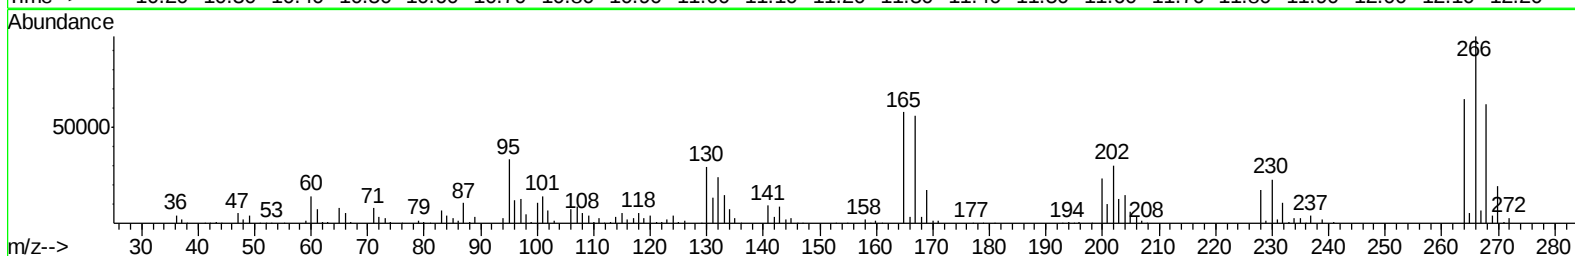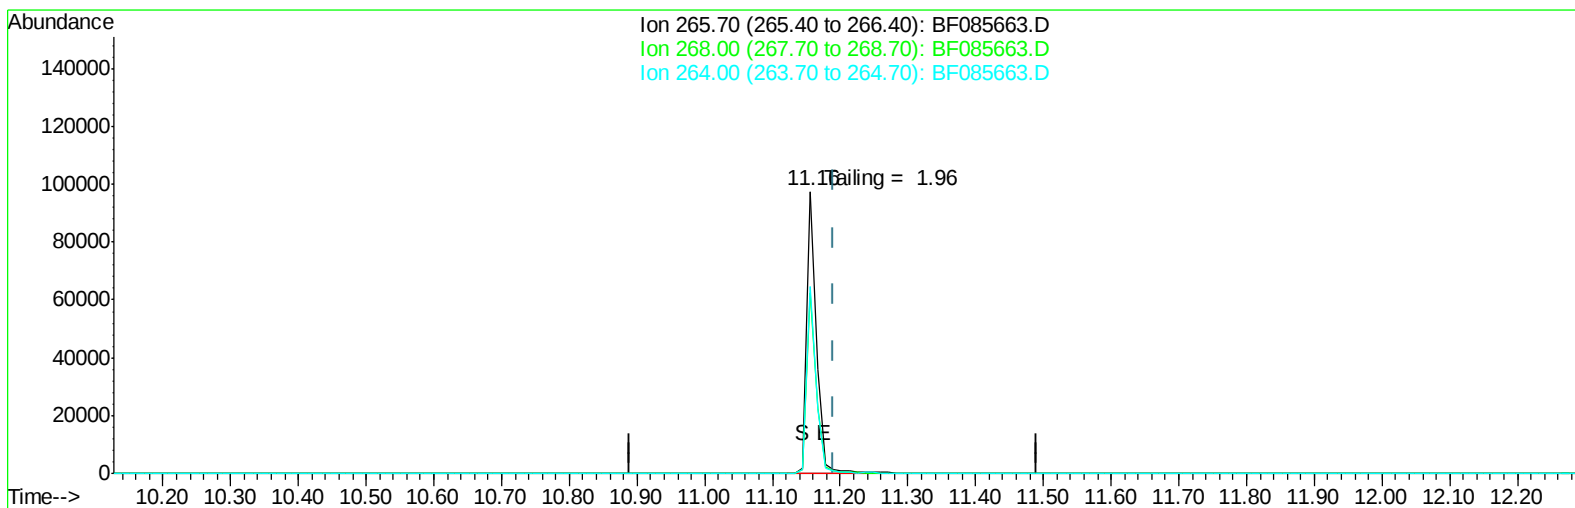

TIC: BF085663.D

(69) Pentachlorophenol (C)

11.156min (-0.034) 57113.51ng




response 98628

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.00
264.00	63.30	66.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

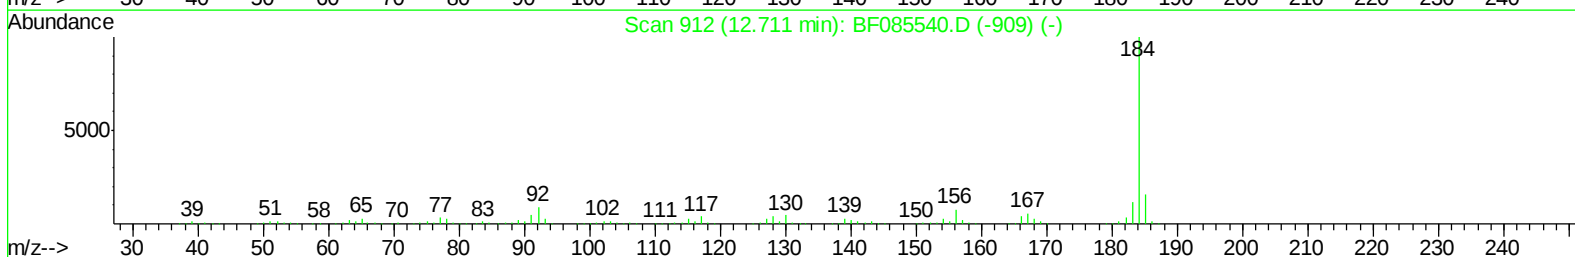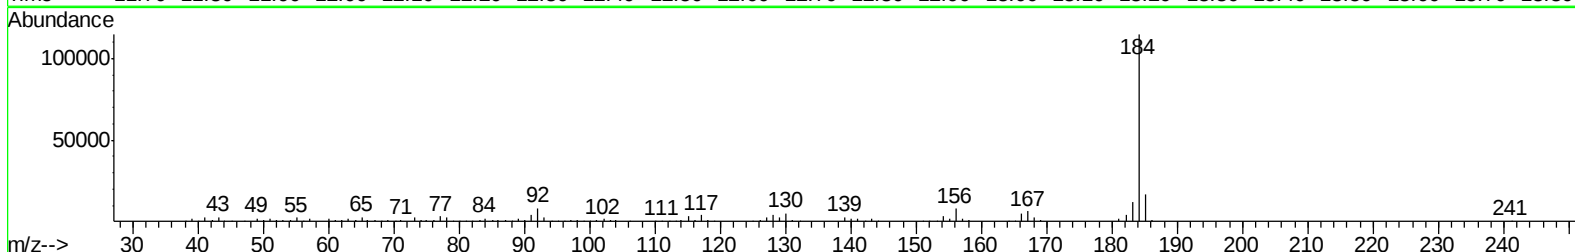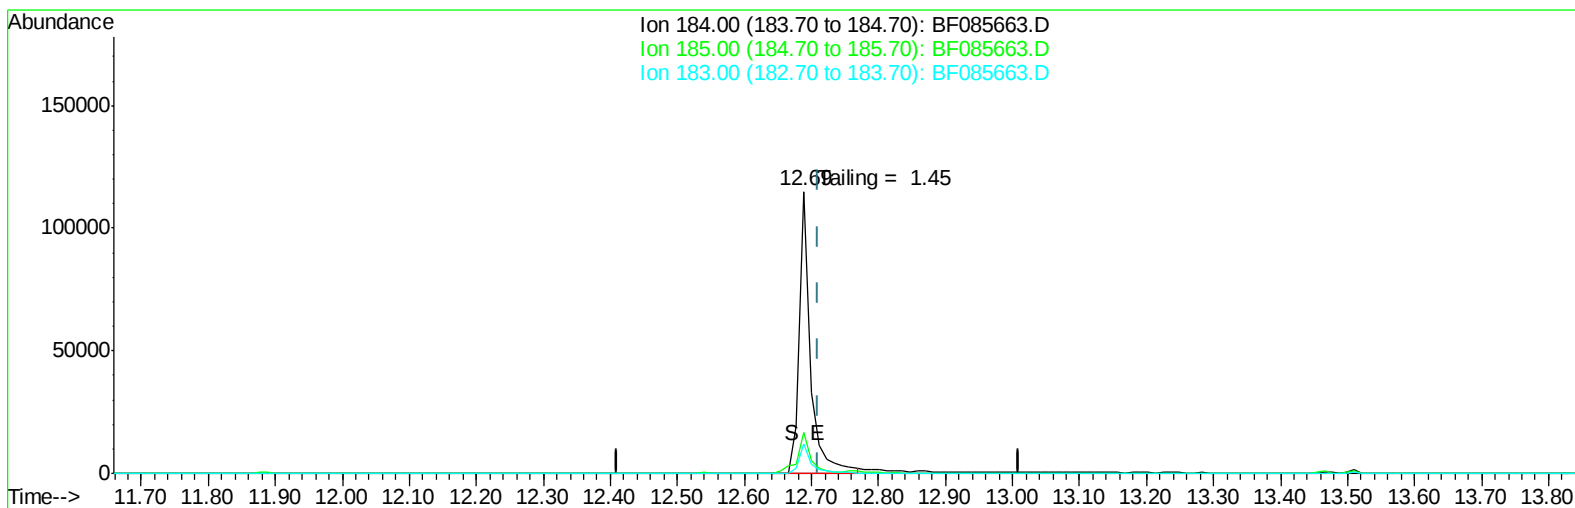

TIC: BF085663.D

(76) Benzidine

12.688min (-0.023) 16249.54ng




response 140437

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.80	10.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

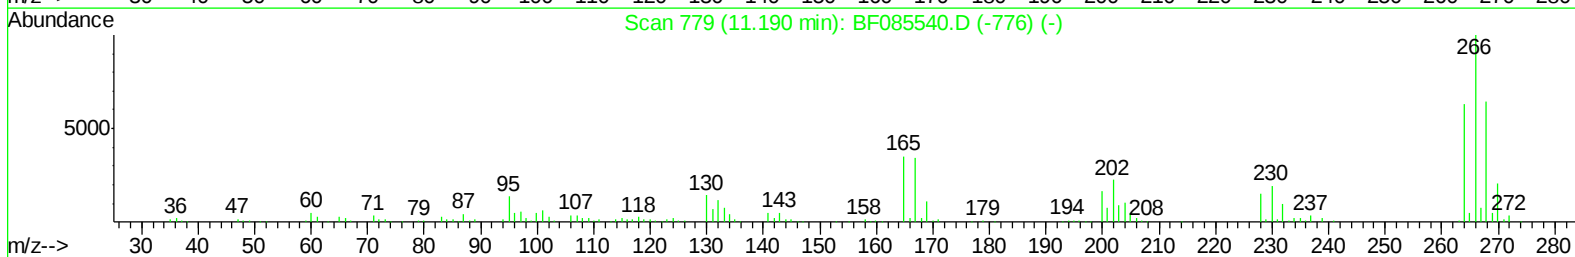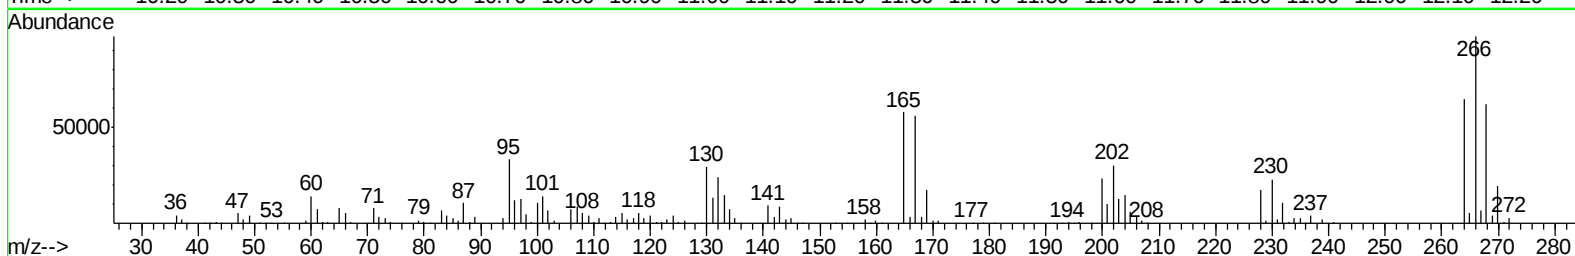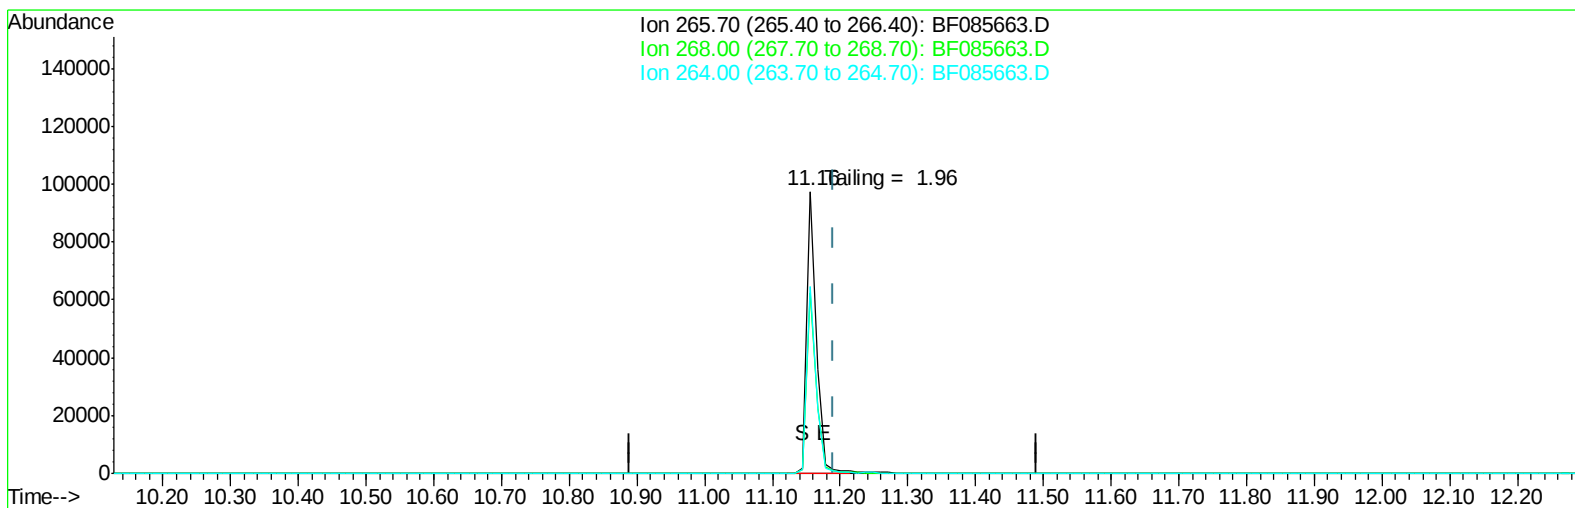

TIC: BF085663.D

(69) Pentachlorophenol (C)

11.156min (-0.034) 57113.51ng




response 98628

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.00
264.00	63.30	66.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

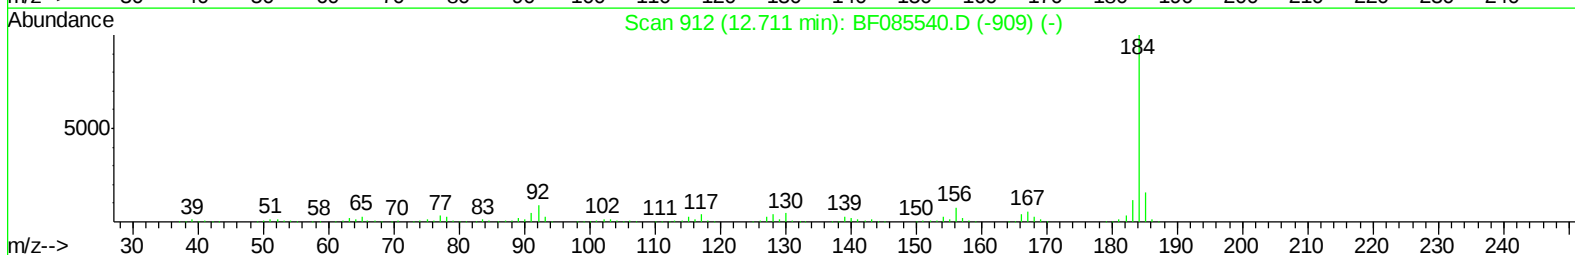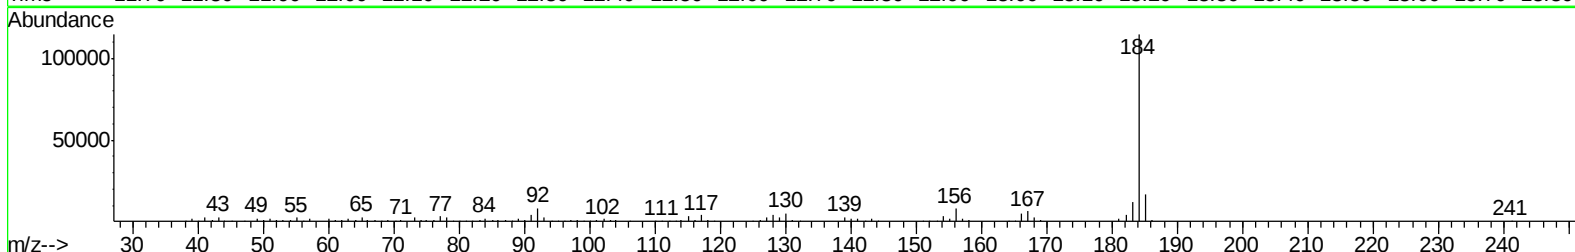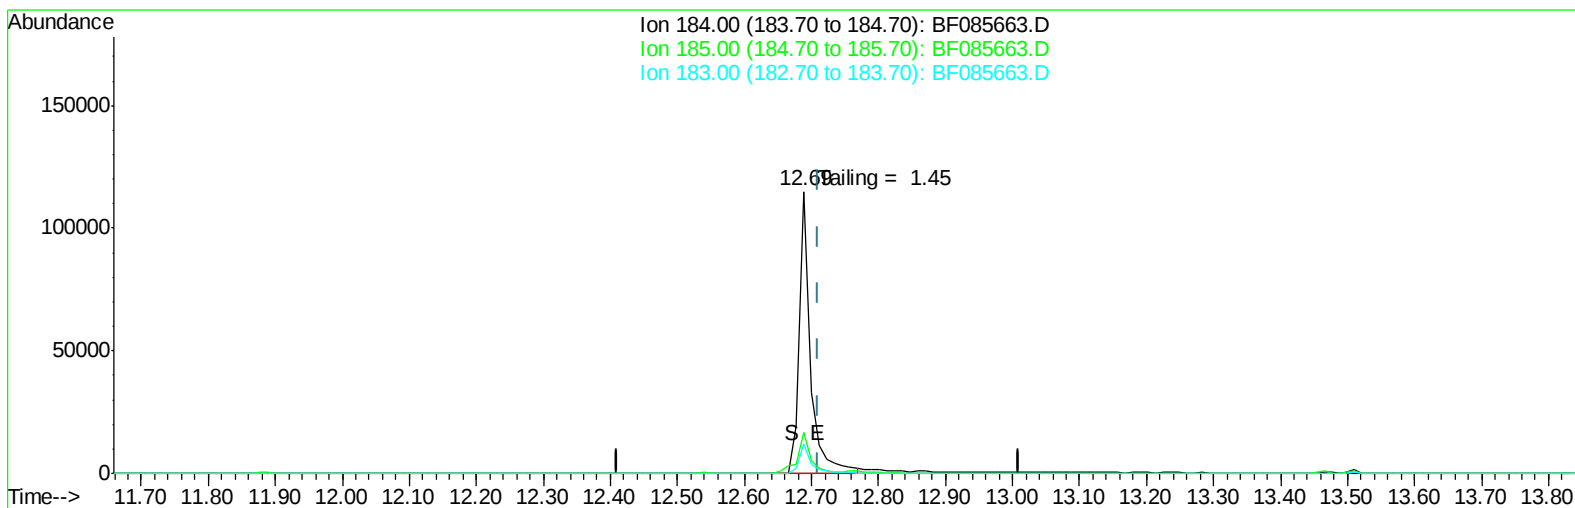

TIC: BF085663.D

(76) Benzidine

12.688min (-0.023) 16249.54ng




response 140437

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.80	10.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085663.D
Acq On : 22 Mar 2016 17:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 02:14:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

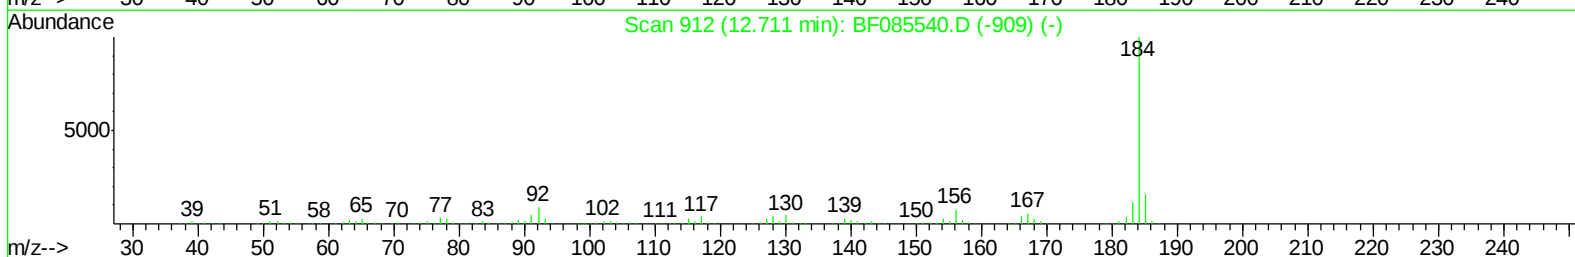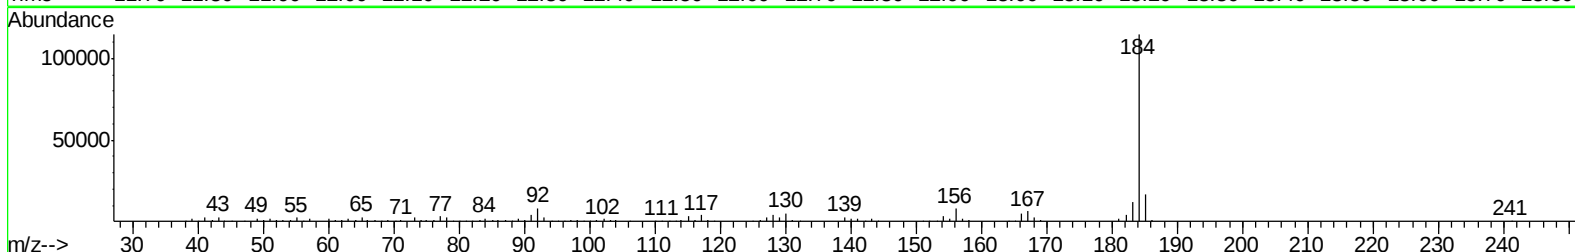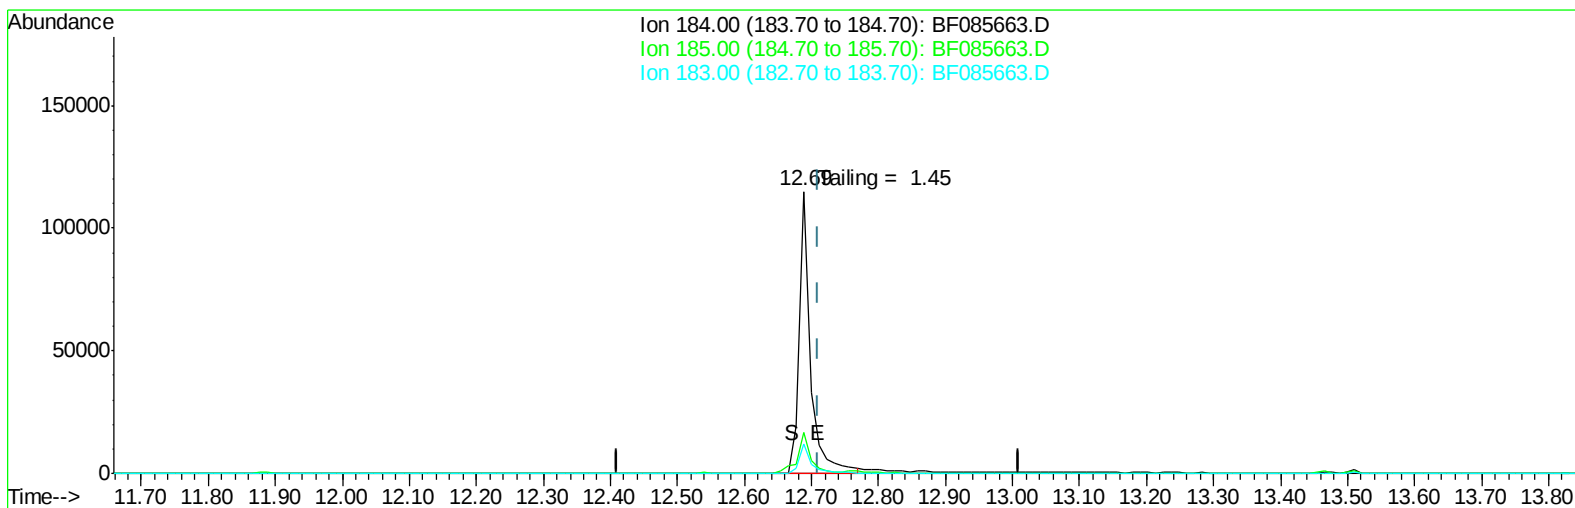

TIC: BF085663.D

(76) Benzidine

12.688min (-0.023) 16249.54ng

response 140437

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.35
183.00	11.80	10.68
0.00	0.00	0.00