
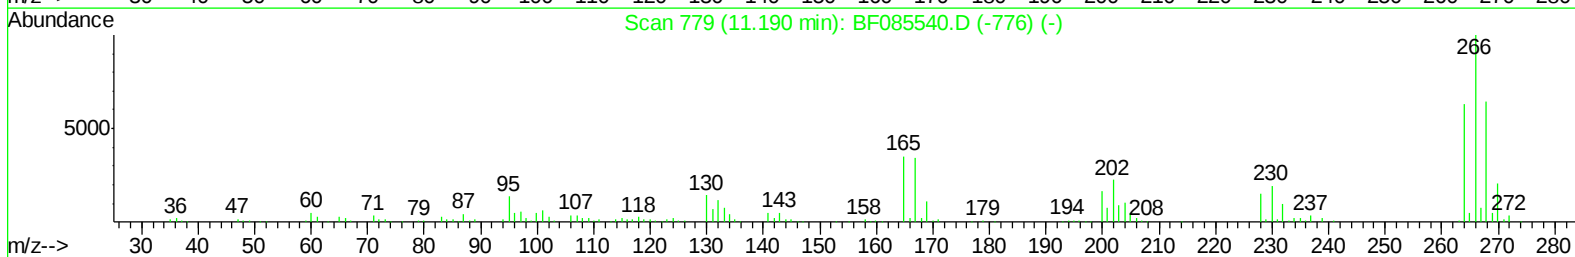
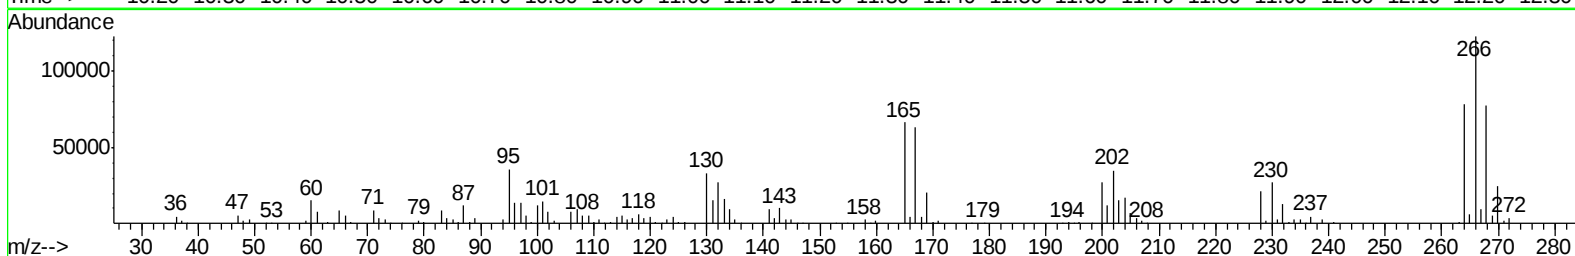


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085682.D
Acq On : 23 Mar 2016 2:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 02:30:54 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

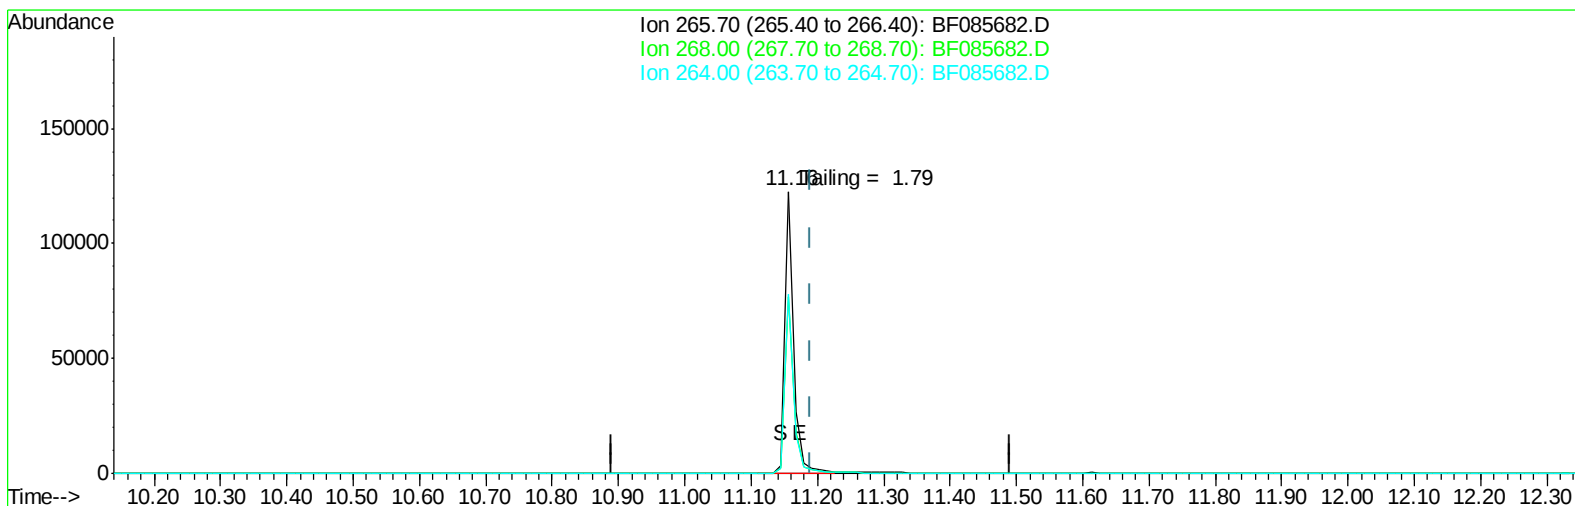

TIC: BF085682.D

(69) Pentachlorophenol (C)




11.156min (-0.034) 34873.58ng

response 114827

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.81
264.00	63.30	63.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
Data File : BF085682.D
Acq On : 23 Mar 2016 2:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 02:30:54 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

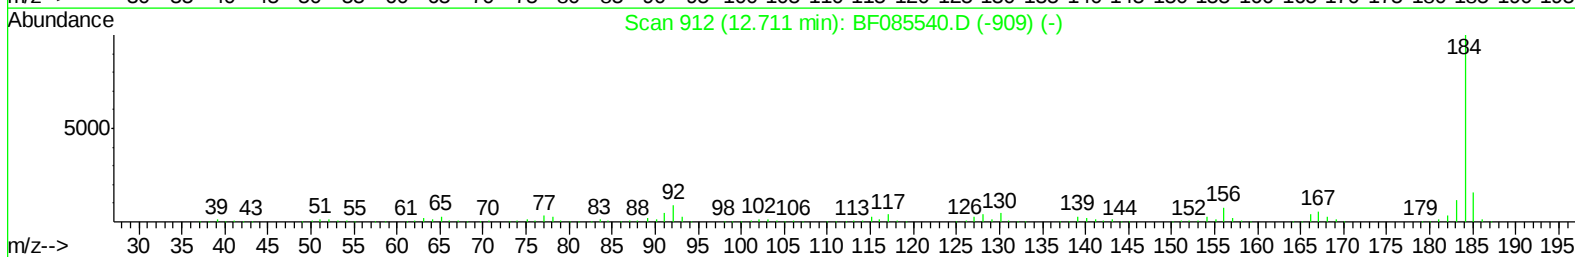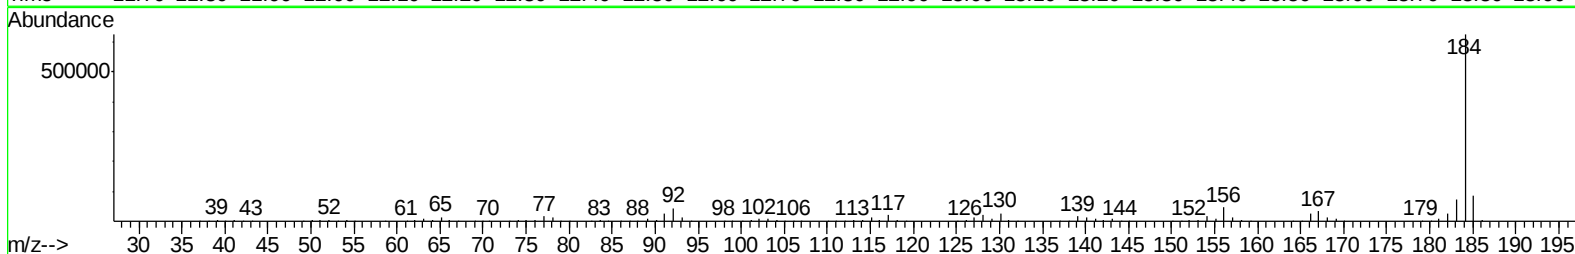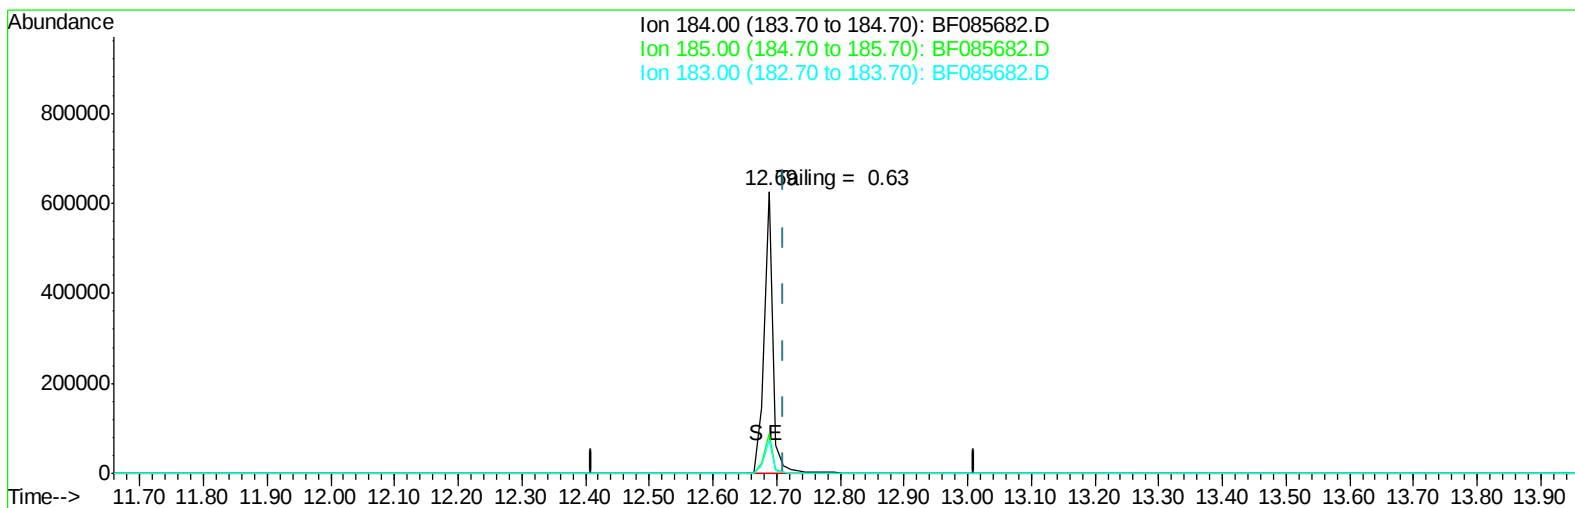

TIC: BF085682.D

(76) Benzidine

12.688min (-0.023) 0.00ng

response 609881

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.09
183.00	11.80	11.63
0.00	0.00	0.00