


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
 Data File : BF085663.D
 Acq On : 22 Mar 2016 17:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 18 23:31:39 2016

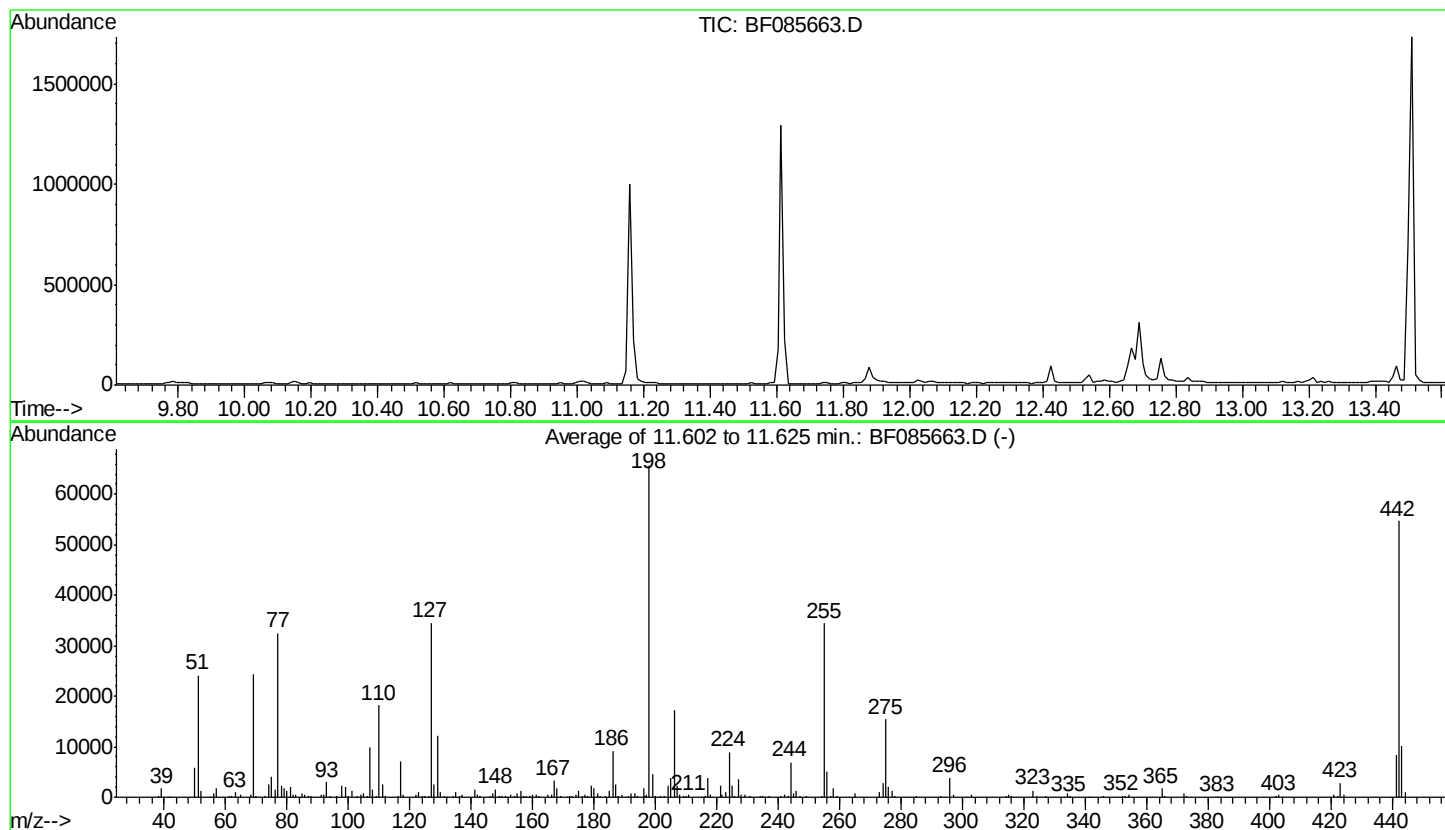

AutoFind: Scans 815, 816, 817; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	24175	PASS
68	69	0.00	2	1.9	451	PASS
69	198	0.00	100	37.0	24292	PASS
70	69	0.00	2	0.6	137	PASS
127	198	10	80	52.6	34562	PASS
197	198	0.00	2	0.6	419	PASS
198	198	100	100	100.0	65662	PASS
199	198	5	9	7.0	4576	PASS
275	198	10	60	23.5	15414	PASS
365	198	1	100	2.6	1732	PASS
441	442	0.01	24	15.4	8428	PASS
442	198	50	100	83.3	54725	PASS
443	442	15	24	18.4	10089	PASS