


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032216\
 Data File : BF085682.D
 Acq On : 23 Mar 2016 2:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 18 23:31:39 2016

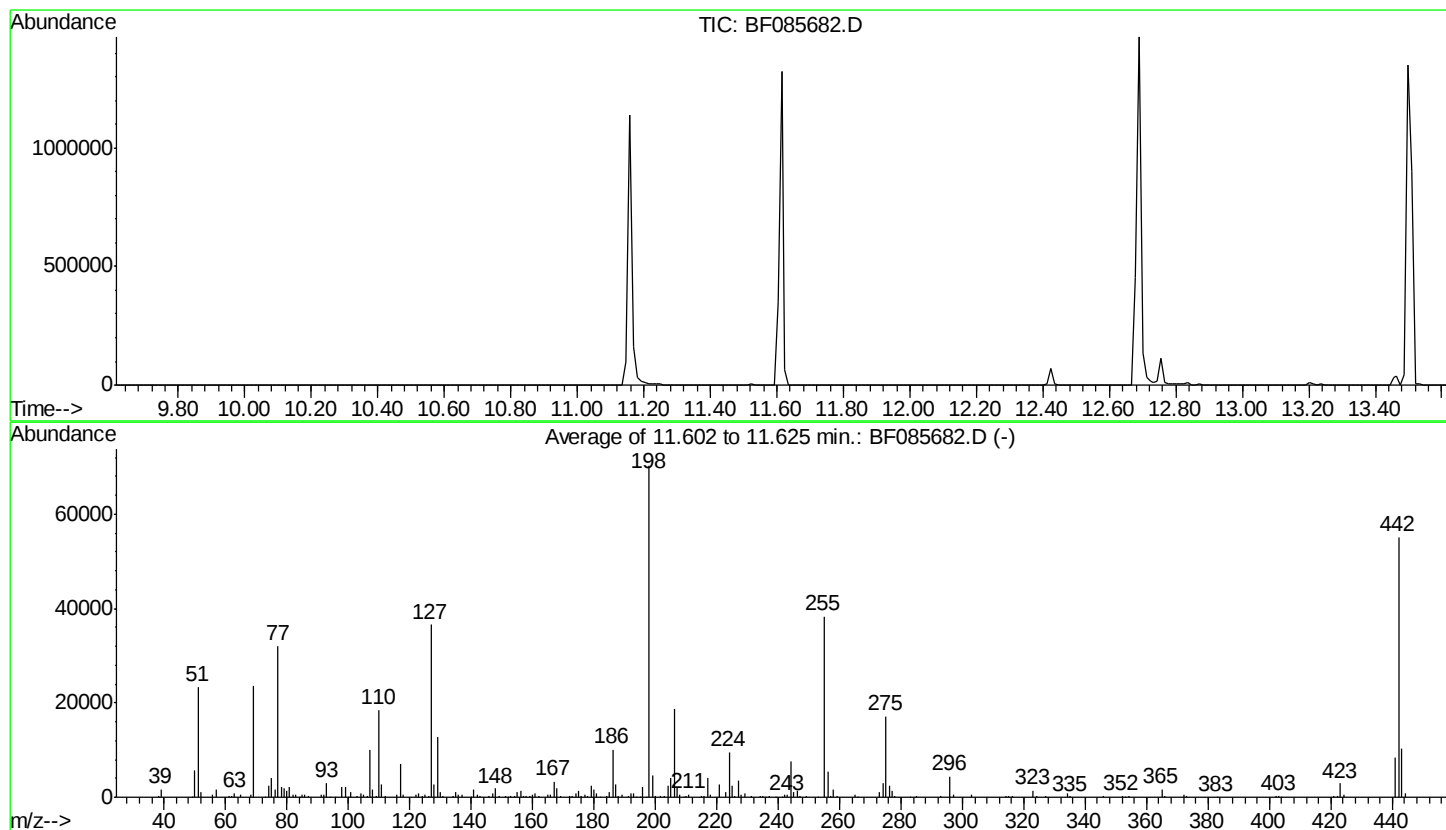

AutoFind: Scans 815, 816, 817; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	23407	PASS
68	69	0.00	2	1.8	432	PASS
69	198	0.00	100	33.8	23719	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	36538	PASS
197	198	0.00	2	0.2	106	PASS
198	198	100	100	100.0	70255	PASS
199	198	5	9	6.4	4521	PASS
275	198	10	60	24.5	17178	PASS
365	198	1	100	2.4	1696	PASS
441	442	0.01	24	15.4	8465	PASS
442	198	50	100	78.4	55059	PASS
443	442	15	24	18.9	10390	PASS