
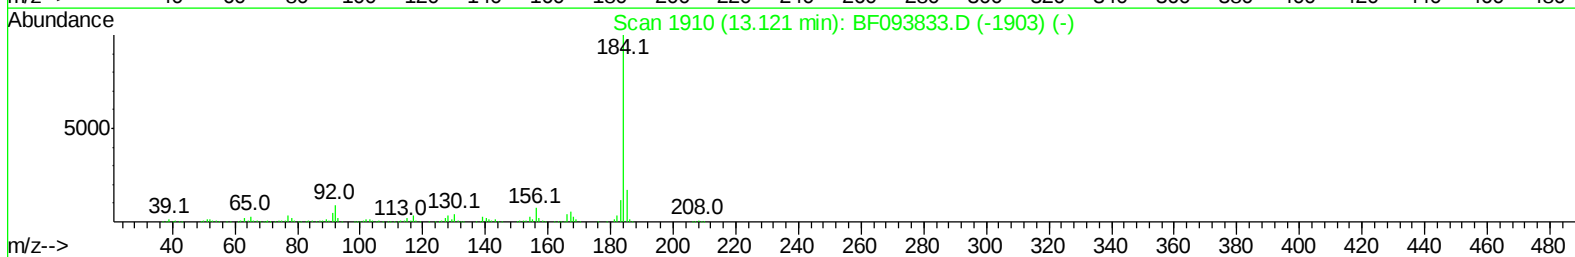
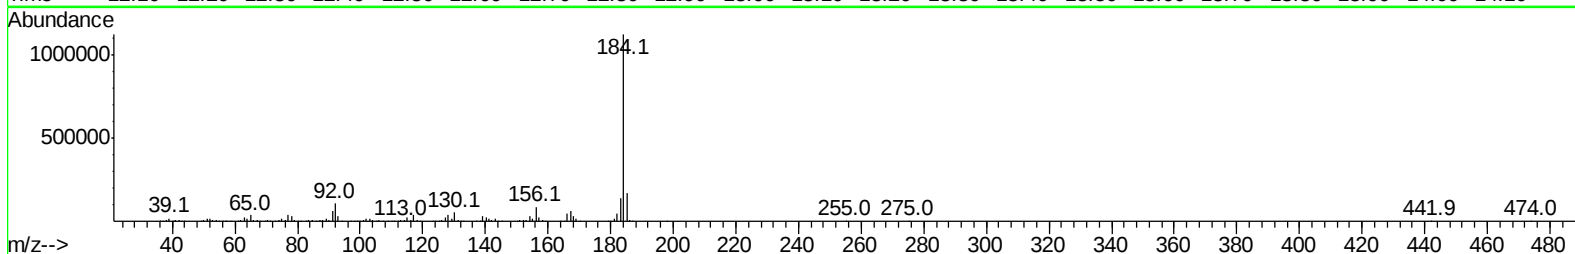


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032217\
Data File : BF093829.D
Acq On : 22 Mar 2017 13:50
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:14:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

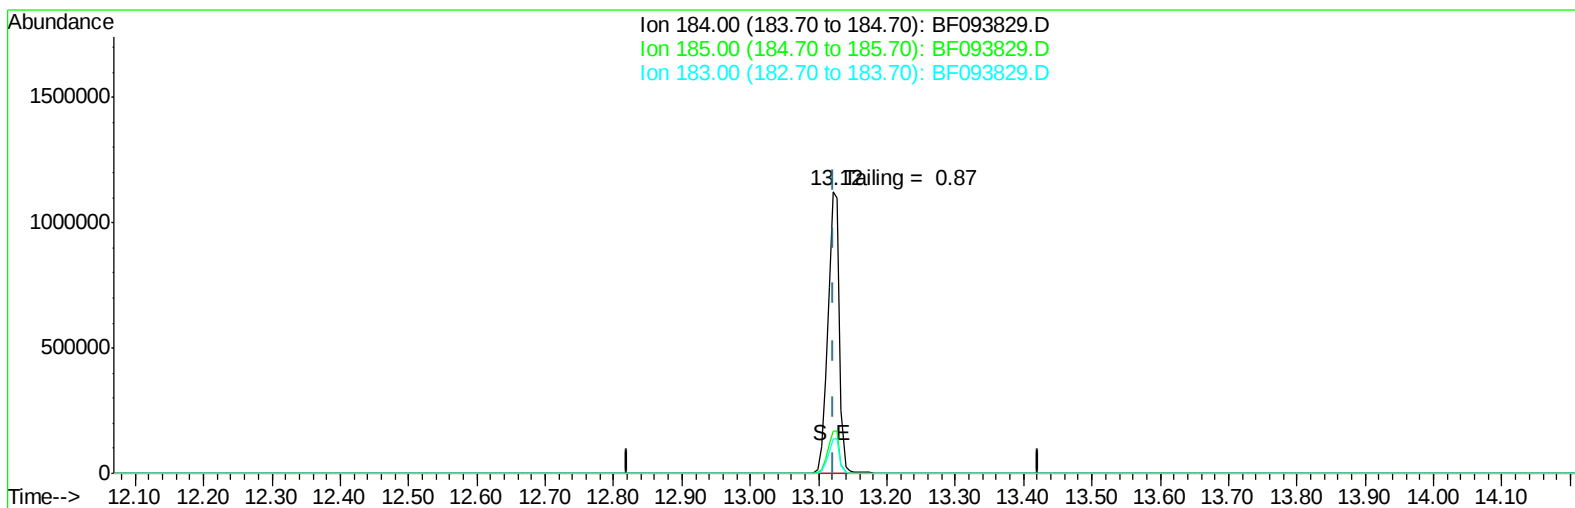

TIC: BF093829.D

(76) Benzidine




13.121min (+0.000) 0.00ng

response 1333848

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.93#
183.00	12.20	12.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032217\
Data File : BF093829.D
Acq On : 22 Mar 2017 13:50
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:14:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

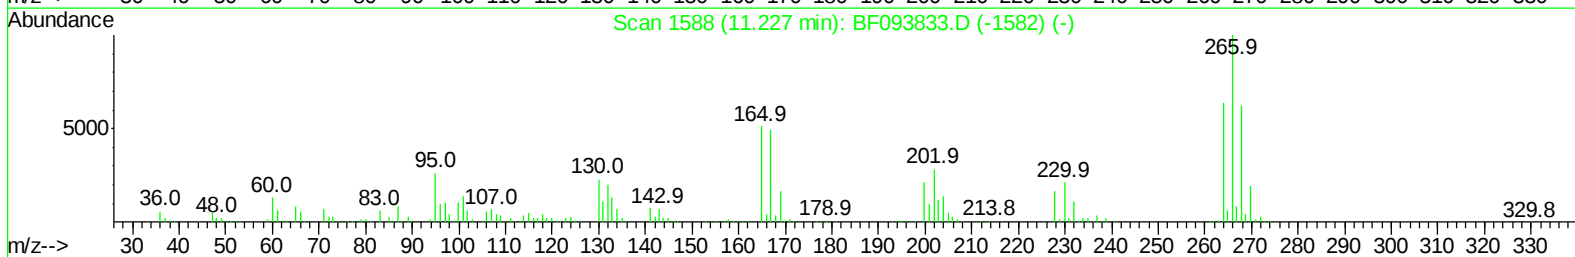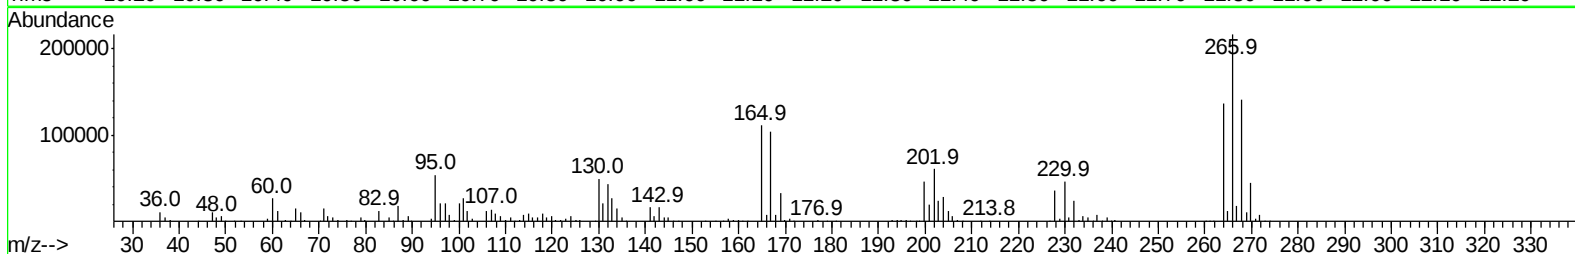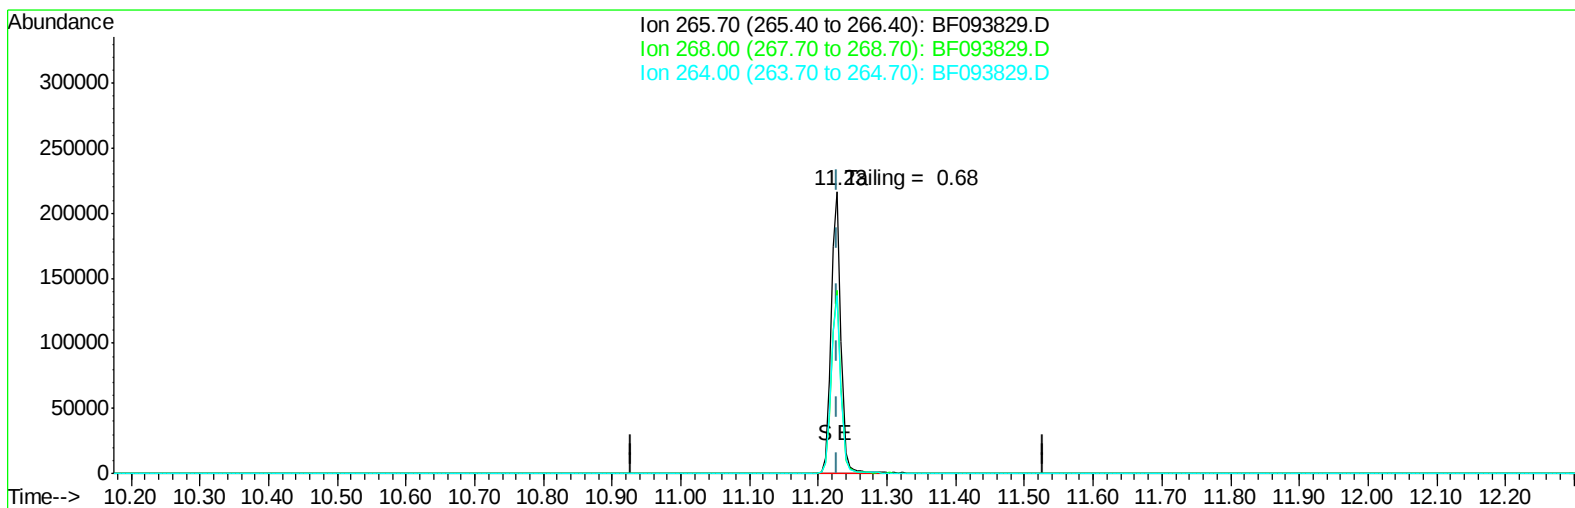

TIC: BF093829.D

(69) Pentachlorophenol (C)

11.227min (+0.000) 0.00ng

response 216092

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.10
264.00	64.60	63.32
0.00	0.00	0.00