
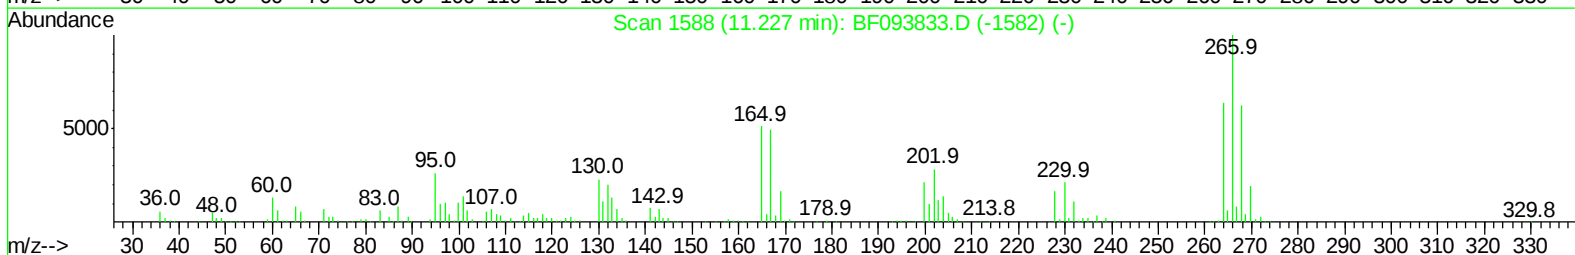
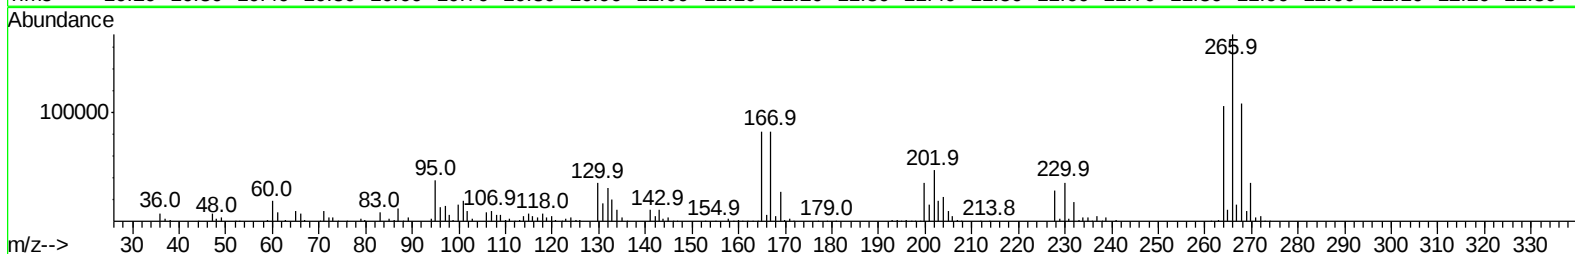


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032217\
Data File : BF093851.D
Acq On : 23 Mar 2017 00:23
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:17:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

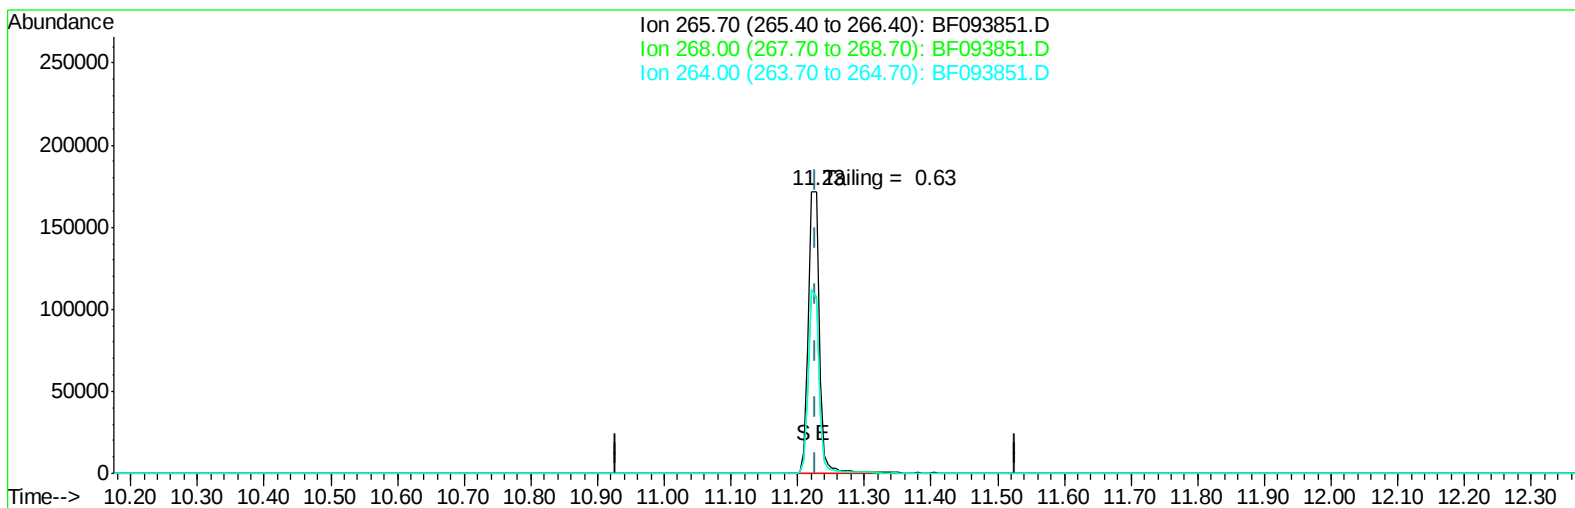

TIC: BF093851.D

(69) Pentachlorophenol (C)




11.227min (+0.000) 0.00ng

response 185840

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.91
264.00	64.60	61.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032217\
Data File : BF093851.D
Acq On : 23 Mar 2017 00:23
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:17:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

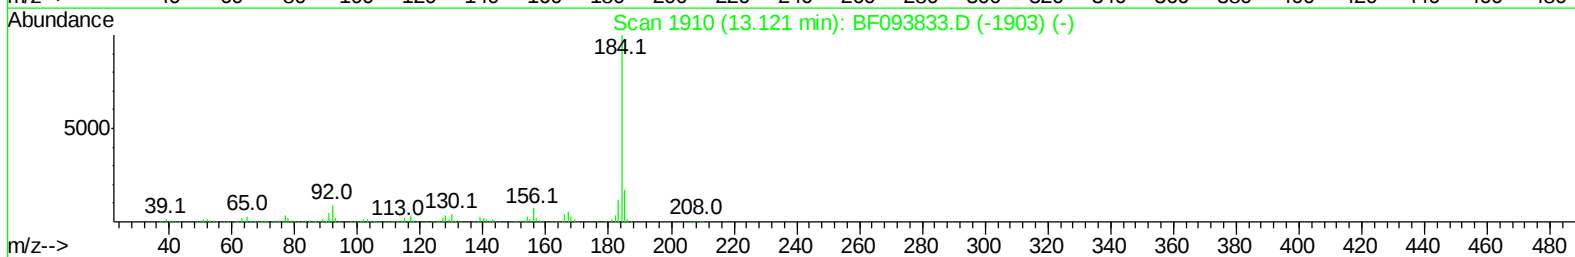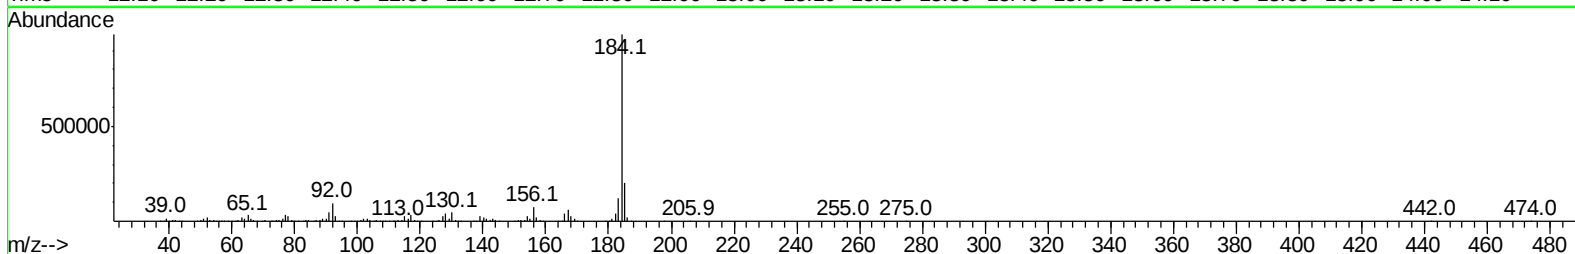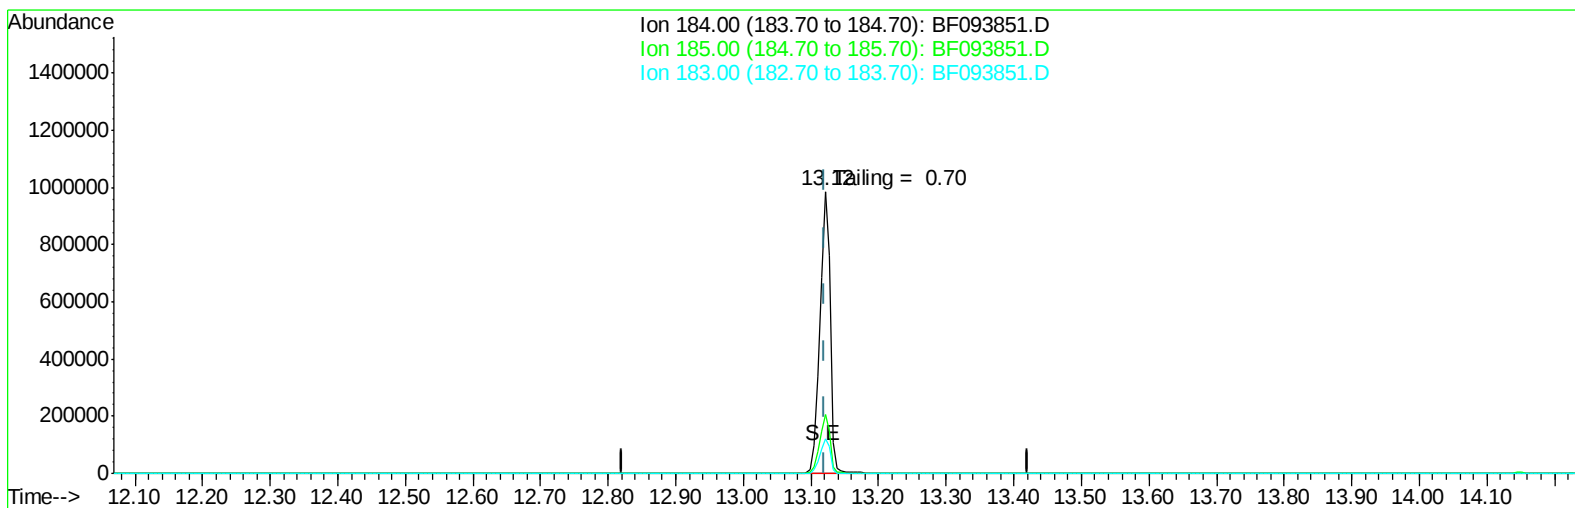

TIC: BF093851.D

(76) Benzidine

13.121min (+0.000) 0.00ng

response 1079166

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	20.78
183.00	12.20	12.40
0.00	0.00	0.00