


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032217\
 Data File : BF093829.D
 Acq On : 22 Mar 2017 13:50
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 23 02:02:22 2017

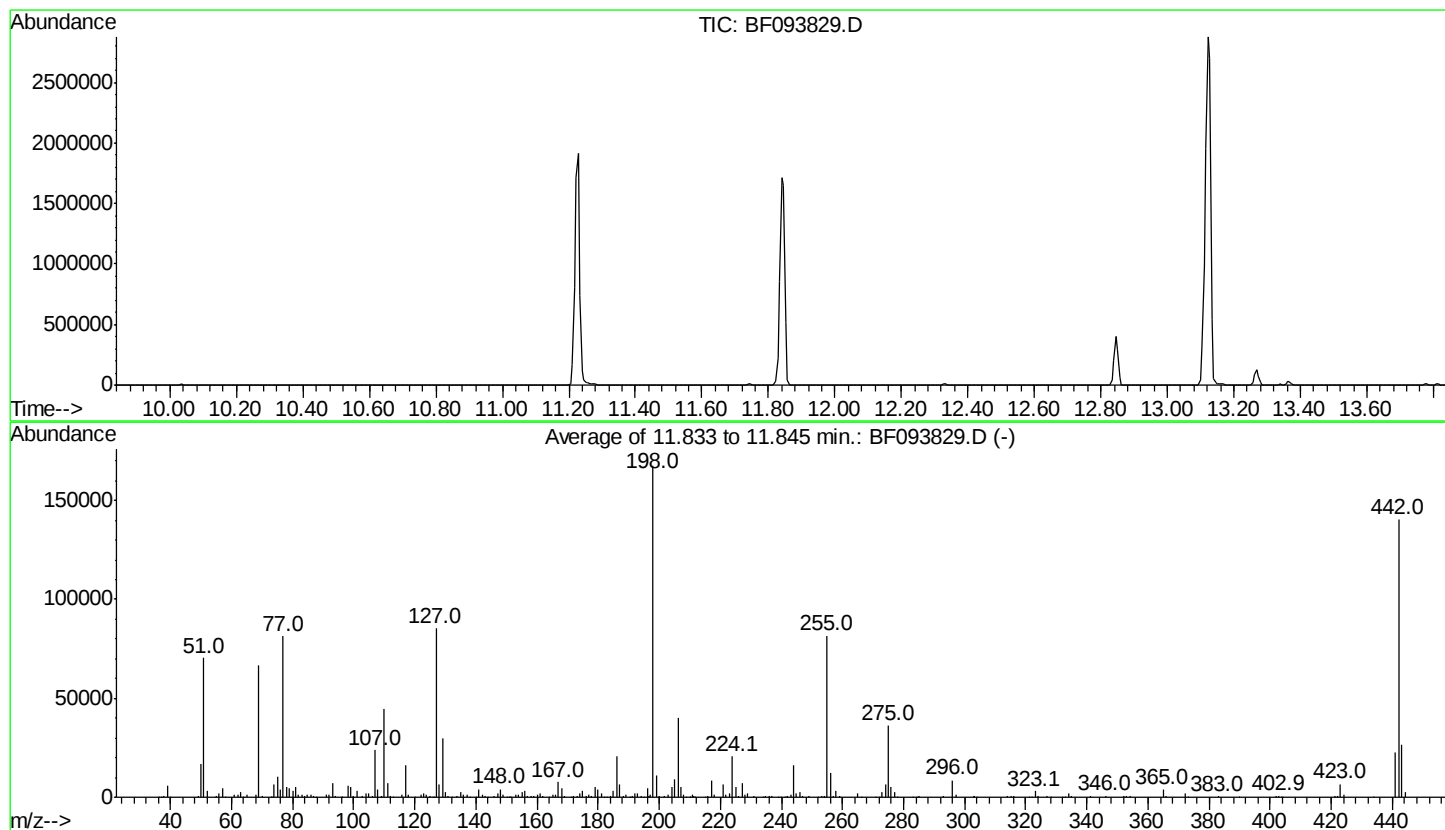

AutoFind: Scans 1691, 1692, 1693; Background Corrected with Scan 1685

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	70434	PASS
68	69	0.00	2	1.6	1045	PASS
69	198	0.00	100	39.6	66386	PASS
70	69	0.00	2	0.6	430	PASS
127	198	10	80	50.8	85173	PASS
197	198	0.00	2	0.8	1273	PASS
198	198	100	100	100.0	167584	PASS
199	198	5	9	6.7	11261	PASS
275	198	10	60	21.5	36024	PASS
365	198	1	100	2.3	3791	PASS
441	442	0.01	24	16.0	22443	PASS
442	198	50	100	83.7	140189	PASS
443	442	15	24	18.8	26399	PASS