


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032217\
 Data File : BF093851.D
 Acq On : 23 Mar 2017 00:23
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 23 02:02:22 2017

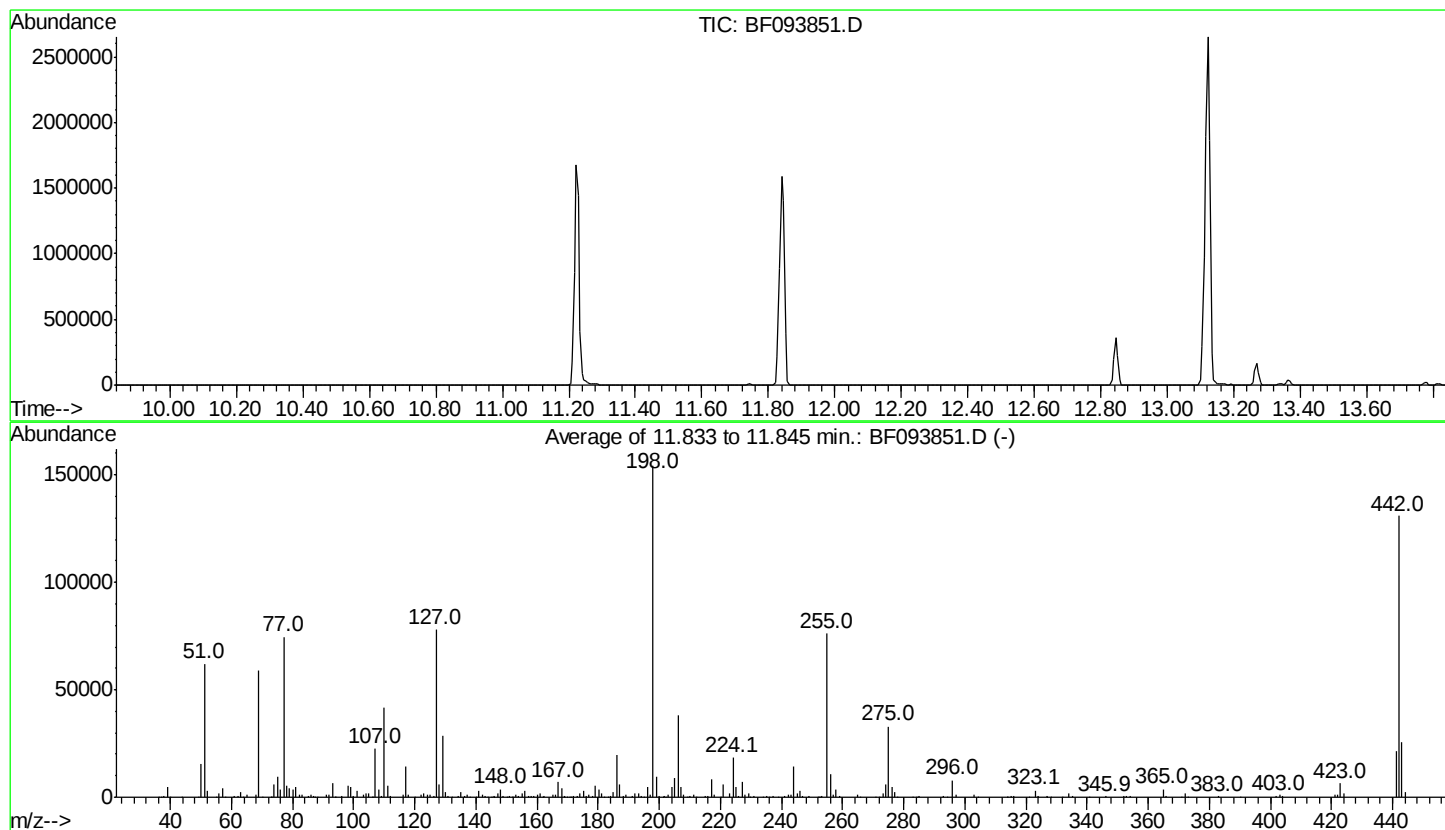

AutoFind: Scans 1691, 1692, 1693; Background Corrected with Scan 1686

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	62168	PASS
68	69	0.00	2	1.9	1104	PASS
69	198	0.00	100	38.1	58776	PASS
70	69	0.00	2	0.5	283	PASS
127	198	10	80	50.5	77984	PASS
197	198	0.00	2	0.8	1242	PASS
198	198	100	100	100.0	154298	PASS
199	198	5	9	6.3	9704	PASS
275	198	10	60	21.3	32840	PASS
365	198	1	100	2.4	3653	PASS
441	442	0.01	24	16.5	21538	PASS
442	198	50	100	84.8	130778	PASS
443	442	15	24	19.8	25901	PASS