


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_F\Data\BF032218\
 Data File : BF103839.D
 Acq On : 22 Mar 2018 9:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 22 11:56:49 2018

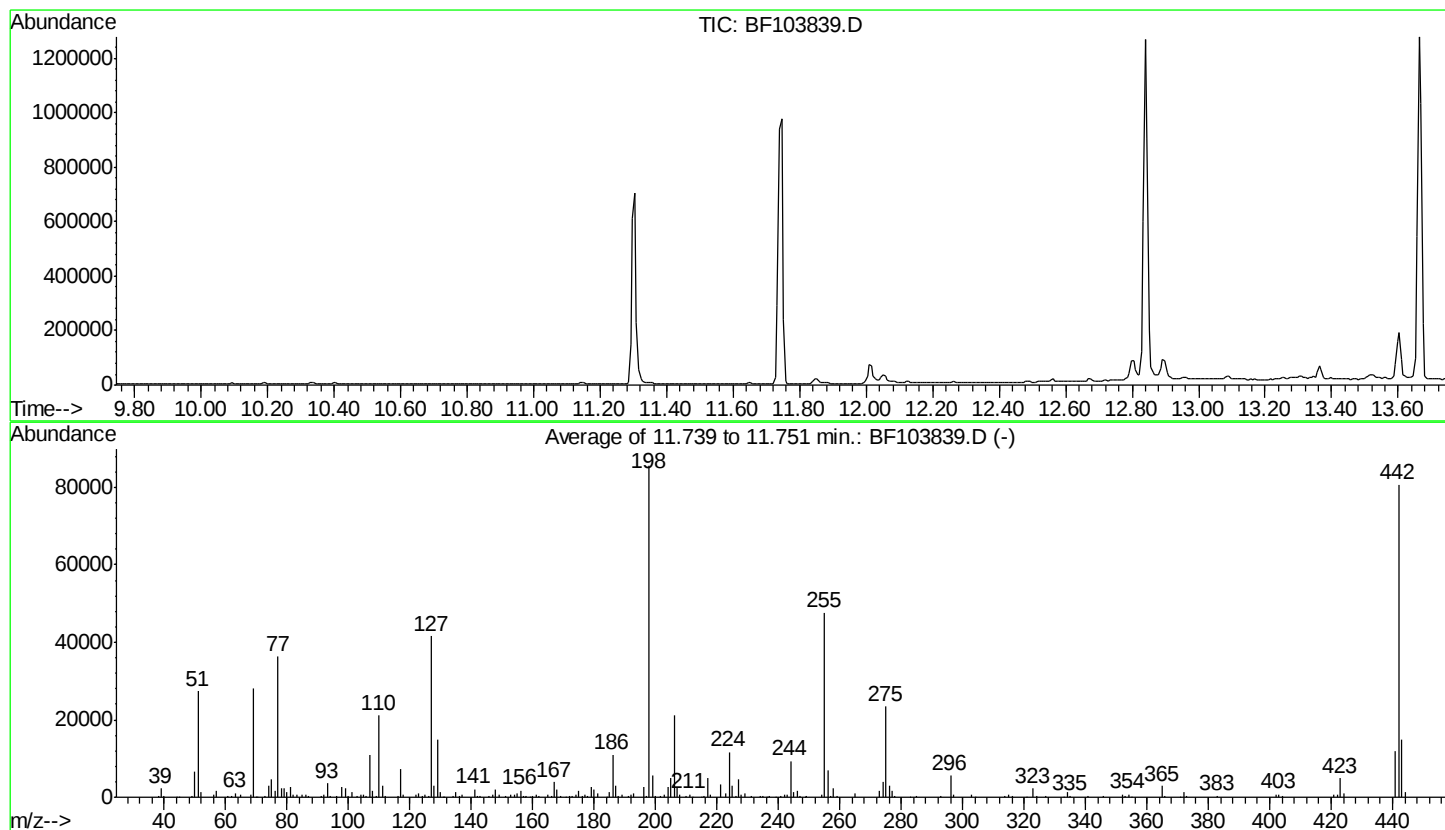

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	27362	PASS
68	69	0.00	2	1.9	525	PASS
69	198	0.00	100	32.8	28034	PASS
70	69	0.00	2	0.5	129	PASS
127	198	10	80	48.6	41624	PASS
197	198	0.00	2	0.4	353	PASS
198	198	100	100	100.0	85592	PASS
199	198	5	9	6.5	5545	PASS
275	198	10	60	27.3	23328	PASS
365	198	1	100	3.4	2938	PASS
441	443	0.01	100	80.4	11967	PASS
442	198	50	100	94.3	80688	PASS
443	442	15	24	18.5	14889	PASS