
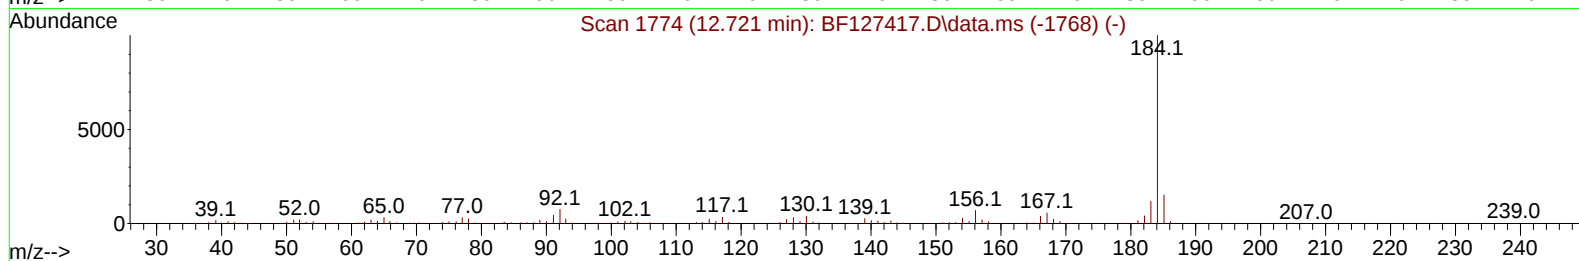
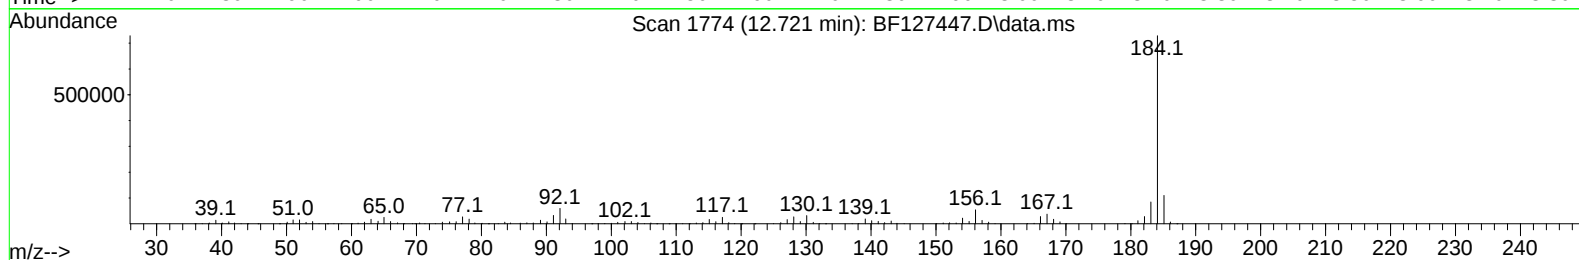


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127447.D
Acq On : 22 Mar 2022 12:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 04:23:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

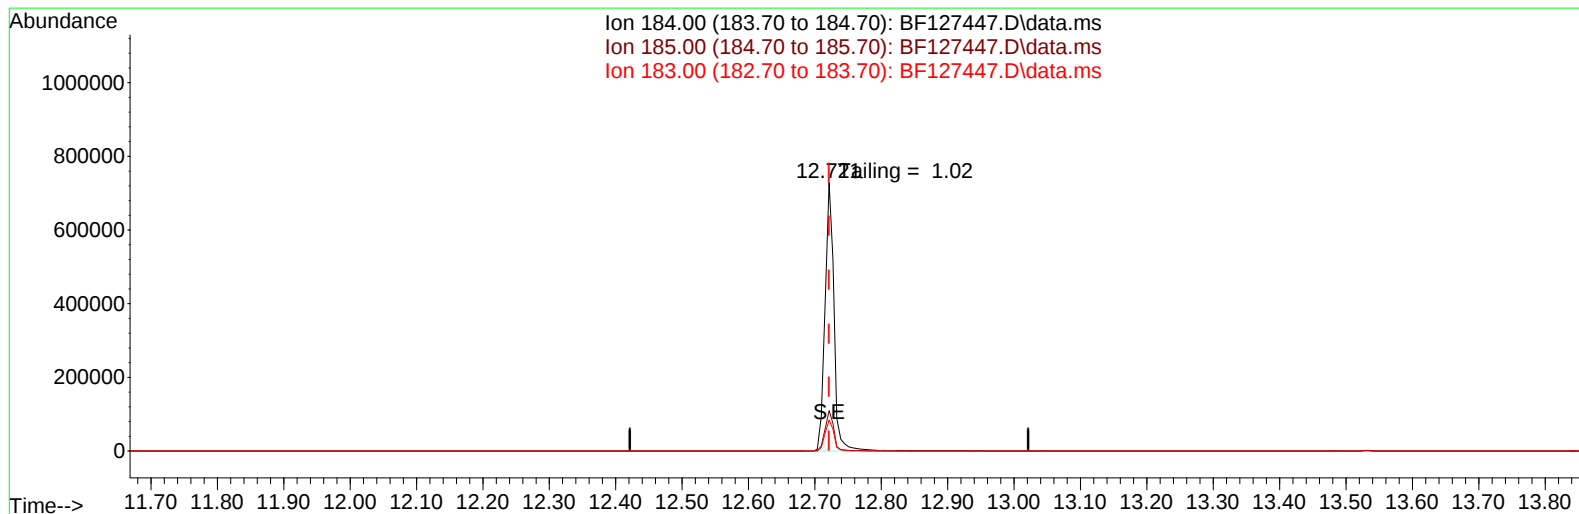

TIC: BF127447.D\data.ms

(77) Benzidine




12.721min (-0.000) 0.00 ng

response 685845

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.05
183.00	11.70	11.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127447.D
Acq On : 22 Mar 2022 12:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 04:23:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

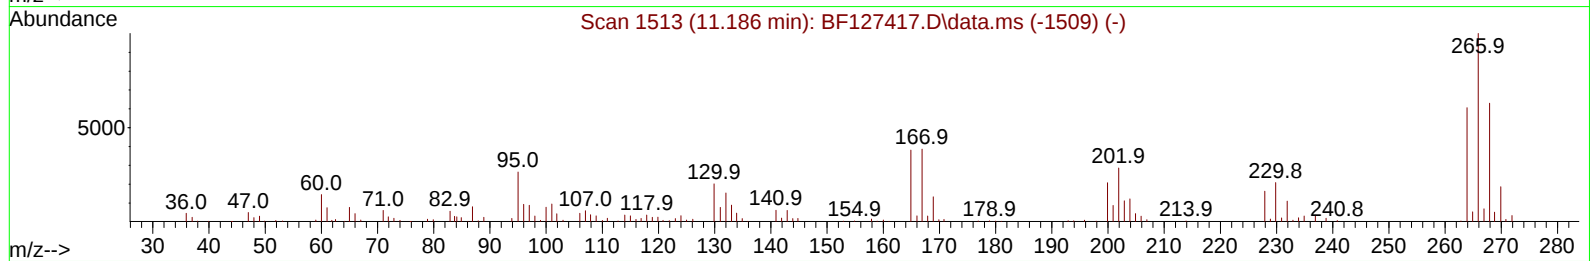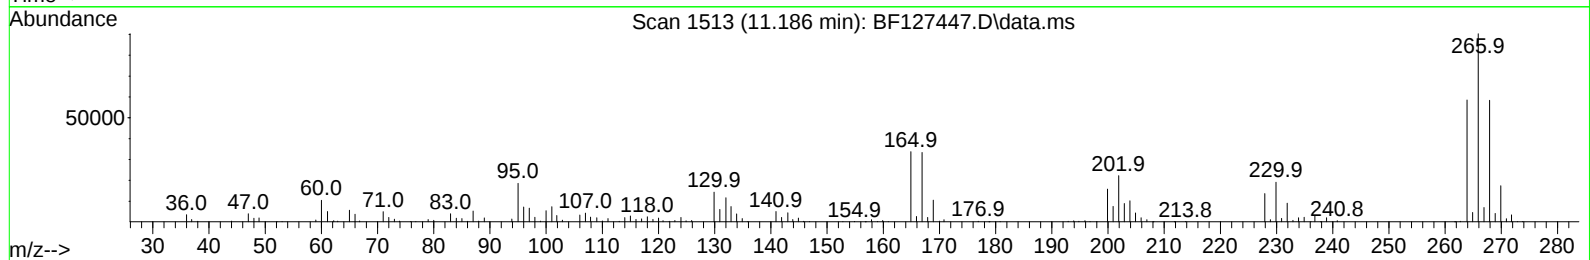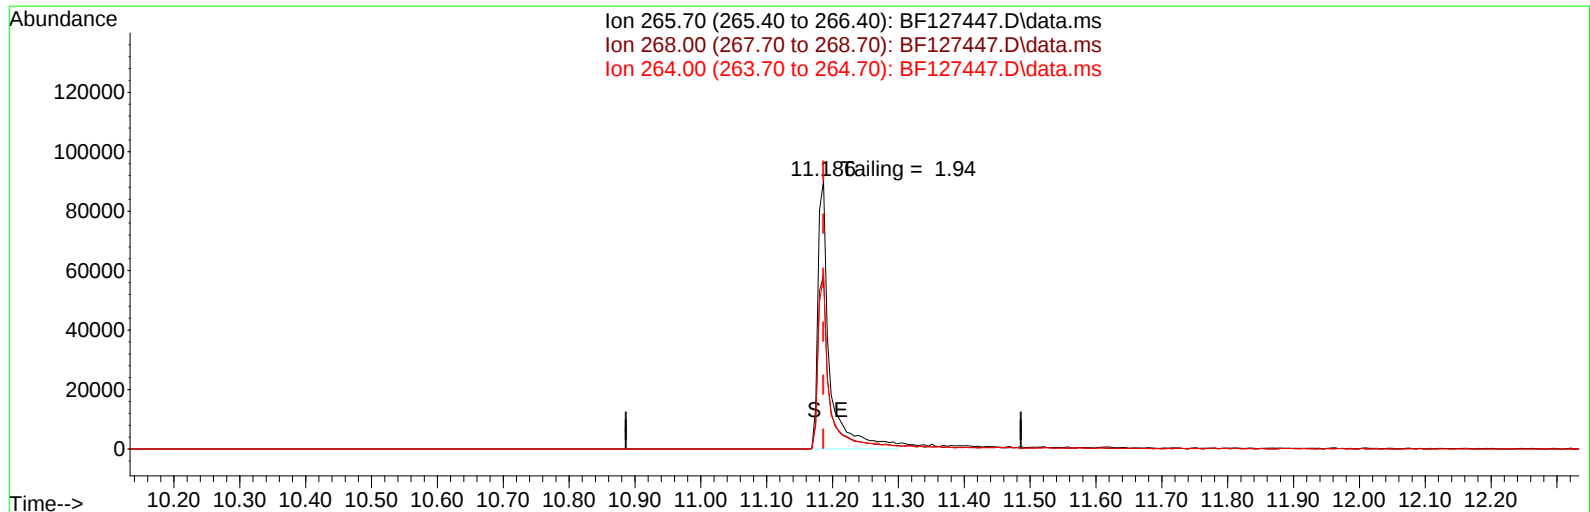

TIC: BF127447.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 42528.50 ng

response 115383

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.66
264.00	60.60	64.81
0.00	0.00	0.00