

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
 Data File : BF127449.D
 Acq On : 22 Mar 2022 13:45
 Operator : CG\JU
 Sample : PB143450BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143450BL

Quant Time: Mar 23 03:00:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 02:16:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.845	152	100949	20.000	ng	0.00
21) Naphthalene-d8	8.128	136	373724	20.000	ng	0.00
39) Acenaphthene-d10	9.886	164	217655	20.000	ng	0.00
64) Phenanthrene-d10	11.374	188	402331	20.000	ng	0.00
76) Chrysene-d12	14.021	240	284178	20.000	ng	0.00
86) Perylene-d12	15.504	264	209363	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	519986	82.221	ng	0.01
7) Phenol-d6	6.481	99	715276	82.741	ng	0.00
23) Nitrobenzene-d5	7.416	82	690135	78.936	ng	0.00
42) 2,4,6-Tribromophenol	10.680	330	153552	66.227	ng	0.00
45) 2-Fluorobiphenyl	9.204	172	1166087	78.232	ng	0.00
79) Terphenyl-d14	12.969	244	1387211	79.911	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127449.D
Acq On : 22 Mar 2022 13:45
Operator : CG\JU
Sample : PB143450BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143450BL

Quant Time: Mar 23 03:00:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration



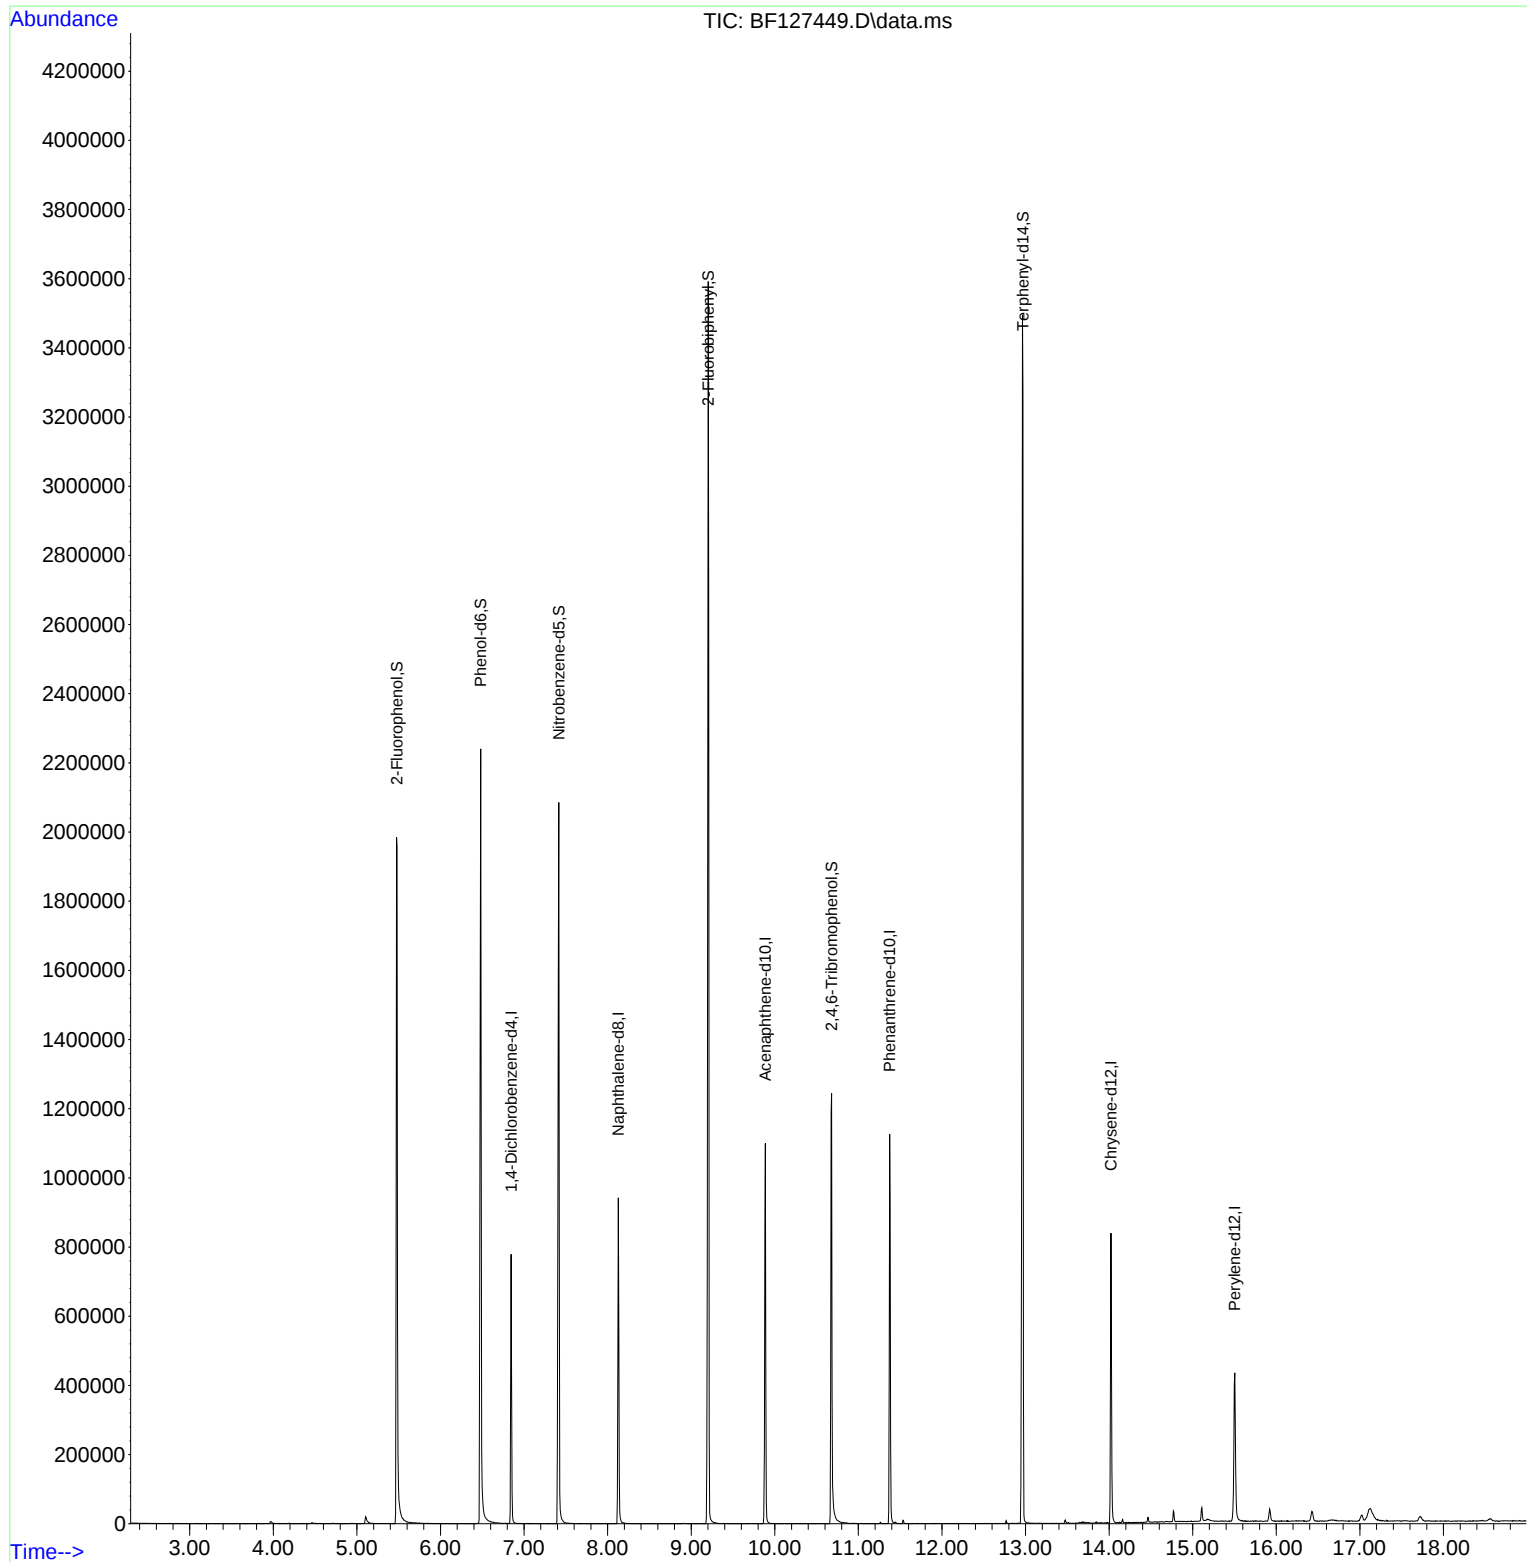




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.845 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45




Instrument :
BNA_F
ClientSampleId :
PB143450BL


Tgt Ion:152 Resp: 100949
Ion Ratio Lower Upper
152 100
150 145.6 117.2 175.8
115 62.9 49.8 74.6

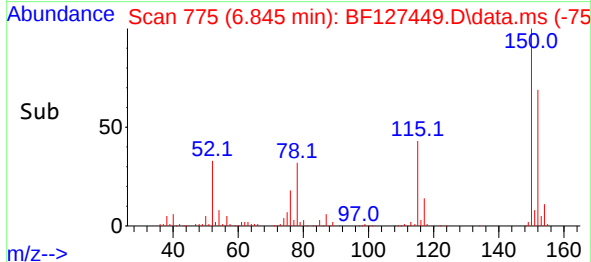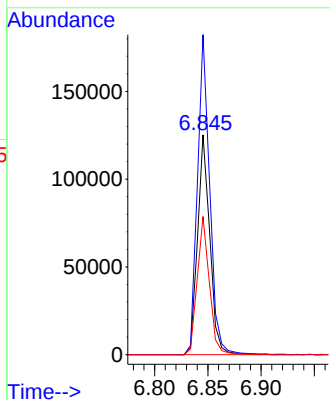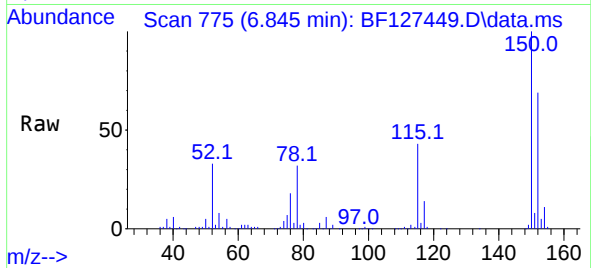

#5
2-Fluorophenol
Concen: 82.221 ng
RT: 5.481 min Scan# 543
Delta R.T. 0.012 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45

Tgt Ion:112 Resp: 519986
Ion Ratio Lower Upper
112 100
64 72.9 58.4 87.6
63 37.2 30.1 45.1


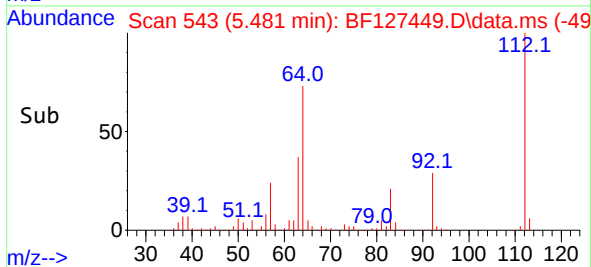
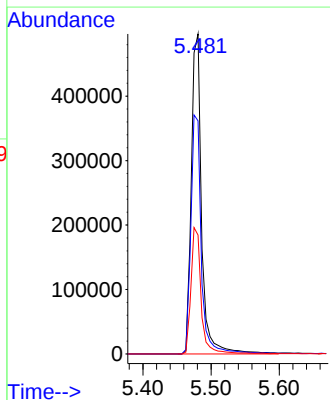
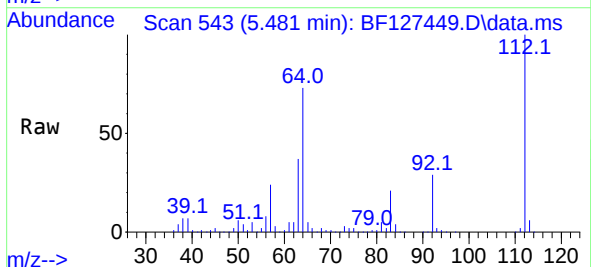


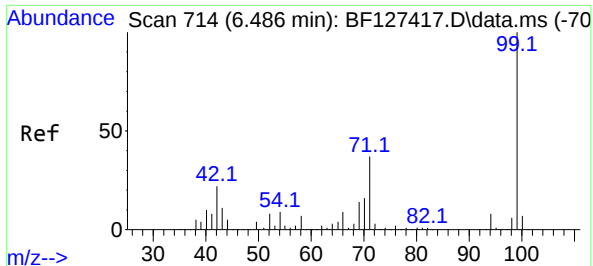

#7
Phenol-d6
Concen: 82.741 ng
RT: 6.481 min Scan# 714
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45




Instrument :
BNA_F
ClientSampleId :
PB143450BL


Tgt Ion: 99 Resp: 715276
Ion Ratio Lower Upper
99 100
42 23.0 17.8 26.6
71 38.0 29.6 44.4

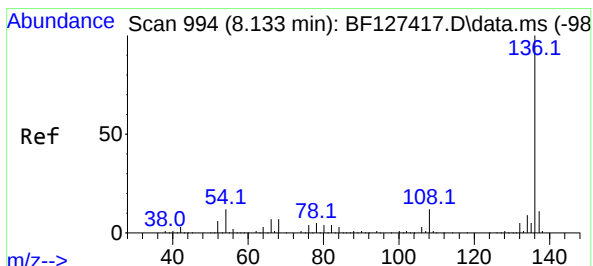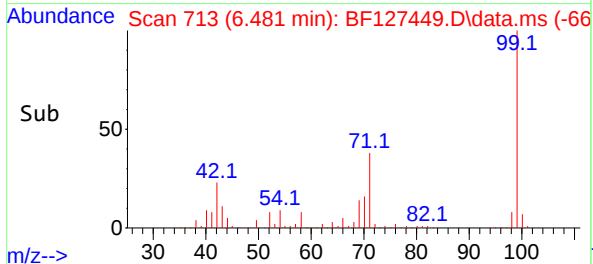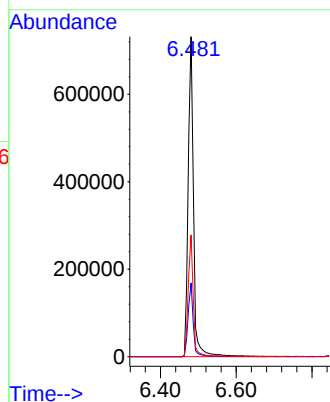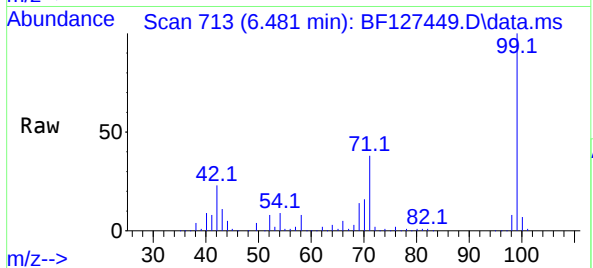

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.128 min Scan# 993
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45

Tgt Ion: 136 Resp: 373724
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 12.4 9.2 13.8
68 7.3 5.4 8.0


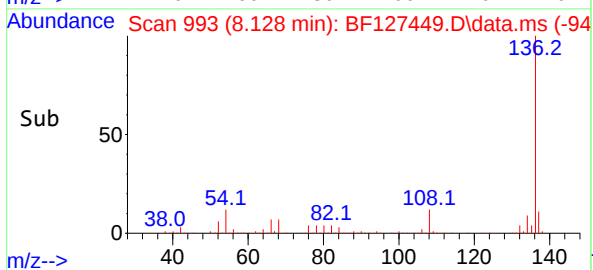
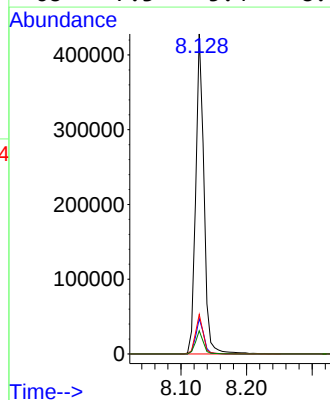
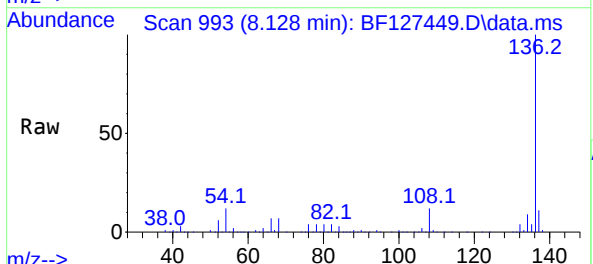


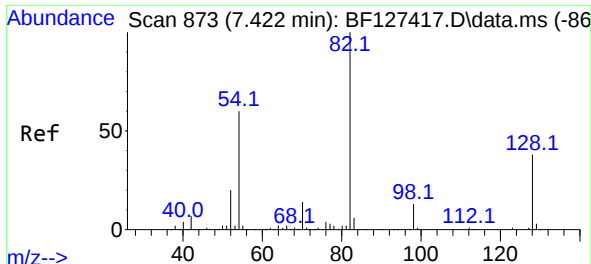

#23
Nitrobenzene-d5
Concen: 78.936 ng
RT: 7.416 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45




Instrument :
BNA_F
ClientSampleId :
PB143450BL


Tgt Ion: 82 Resp: 690135
Ion Ratio Lower Upper
82 100
128 38.1 30.6 45.8
54 60.9 48.2 72.2

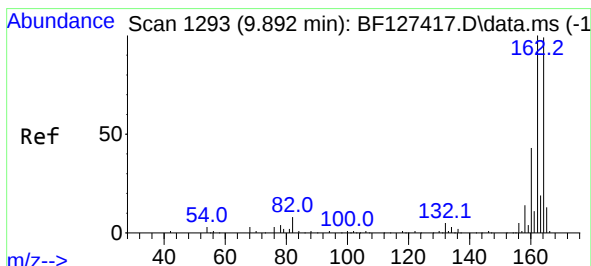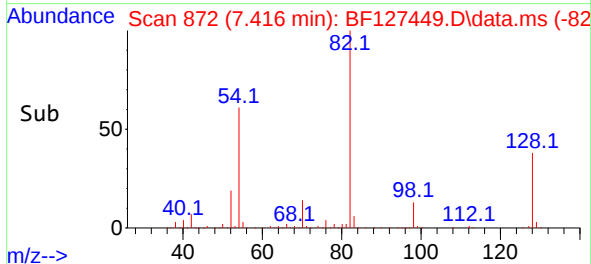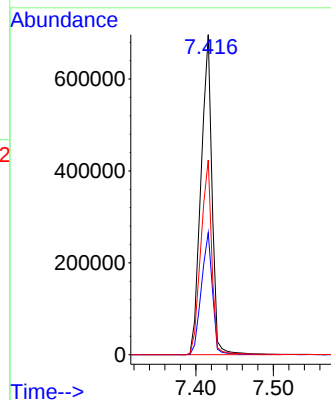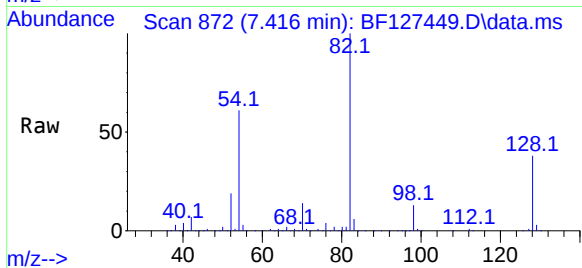

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.886 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45

Tgt Ion:164 Resp: 217655
Ion Ratio Lower Upper
164 100
162 101.9 81.2 121.8
160 44.1 34.6 52.0

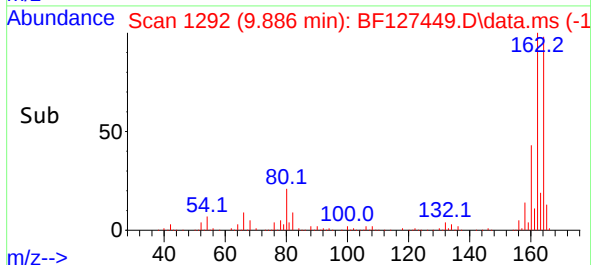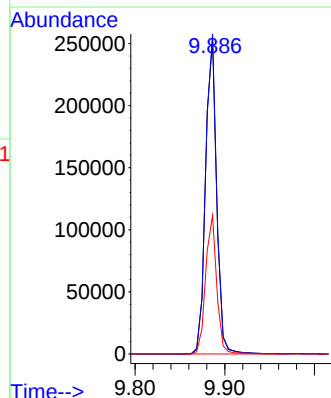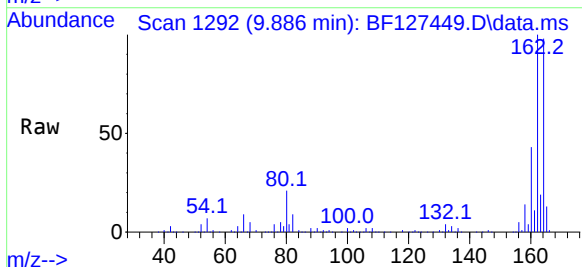

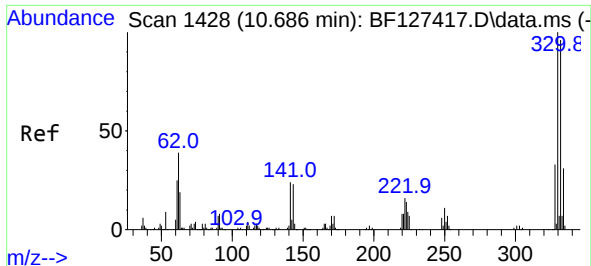

#42

2,4,6-Tribromophenol

Concen: 66.227 ng

RT: 10.680 min Scan# 1428

Delta R.T. -0.006 min

Lab File: BF127449.D

Acq: 22 Mar 2022 13:45

Instrument :

BNA_F

ClientSampleId :

PB143450BL




Tgt Ion:330 Resp: 153552

Ion Ratio Lower Upper

330 100

332 97.9 79.1 118.7

141 34.5 26.2 39.4

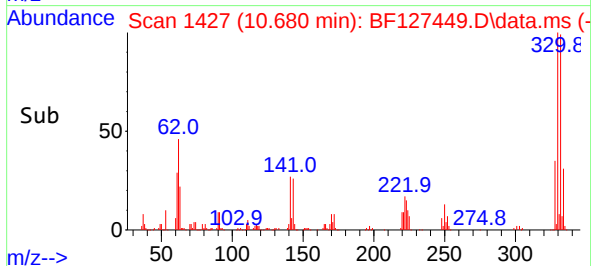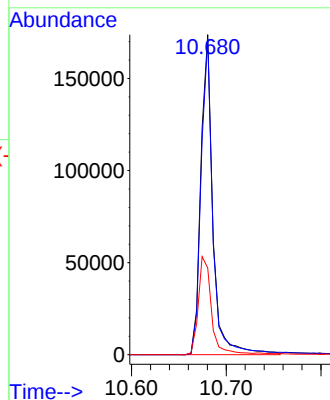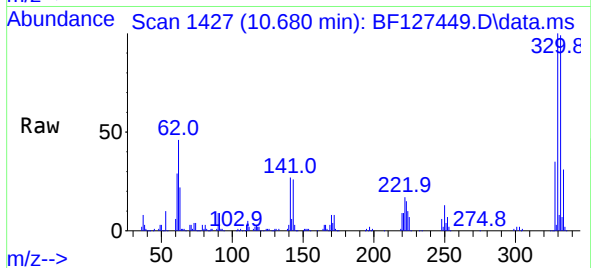

#45

2-Fluorobiphenyl

Concen: 78.232 ng

RT: 9.204 min Scan# 1176

Delta R.T. -0.006 min

Lab File: BF127449.D

Acq: 22 Mar 2022 13:45




Tgt Ion:172 Resp: 1166087

Ion Ratio Lower Upper

172 100

171 35.6 28.4 42.6

170 23.7 18.6 27.8


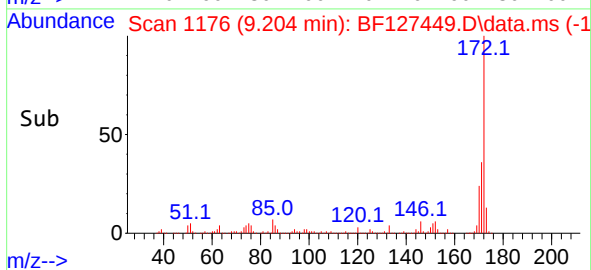
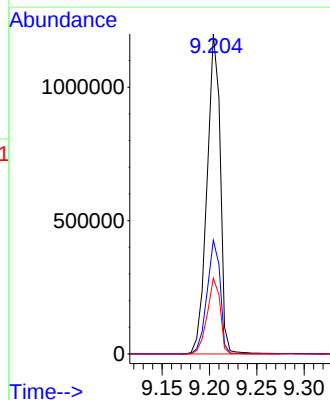
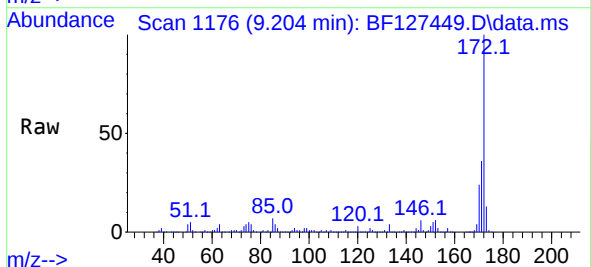




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.374 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45




Instrument :
BNA_F
ClientSampleId :
PB143450BL


Tgt Ion:188 Resp: 402331
Ion Ratio Lower Upper
188 100
94 10.8 7.4 11.0
80 11.6 8.0 12.0

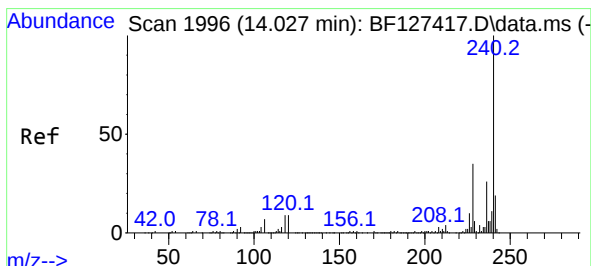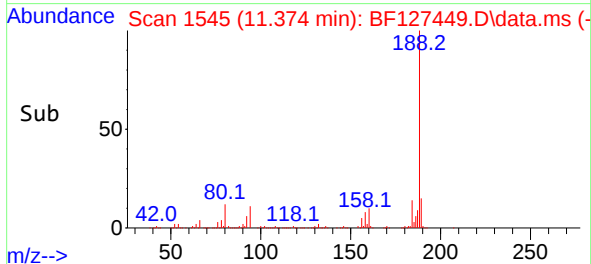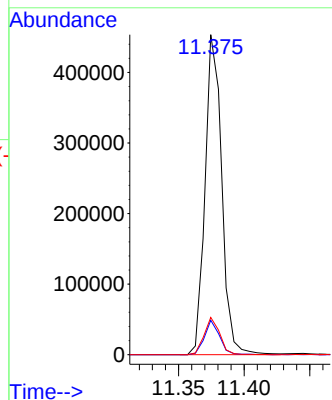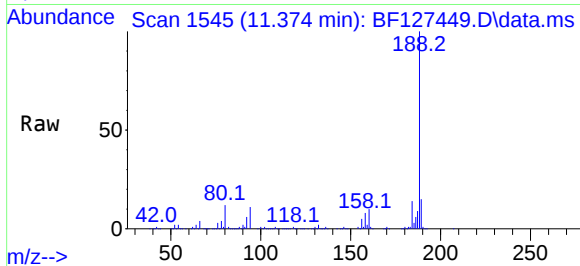

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.021 min Scan# 1995
Delta R.T. -0.006 min
Lab File: BF127449.D
Acq: 22 Mar 2022 13:45

Tgt Ion:240 Resp: 284178
Ion Ratio Lower Upper
240 100
120 9.6 7.1 10.7
236 24.9 20.7 31.1


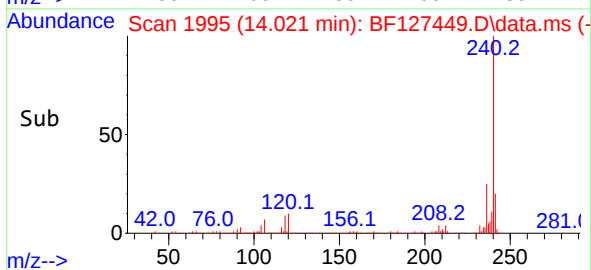
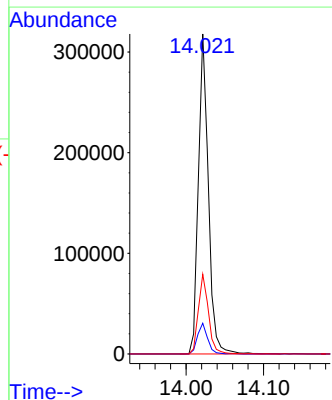
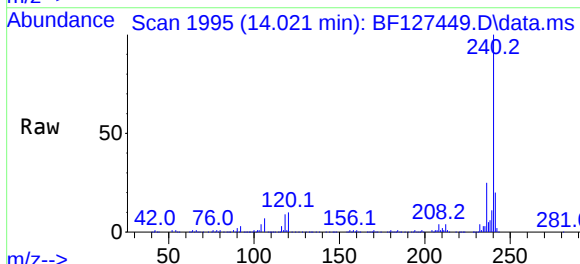


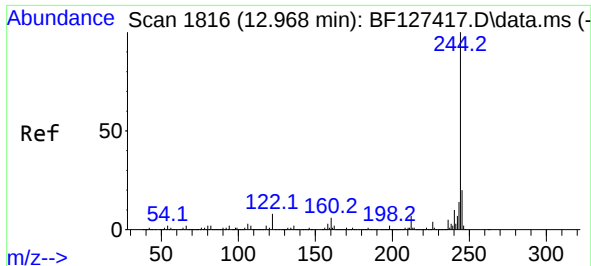

#79
 Terphenyl-d14
 Concen: 79.911 ng
 RT: 12.969 min Scan# 1816
 Delta R.T. 0.000 min
 Lab File: BF127449.D
 Acq: 22 Mar 2022 13:45

Instrument :
 BNA_F
 ClientSampleId :
 PB143450BL

Tgt Ion:244 Resp: 1387211
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.7 8.5
 122 7.8 6.2 9.2

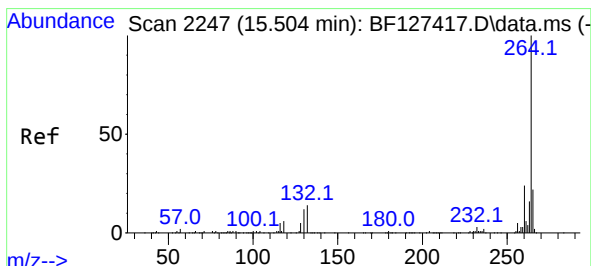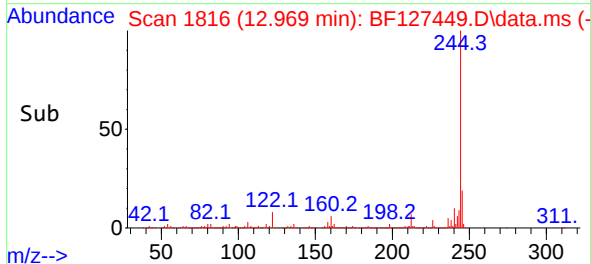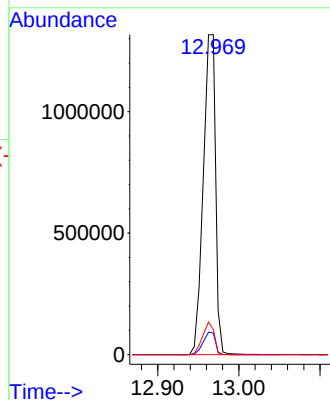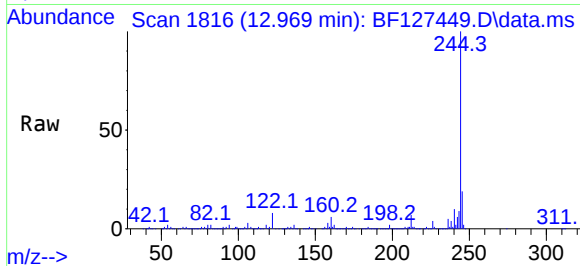

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.504 min Scan# 2247
 Delta R.T. 0.000 min
 Lab File: BF127449.D
 Acq: 22 Mar 2022 13:45

Tgt Ion:264 Resp: 209363
 Ion Ratio Lower Upper
 264 100
 260 22.9 19.1 28.7
 265 21.0 17.4 26.2

