

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
 Data File : BF127453.D
 Acq On : 22 Mar 2022 15:47
 Operator : CG\JU
 Sample : PB143505BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143505BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	539	543	569	rBV	2991659	3167639	85.35%	14.158%
2	6.486	709	714	717	rBV	2859425	3121253	84.10%	13.950%
3	6.845	772	775	785	rBV	756589	628659	16.94%	2.810%
4	7.416	867	872	875	rBV	2145069	2165958	58.36%	9.681%
5	8.128	989	993	1005	rBV	923187	819395	22.08%	3.662%
6	9.204	1170	1176	1179	rBV	3600124	3627384	97.74%	16.212%
7	9.886	1288	1292	1312	rVB	1153692	954344	25.72%	4.265%
8	10.680	1423	1427	1430	rBV	2204219	1925869	51.89%	8.608%
9	11.374	1542	1545	1554	rBV	1104530	991163	26.71%	4.430%
10	12.963	1810	1815	1818	rBV	3581831	3711175	100.00%	16.587%
11	14.021	1992	1995	2005	rBV	768446	716307	19.30%	3.202%
12	15.504	2237	2247	2259	rBV	405981	544863	14.68%	2.435%




Sum of corrected areas: 22374009

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127453.D
Acq On : 22 Mar 2022 15:47
Operator : CG\JU
Sample : PB143505BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143505BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

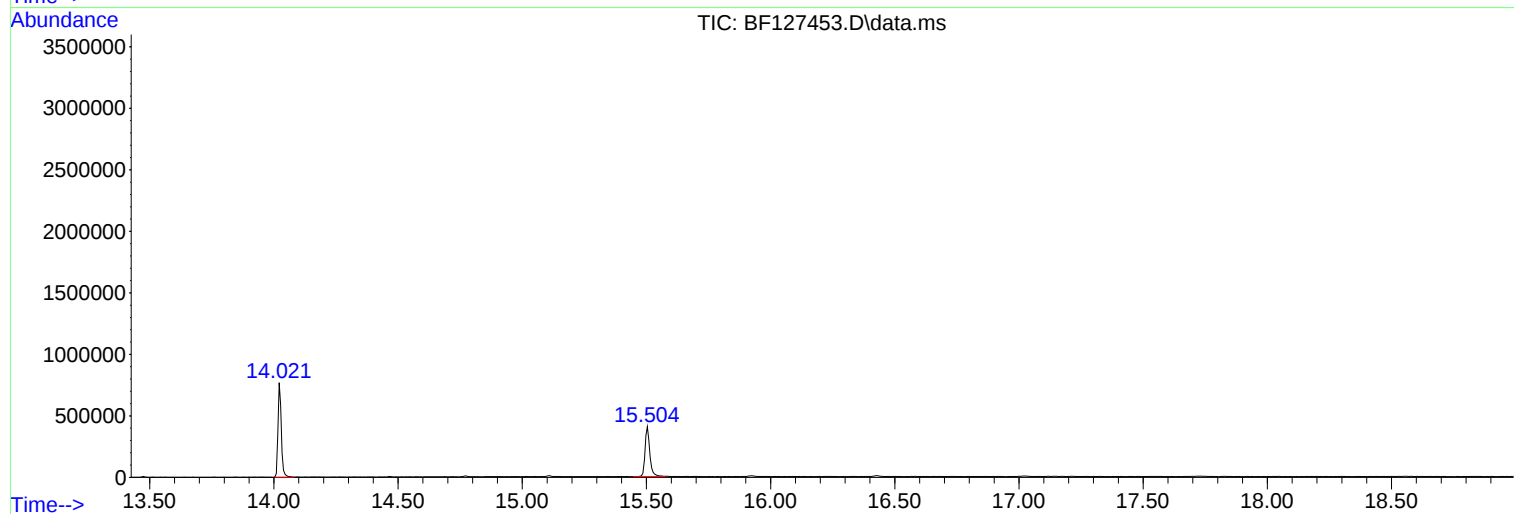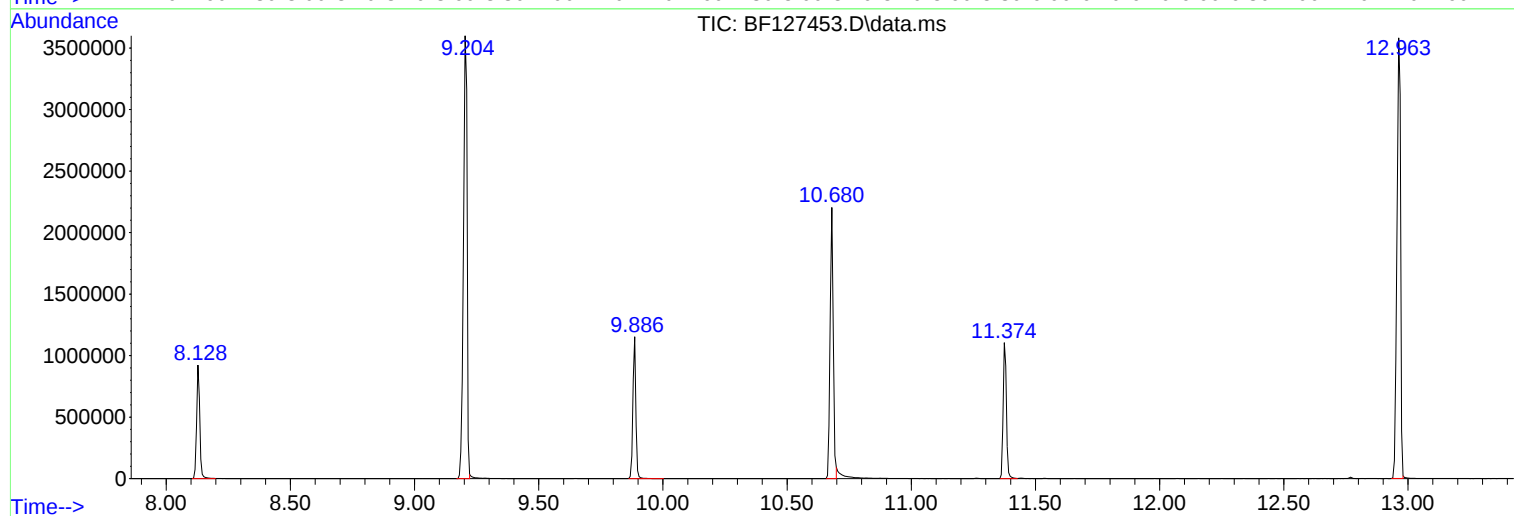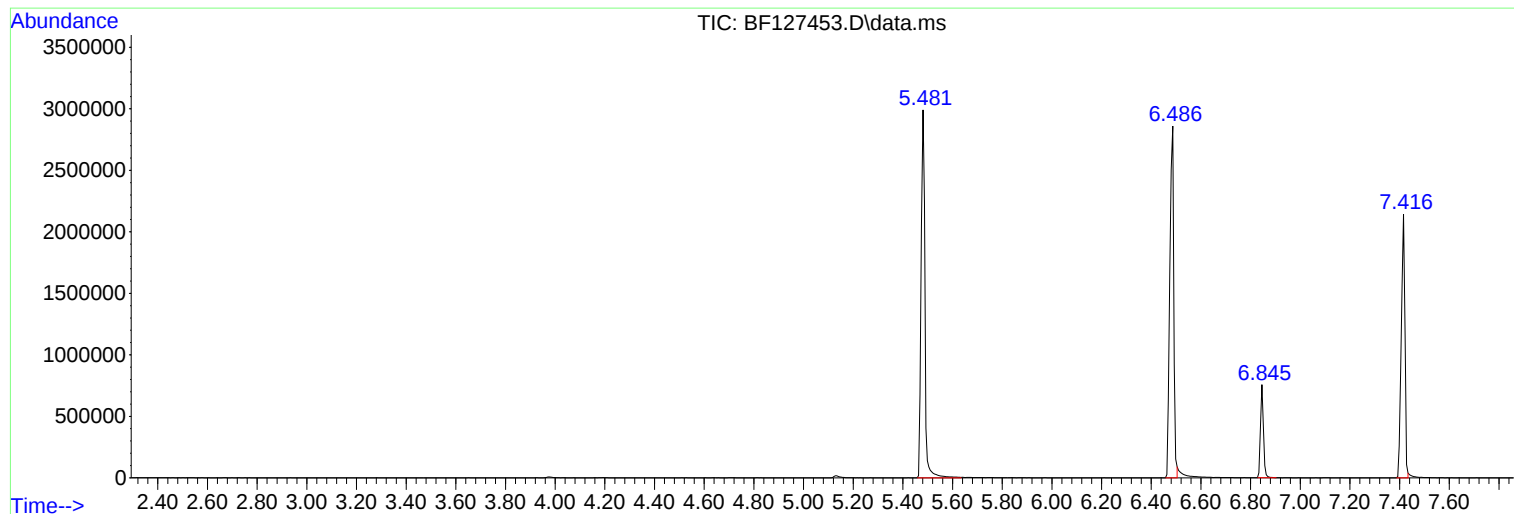

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127453.D
Acq On : 22 Mar 2022 15:47
Operator : CG\JU
Sample : PB143505BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143505BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127453.D
Acq On : 22 Mar 2022 15:47
Operator : CG\JU
Sample : PB143505BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143505BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------