

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
 Data File : BF127468.D
 Acq On : 22 Mar 2022 23:07
 Operator : CG\JU
 Sample : N1949-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CP-BH1-031422-2-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	473	476	485	rBV	20846	29656	1.20%	0.177%
2	5.469	538	541	564	rBV	2158037	2050304	82.72%	12.251%
3	6.481	709	713	732	rBV	2245439	2182019	88.03%	13.038%
4	6.845	772	775	784	rBV	747627	603760	24.36%	3.608%
5	7.410	867	871	883	rBV	1441539	1458697	58.85%	8.716%
6	8.128	989	993	998	rBV	932820	783164	31.60%	4.680%
7	9.204	1172	1176	1179	rBV	2970125	2478616	100.00%	14.811%
8	9.886	1288	1292	1295	rBV	1040375	926765	37.39%	5.538%
9	10.675	1423	1426	1441	rBV	1465389	1492953	60.23%	8.921%
10	11.375	1541	1545	1553	rBV	1145171	984401	39.72%	5.882%
11	12.963	1810	1815	1818	rBV	2624293	2459207	99.22%	14.695%
12	13.980	1975	1988	1991	rBV2	26022	64064	2.58%	0.383%
13	14.021	1991	1995	2006	rVB	676799	611191	24.66%	3.652%
14	15.104	2176	2179	2185	rVB2	29007	34497	1.39%	0.206%
15	15.504	2240	2247	2255	rBV	422450	547128	22.07%	3.269%
16	15.921	2313	2318	2323	rBV3	19014	28911	1.17%	0.173%




Sum of corrected areas: 16735333

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127468.D
Acq On : 22 Mar 2022 23:07
Operator : CG\JU
Sample : N1949-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CP-BH1-031422-2-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

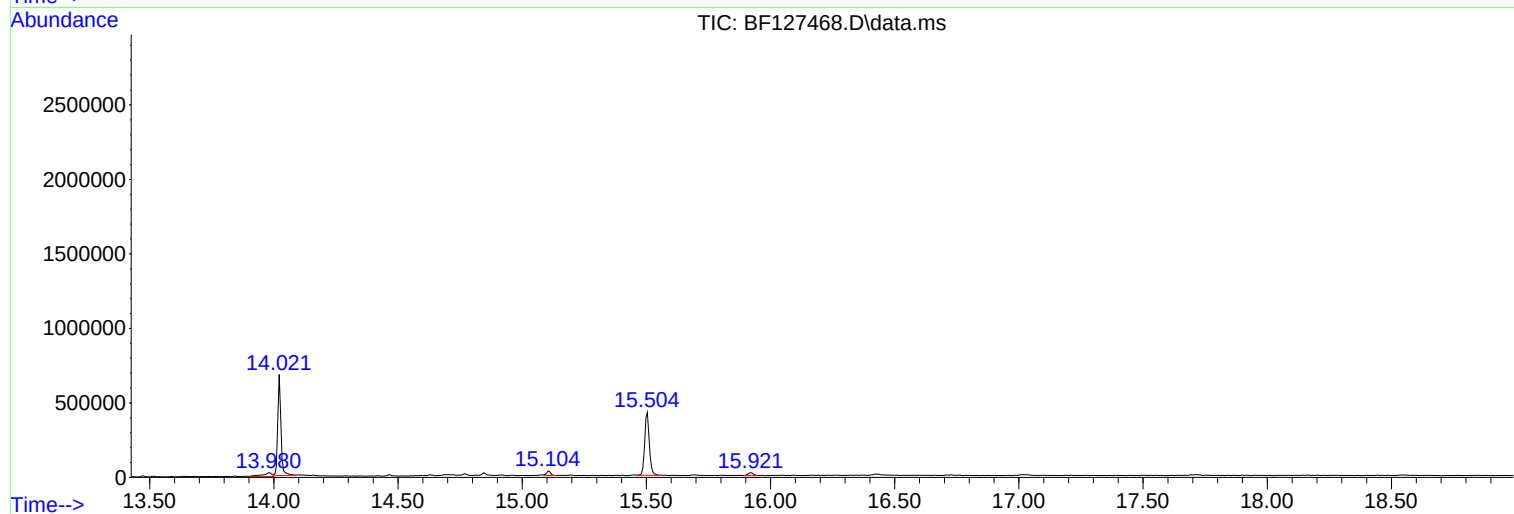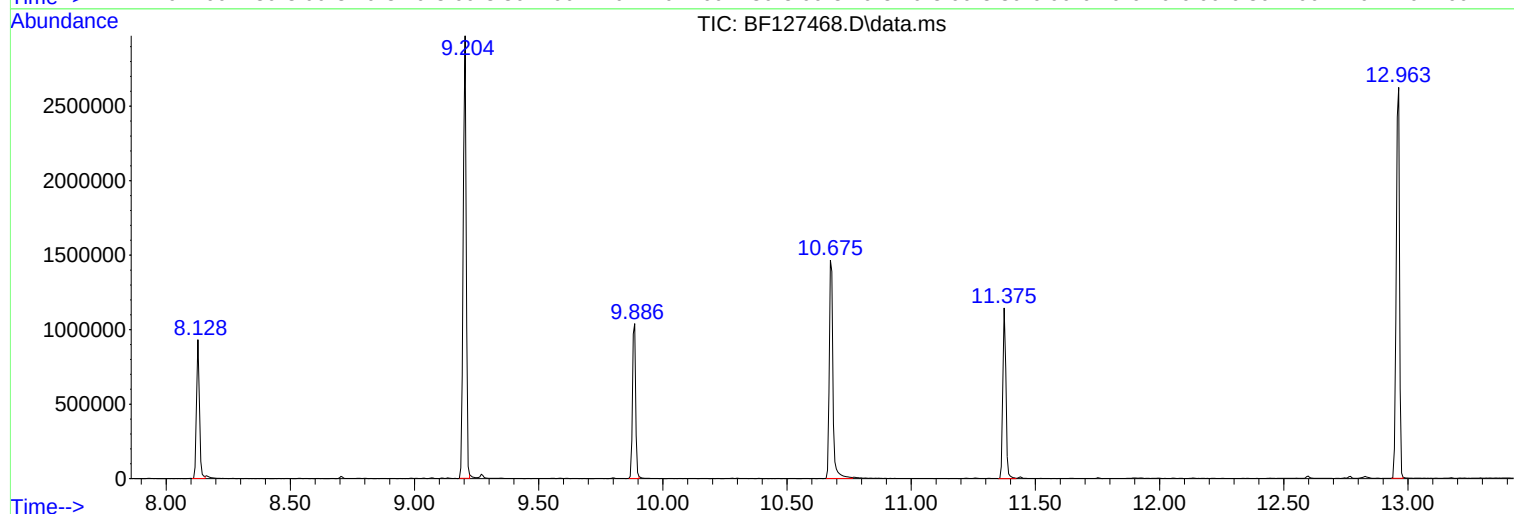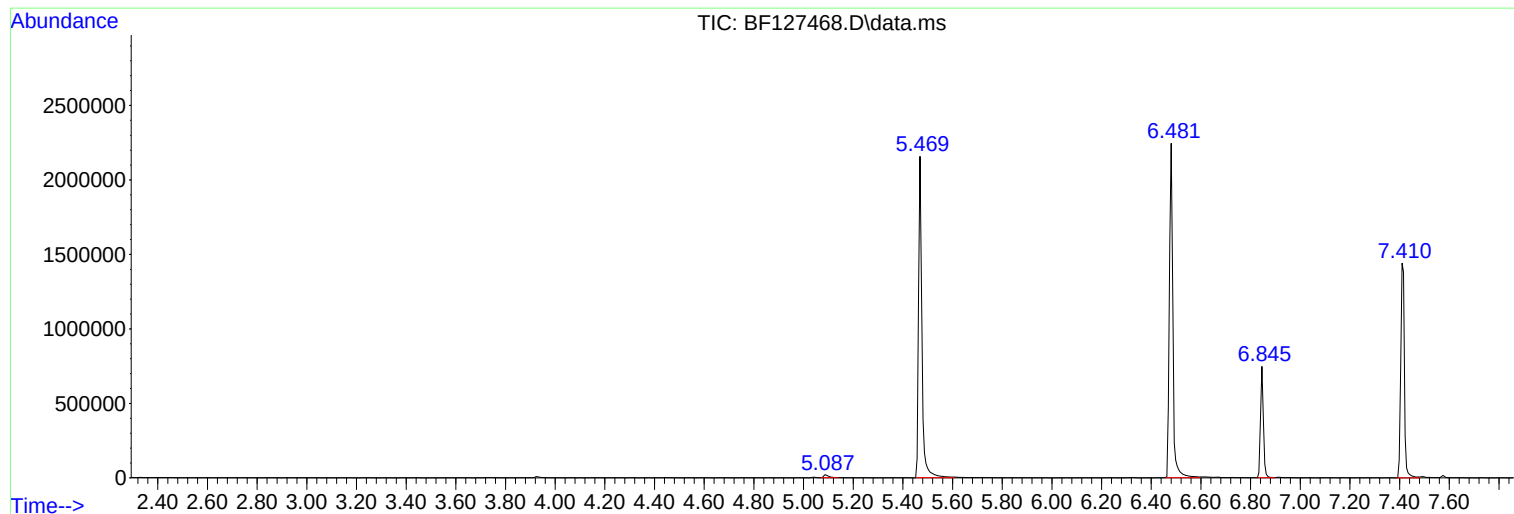

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127468.D
Acq On : 22 Mar 2022 23:07
Operator : CG\JU
Sample : N1949-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CP-BH1-031422-2-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
Data File : BF127468.D
Acq On : 22 Mar 2022 23:07
Operator : CG\JU
Sample : N1949-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CP-BH1-031422-2-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------