
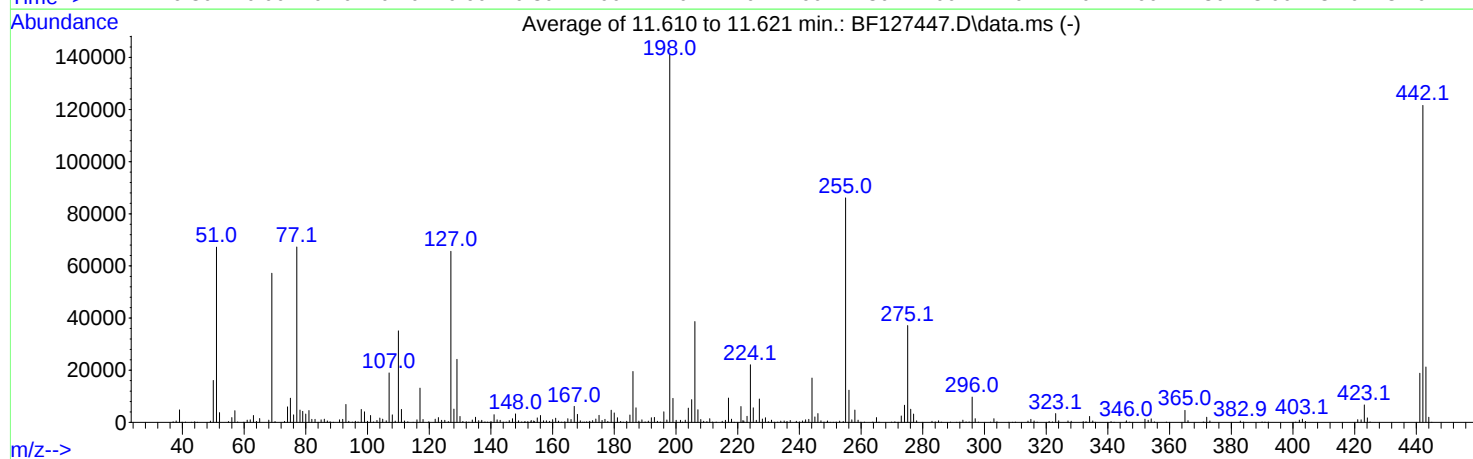


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
 Data File : BF127447.D
 Acq On : 22 Mar 2022 12:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 22 02:16:33 2022

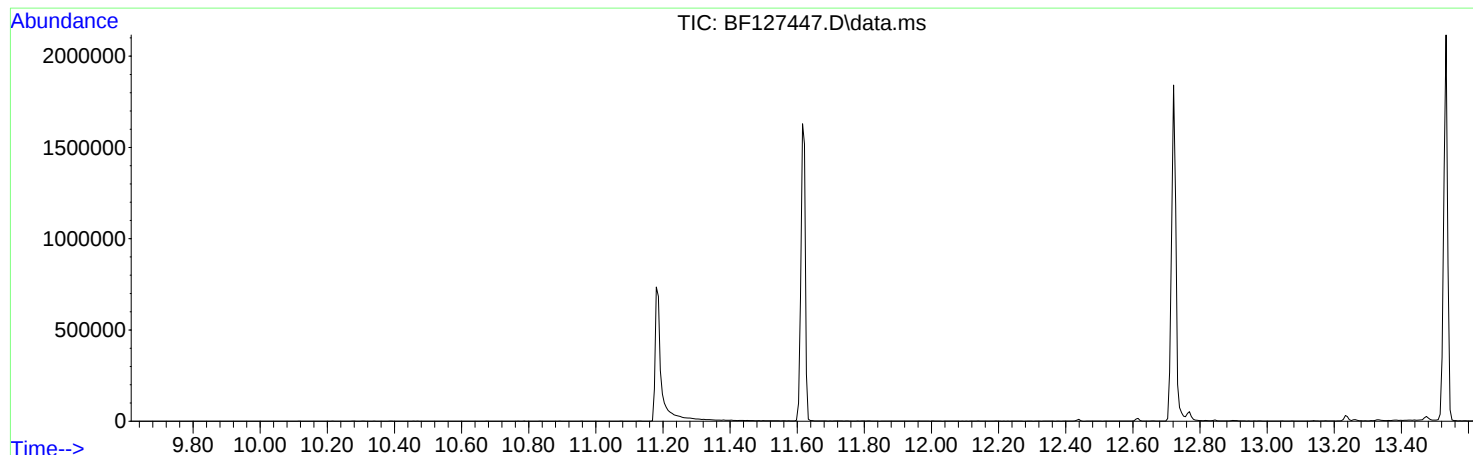




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	67176	PASS
68	69	0.00	2	1.6	893	PASS
69	198	0.00	100	40.6	57229	PASS
70	69	0.00	2	0.5	290	PASS
127	198	10	80	46.5	65624	PASS
197	198	0.00	2	0.6	915	PASS
198	198	100	100	100.0	141104	PASS
199	198	5	9	6.5	9185	PASS
275	198	10	60	26.3	37137	PASS
365	198	1	100	3.3	4636	PASS
441	198	0.01	100	13.4	18867	PASS
442	442	50	100	100.0	121605	PASS
443	442	15	24	17.5	21245	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032222\
 Data File : BF127447.D
 Acq On : 22 Mar 2022 12:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 04:23:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 02:16:33 2022
 Response via : Initial Calibration

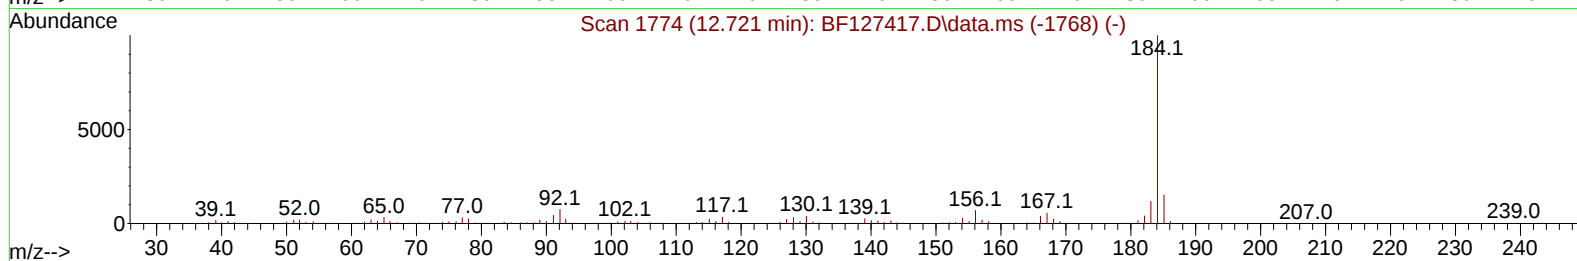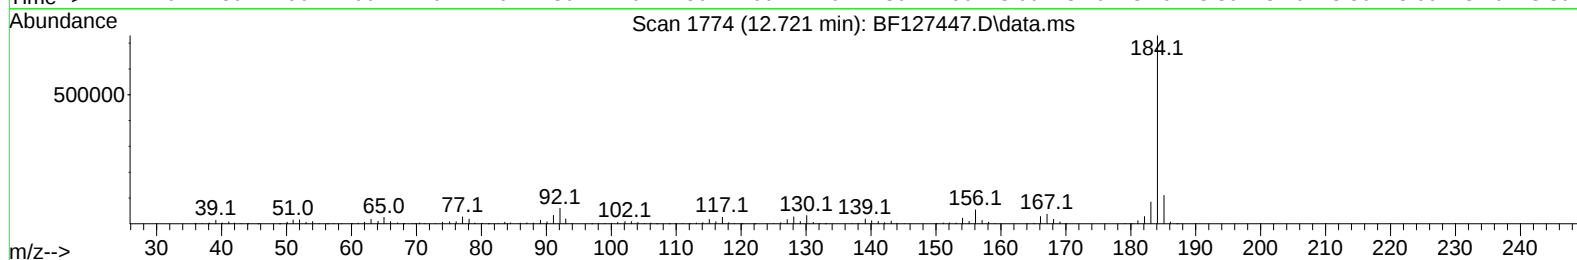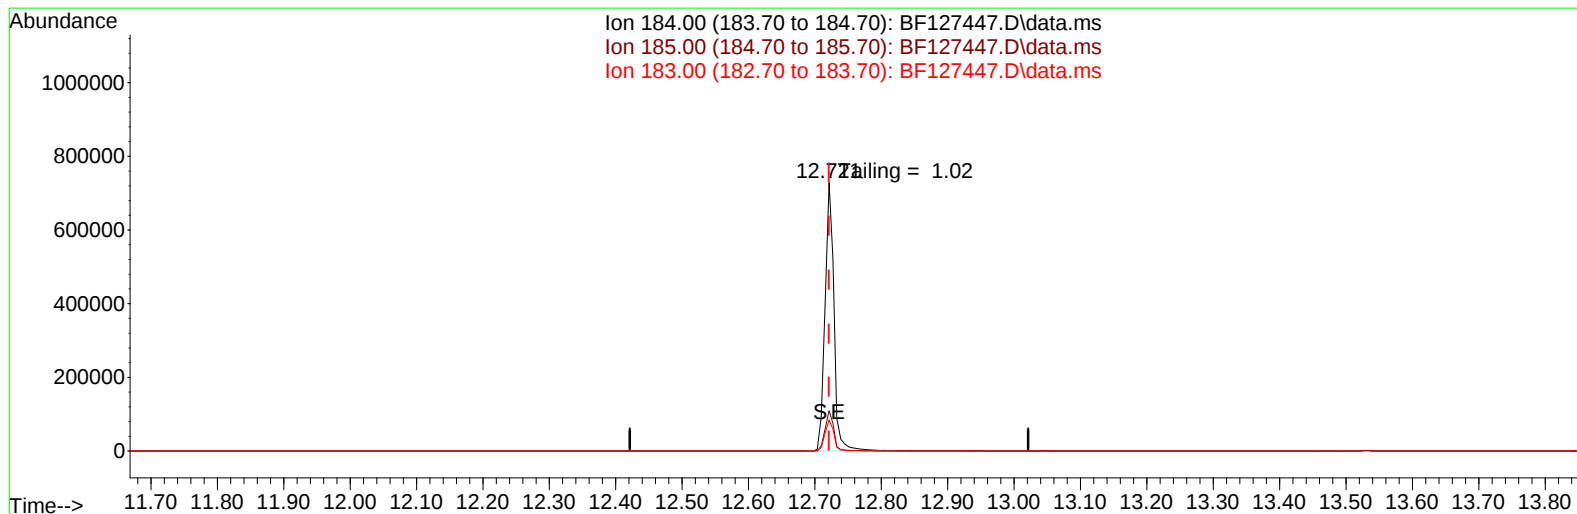

TIC: BF127447.D\data.ms

(77) Benzidine

12.721min (-0.000) 0.00 ng

response 685845

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.05
183.00	11.70	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_F	<u>BF127447.D</u>
Compound Name	Response	Retention Time
DDT	344477	13.533
DDD	8423	13.233
DDE	1122	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9545	354022	2.70

Instrument :
BNA_F
ClientSampleId :
DFTPP