
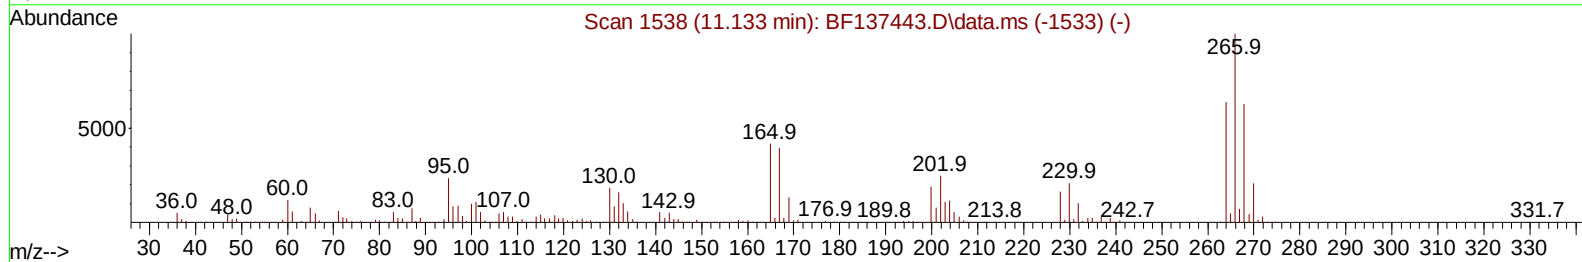
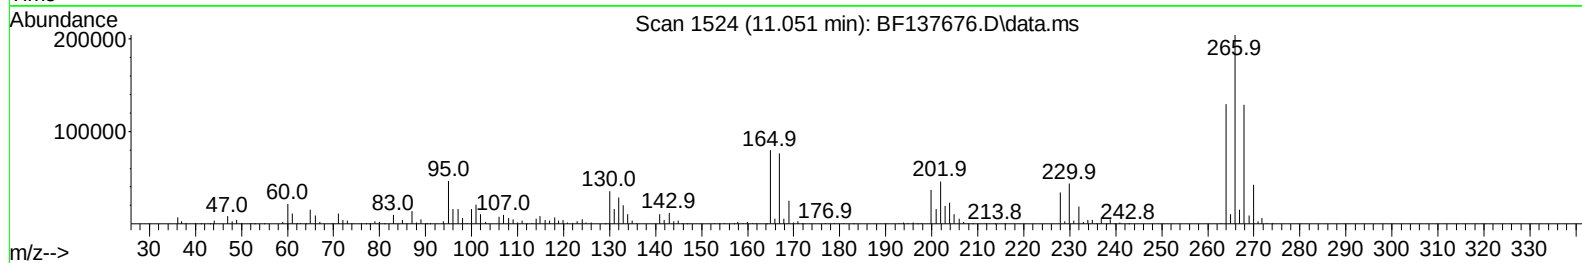


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032224\
Data File : BF137676.D
Acq On : 22 Mar 2024 11:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 01:05:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

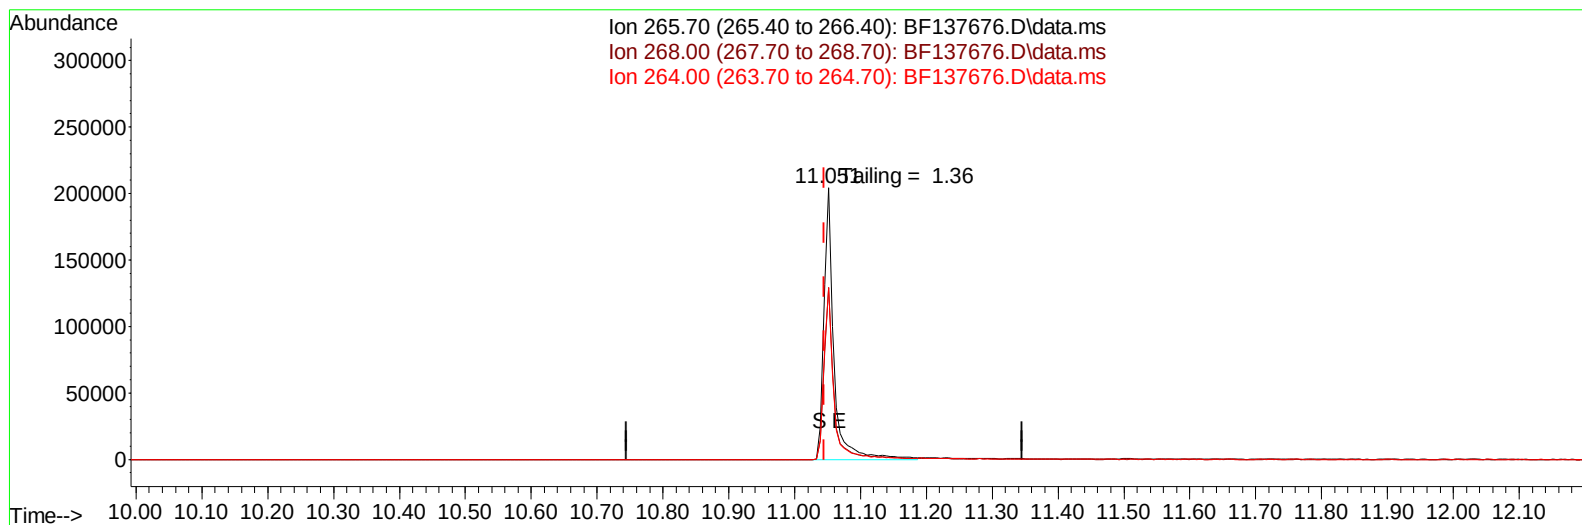

TIC: BF137676.D\data.ms

(70) Pentachlorophenol (C)




11.051min (+ 0.006) 39520.27 ng

response 213409

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.22
264.00	63.60	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032224\
Data File : BF137676.D
Acq On : 22 Mar 2024 11:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 01:05:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

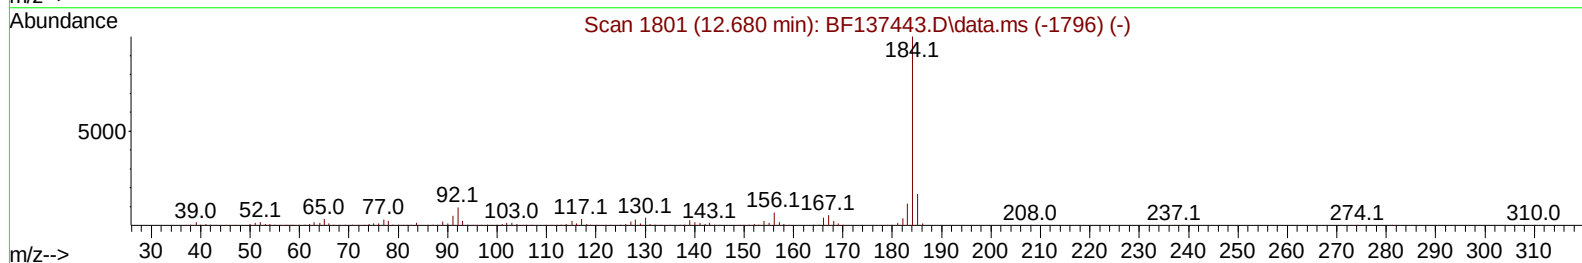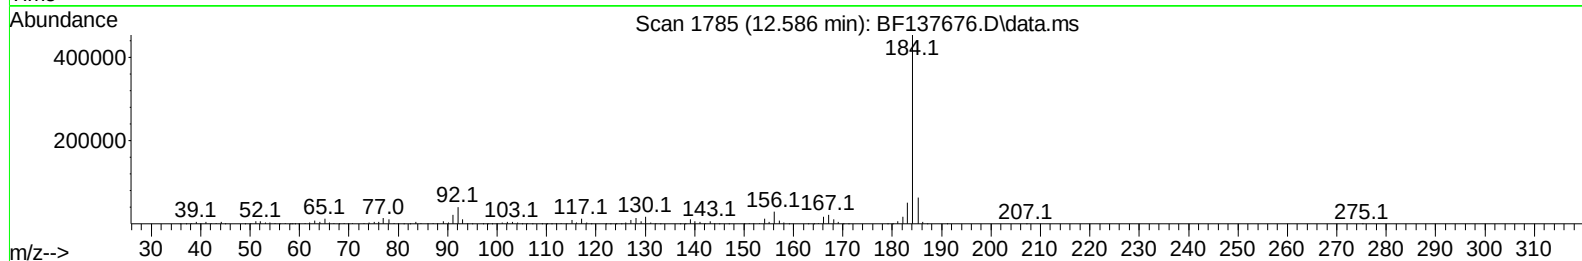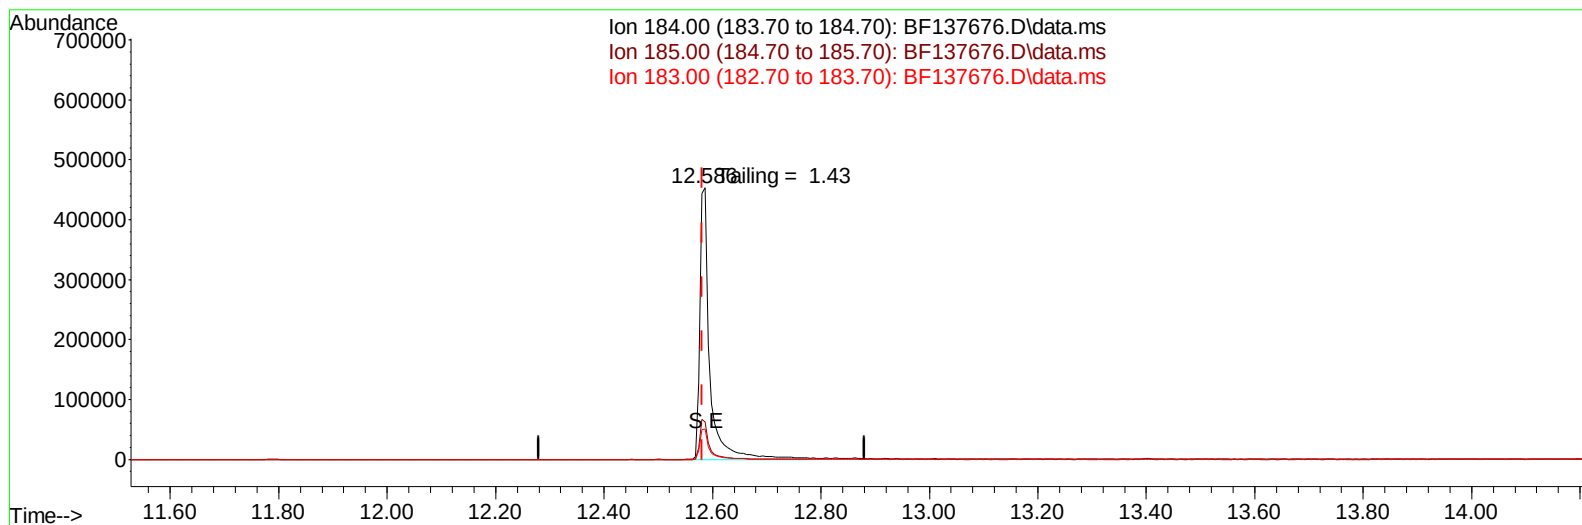

TIC: BF137676.D\data.ms

(77) Benzidine

12.586min (+ 0.006) 302787.40 ng m

response 607611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	13.86
183.00	11.60	11.12
0.00	0.00	0.00