


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032224\
Data File : BF137676.D
Acq On : 22 Mar 2024 11:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

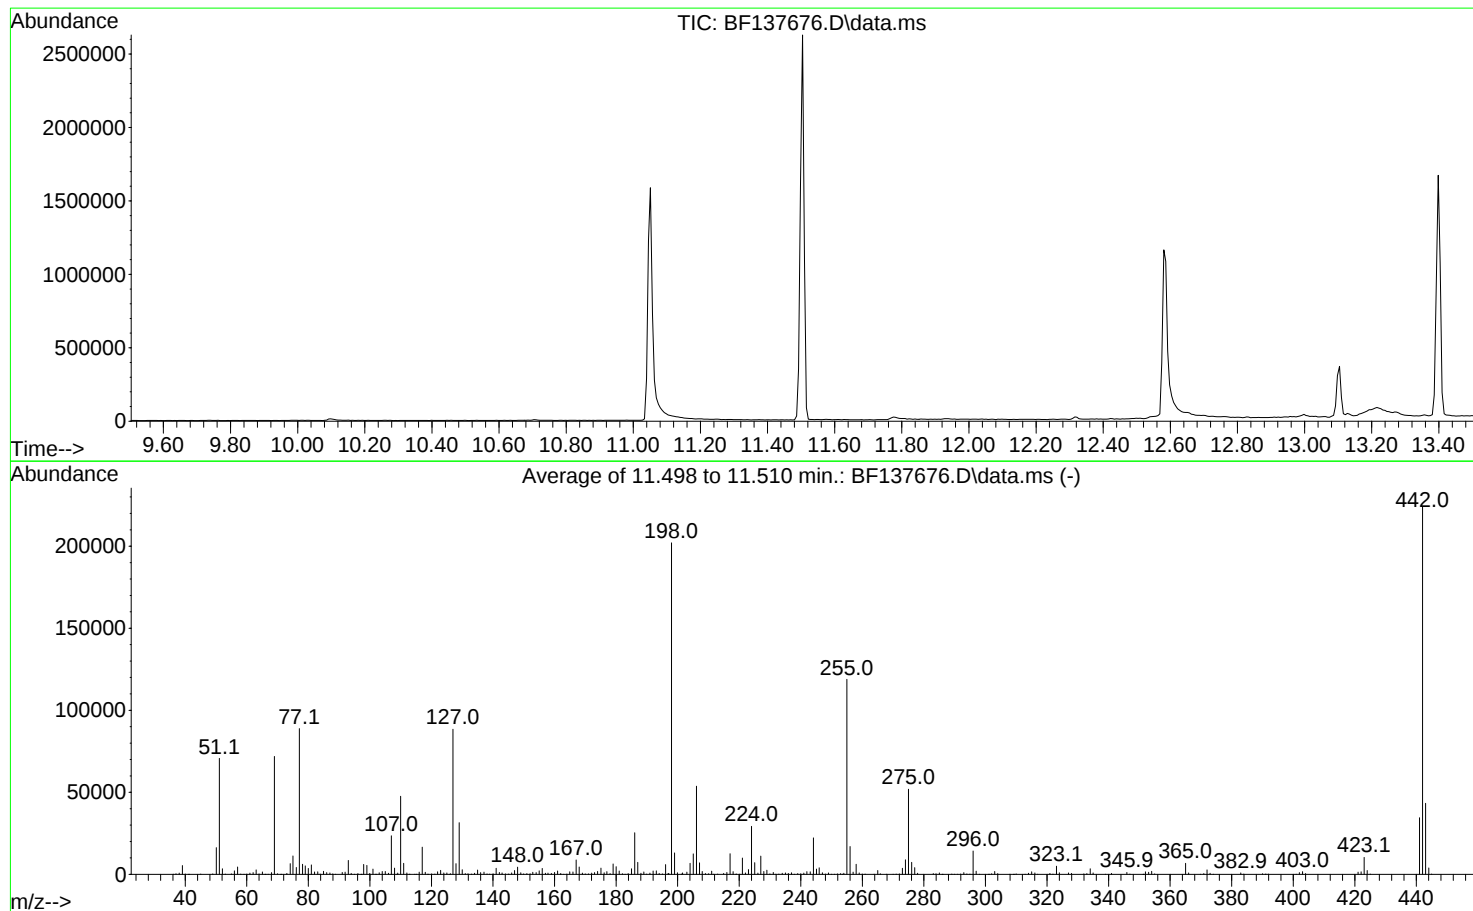




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	70667	PASS
68	69	0.00	2	1.5	1069	PASS
69	198	0.00	100	35.6	71880	PASS
70	69	0.00	2	0.6	396	PASS
127	198	10	80	43.8	88411	PASS
197	198	0.00	2	0.3	587	PASS
198	198	100	100	100.0	202019	PASS
199	198	5	9	6.5	13095	PASS
275	198	10	60	25.7	51843	PASS
365	198	1	100	3.4	6771	PASS
441	198	0.01	100	17.1	34488	PASS
442	442	50	100	100.0	224200	PASS
443	442	15	24	19.3	43291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032224\
Data File : BF137676.D
Acq On : 22 Mar 2024 11:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 01:05:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

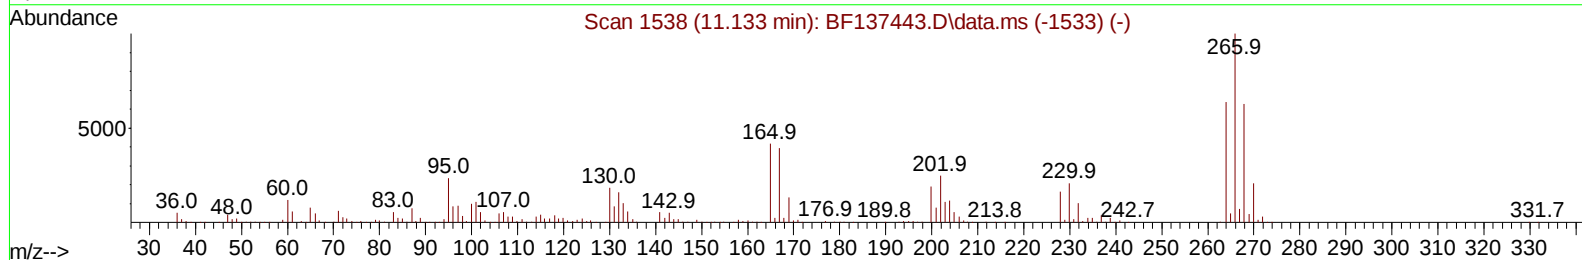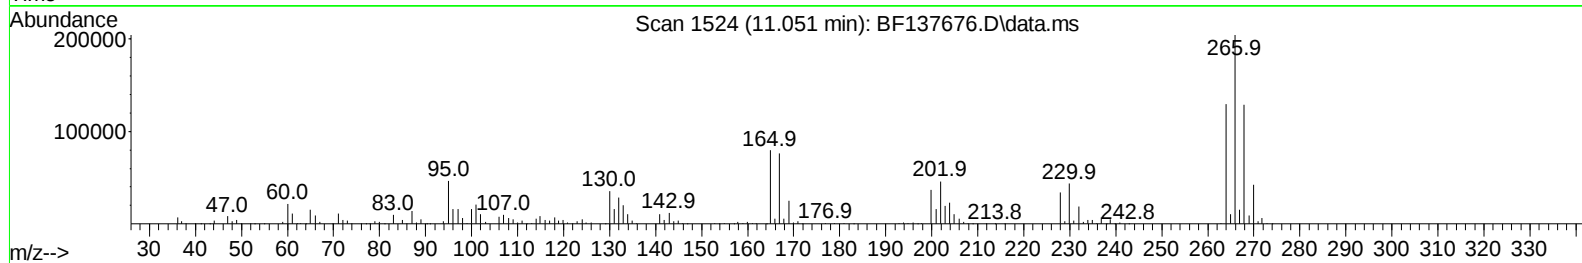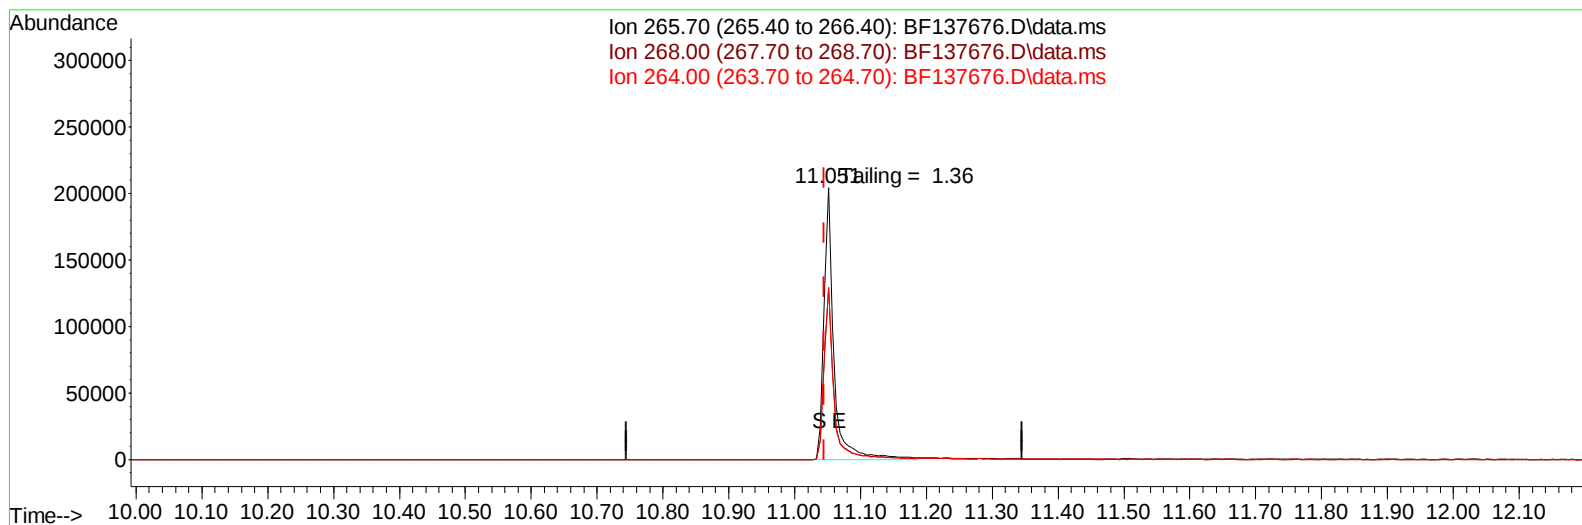

TIC: BF137676.D\data.ms

(70) Pentachlorophenol (C)

11.051min (+ 0.006) 39520.27 ng




response 213409

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.22
264.00	63.60	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032224\
Data File : BF137676.D
Acq On : 22 Mar 2024 11:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 01:05:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

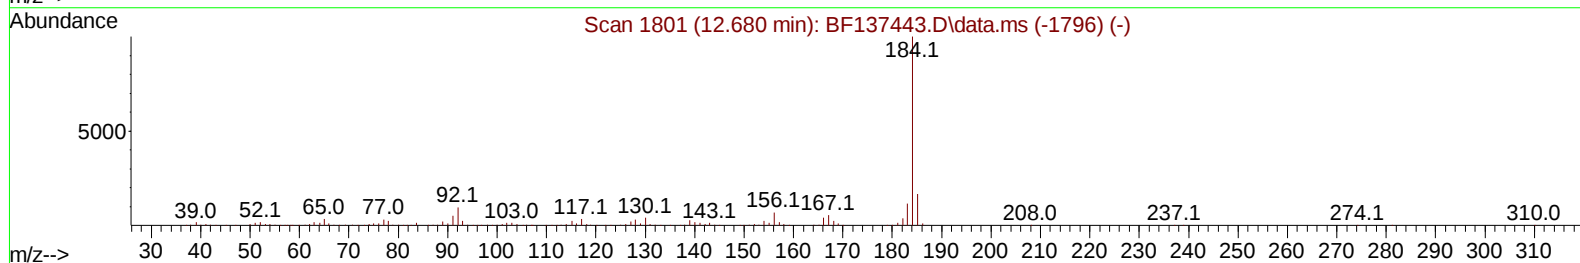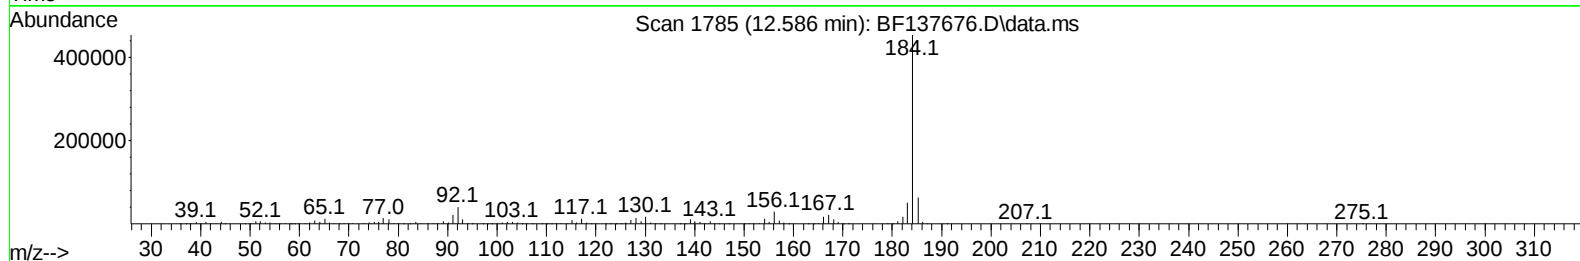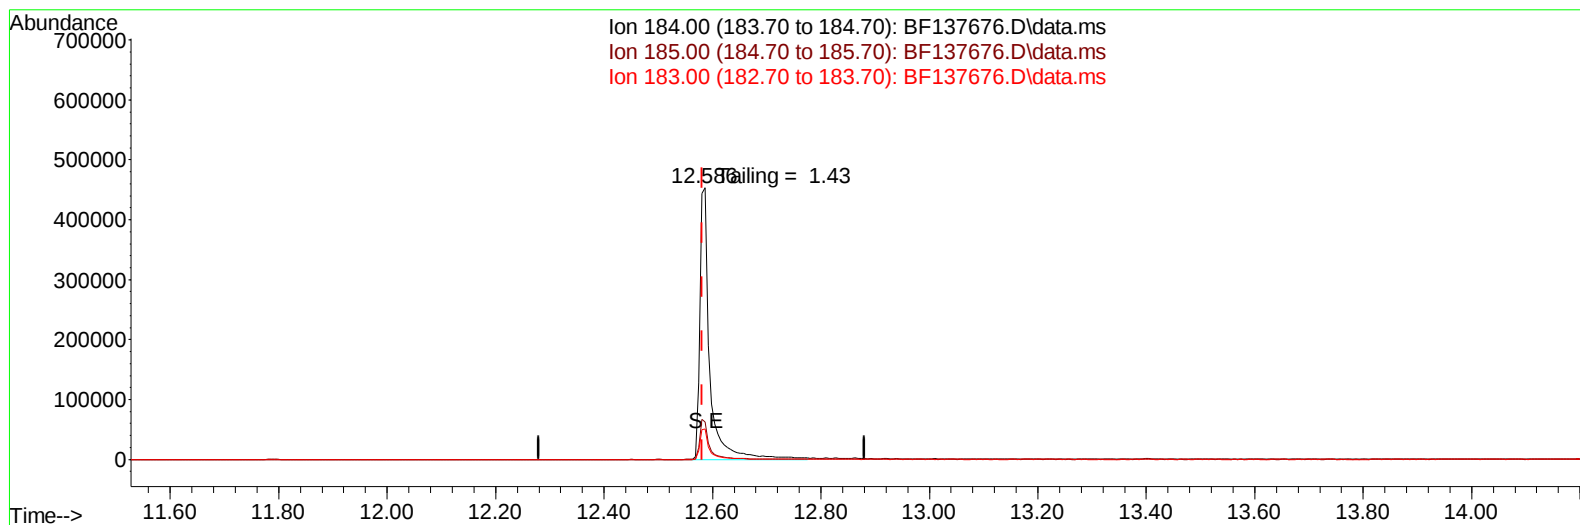

TIC: BF137676.D\data.ms

(77) Benzidine

12.586min (+ 0.006) 302787.40 ng m

response 607611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	13.86
183.00	11.60	11.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2024	BNA_F	<u>BF137676.D</u>
Compound Name	Response	Retention Time
DDT	272320	13.398
DDD	66423	13.104
DDE	439	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66862	339182	19.71

Instrument :
BNA_F
ClientSampleId :
DFTPP