


Data Path : Z:\HPCHEM1\BNA_F\Data\BF032315\
 Data File : BF077891.D
 Acq On : 23 Mar 2015 11:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 02:09:19 2015

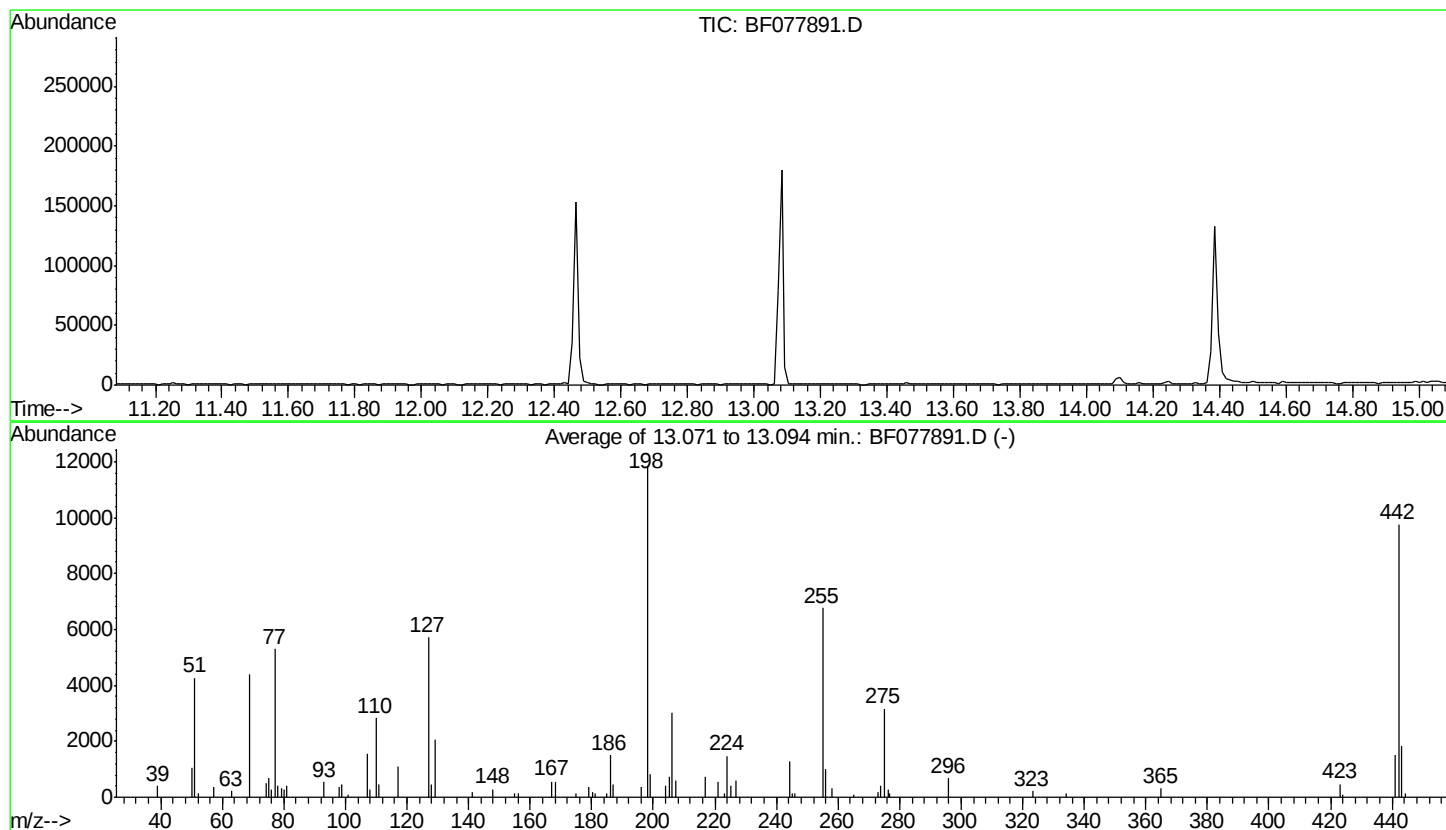

AutoFind: Scans 1066, 1067, 1068; Background Corrected with Scan 1063

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	4274	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.2	4406	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	5706	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11856	PASS
199	198	5	9	7.1	840	PASS
275	198	10	60	26.8	3175	PASS
365	198	1	100	2.5	301	PASS
441	442	0.01	24	15.5	1514	PASS
442	198	50	100	82.2	9745	PASS
443	442	15	24	19.0	1853	PASS