
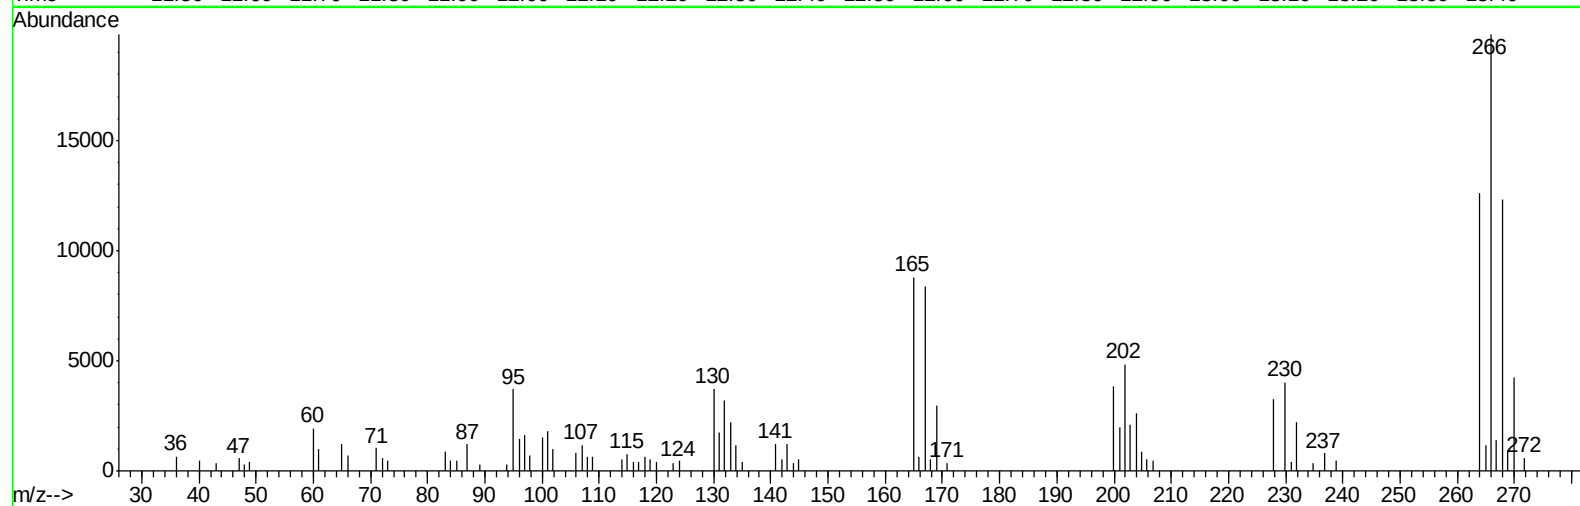


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032315\
Data File : BF077891.D
Acq On : 23 Mar 2015 11:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 02:58:36 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 24 02:23:28 2015
Response via : Initial Calibration

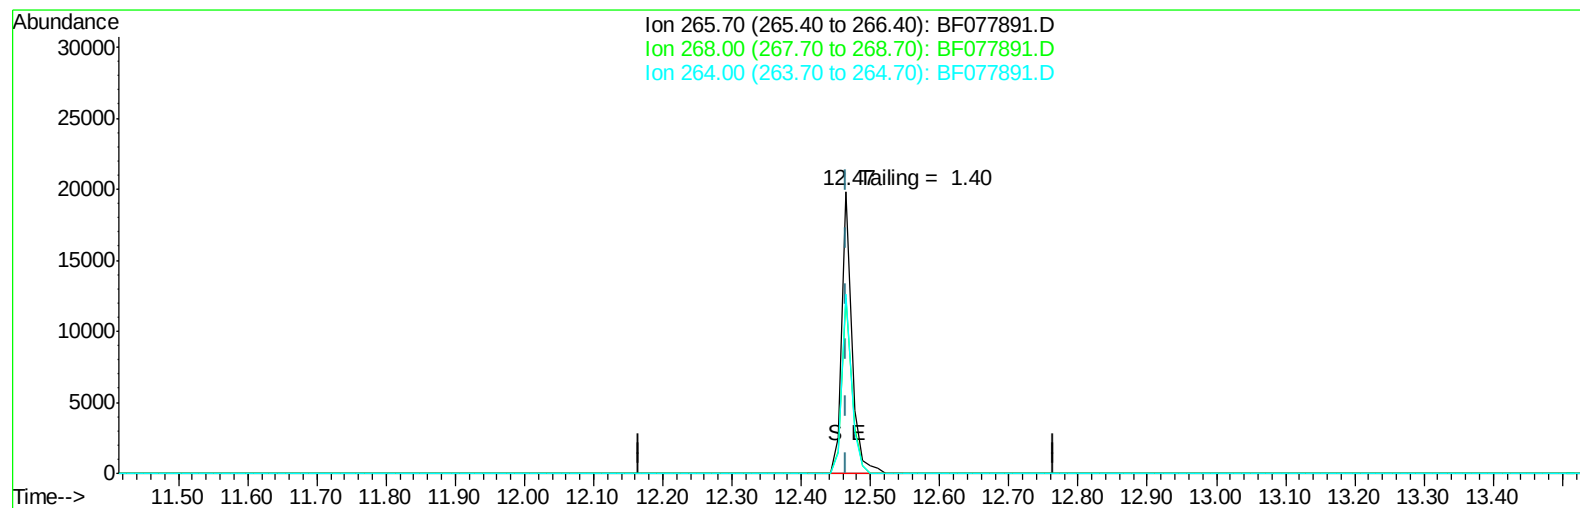

TIC: BF077891.D

(69) Pentachlorophenol (C)



12.465min (+0.000) 0.00ng

response 19653

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.30
264.00	61.20	63.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032315\
Data File : BF077891.D
Acq On : 23 Mar 2015 11:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 02:58:36 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 24 02:23:28 2015
Response via : Initial Calibration

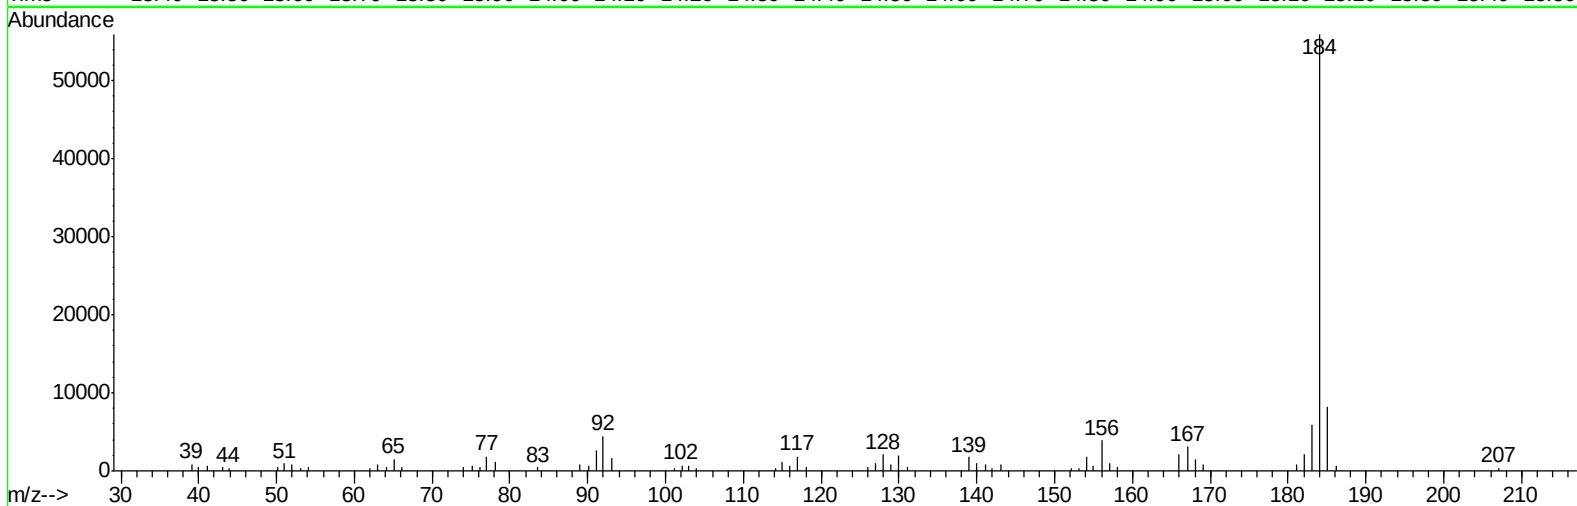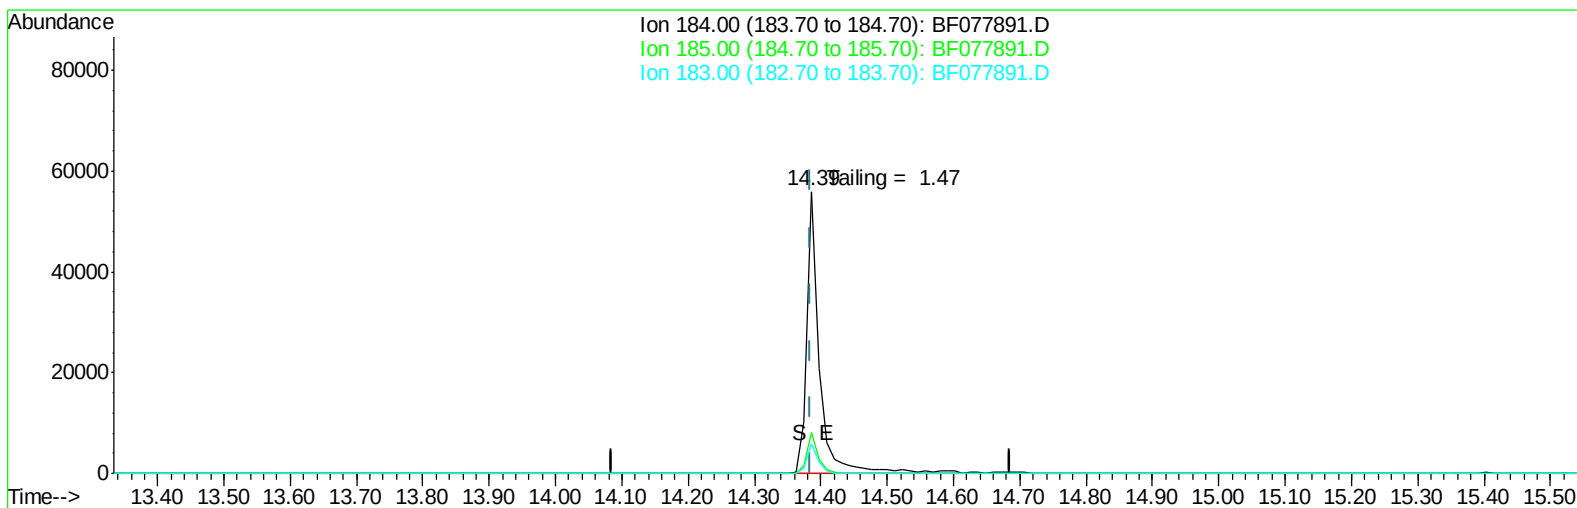

TIC: BF077891.D

(76) Benzidine

14.385min (+0.000) 0.00ng

response 73123

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.62
183.00	11.10	10.60
0.00	0.00	0.00