


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032317\
 Data File : BF093876.D
 Acq On : 23 Mar 2017 13:45
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 23 02:02:22 2017

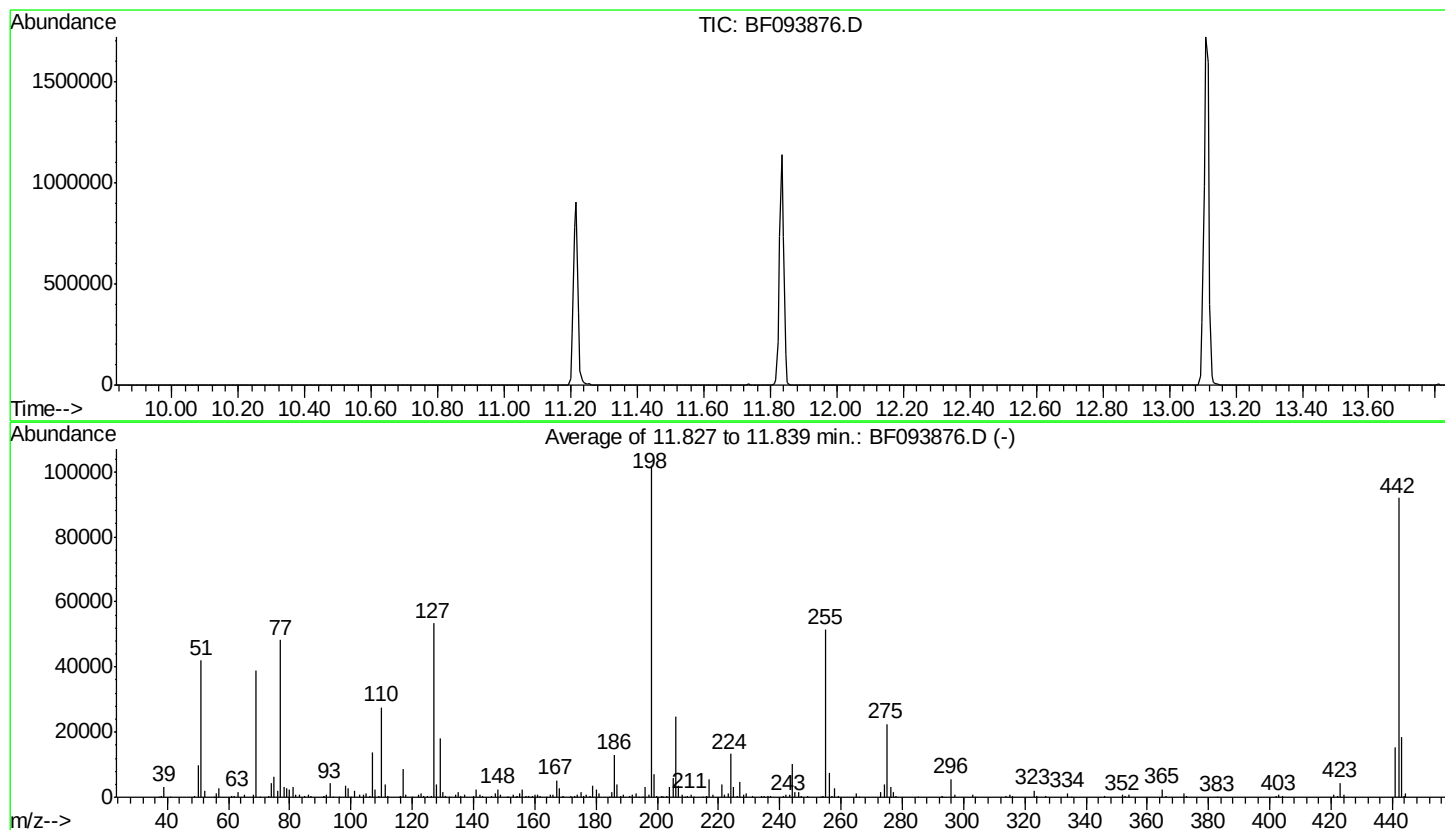

AutoFind: Scans 1690, 1691, 1692; Background Corrected with Scan 1684

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	42002	PASS
68	69	0.00	2	2.0	769	PASS
69	198	0.00	100	38.1	38786	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	52.4	53402	PASS
197	198	0.00	2	0.7	698	PASS
198	198	100	100	100.0	101877	PASS
199	198	5	9	7.0	7182	PASS
275	198	10	60	22.1	22546	PASS
365	198	1	100	2.5	2513	PASS
441	442	0.01	24	16.8	15438	PASS
442	198	50	100	90.2	91861	PASS
443	442	15	24	19.9	18304	PASS