

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF032318\
 Data File : BF103900.D
 Acq On : 24 Mar 2018 00:56
 Operator : JU/SJ
 Sample : J2012-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :


Quant Time: Mar 24 03:13:36 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 23 13:26:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	127499	20.00	ng	0.00
21) Naphthalene-d8	8.26	136	473048	20.00	ng	0.00
38) Acenaphthene-d10	10.02	164	200136	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	307324	20.00	ng	0.00
75) Chrysene-d12	14.16	240	246672	20.00	ng	0.00
86) Perylene-d12	15.71	264	186061	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.60	112	351778	41.97	ng	0.00
7) Phenol-d6	6.59	99	277593	27.07	ng	-0.01
23) Nitrobenzene-d5	7.54	82	765921	112.91	ng	0.00
41) 2,4,6-Tribromophenol	10.81	330	172088	100.01	ng	0.00
44) 2-Fluorobiphenyl	9.33	172	1314346	104.76	ng	0.00
78) Terphenyl-d14	13.10	244	1000565	94.15	ng	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	7.54	70	98488	14.985	ng	# 73
25) Isophorone	7.54	82	765909	48.774	ng	# 64
47) 2-Nitroaniline	9.33	65	1918	7.289	ng	# 1
50) 2,6-Dinitrotoluene	10.02	165	25764	11.982	ng	# 25
52) 3-Nitroaniline	10.22	138	107	3.842	ng	# 2
55) 4-Nitrophenol	10.22	139	4563	6.501	ng	# 9
56) 2,4-Dinitrotoluene	10.02	165	25765	12.207	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.81	198	116	8.229	ng	# 1
66) 4-Bromophenyl-phenylether	10.81	248	10176	3.225	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

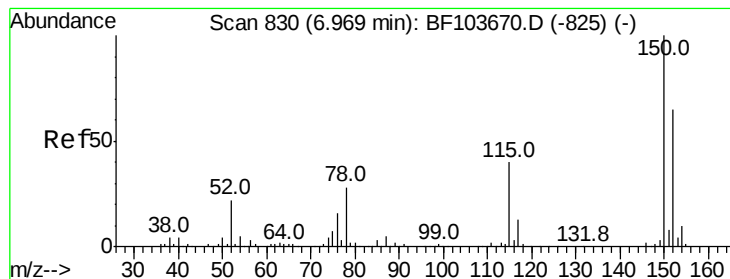


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 831
Delta R.T. -0.00 min
Lab File: BF103900.D
Acq: 24 Mar 2018 00:56

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 127499
Ion Ratio Lower Upper
152 100
150 157.5 124.6 186.8
115 61.5 50.1 75.1

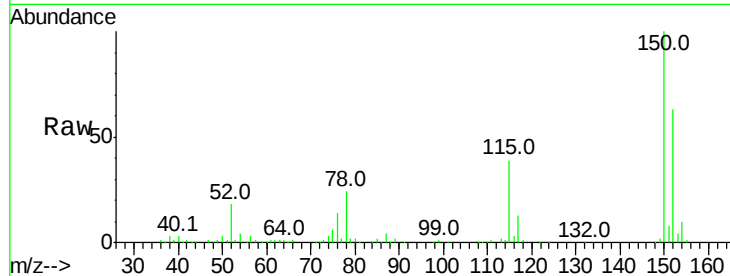


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

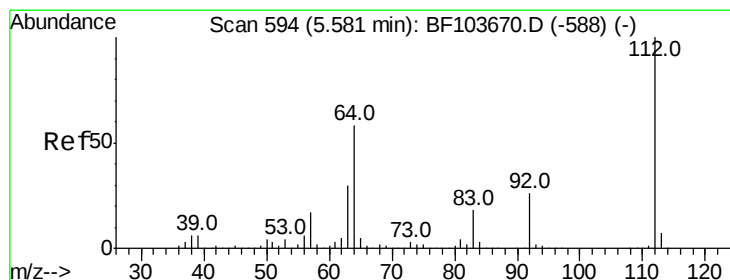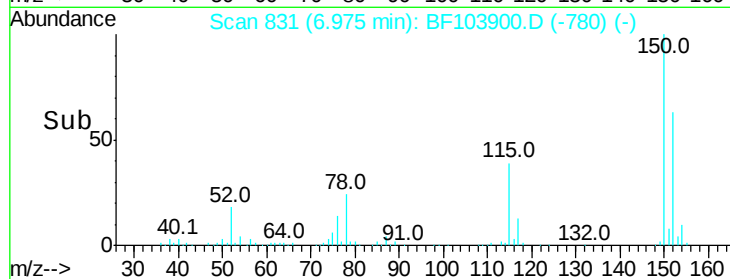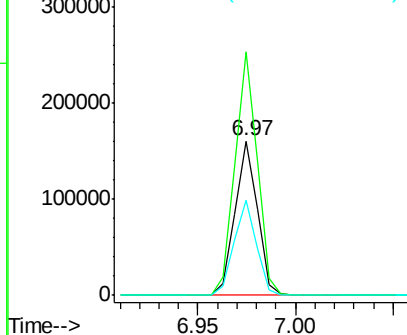



#5


2-Fluorophenol
Concen: 41.965 ng
RT: 5.60 min Scan# 597
Delta R.T. 0.01 min
Lab File: BF103900.D
Acq: 24 Mar 2018 00:56

Tgt Ion:112 Resp: 351778
Ion Ratio Lower Upper
112 100
64 52.1 47.9 71.9
63 25.1 23.7 35.5

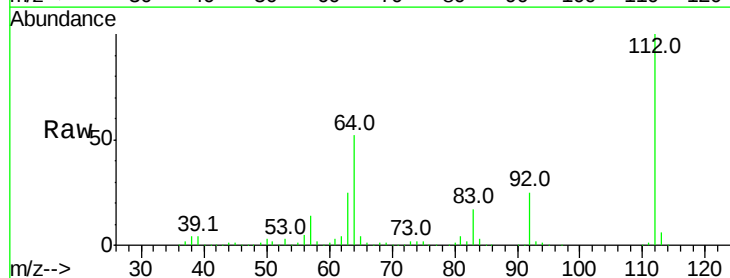

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

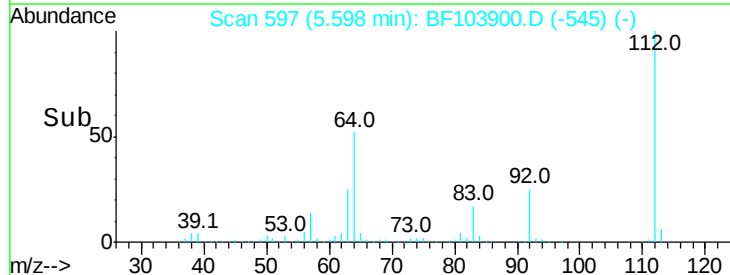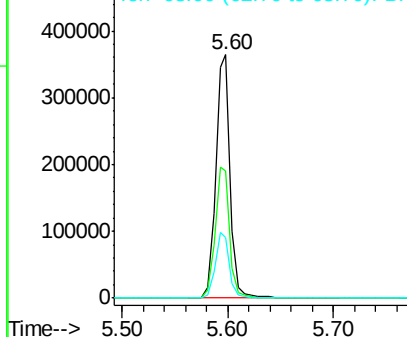

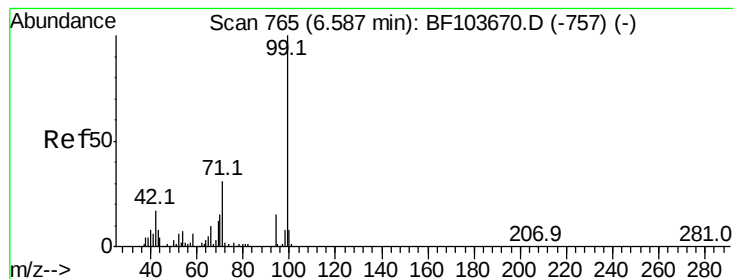

#7

Phenol-d6

Concen: 27.068 ng

RT: 6.59 min Scan# 765

Delta R.T. -0.01 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 277593

Ion Ratio Lower Upper

99 100

42 16.0 14.5 21.7

71 31.4 25.4 38.0

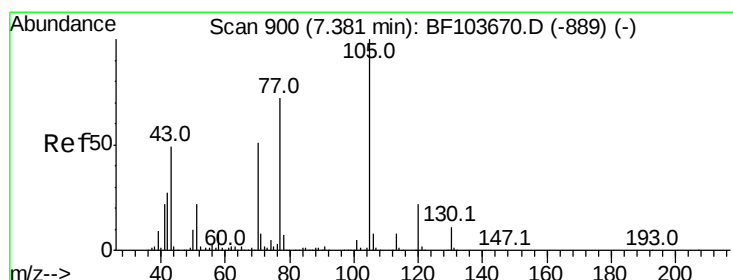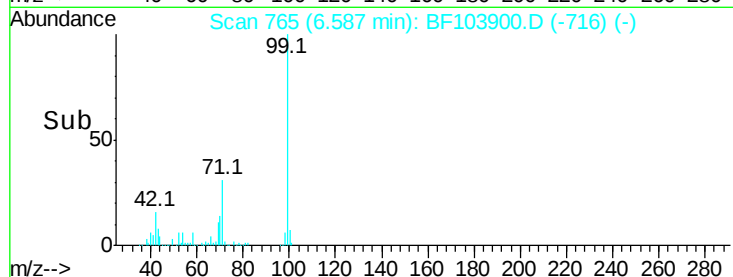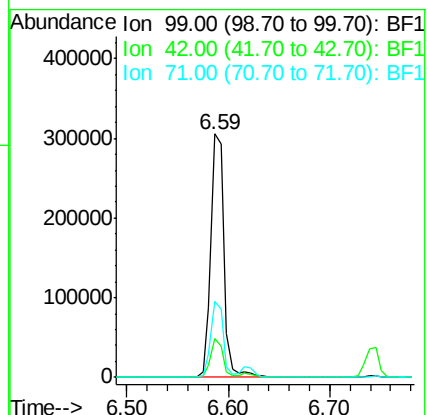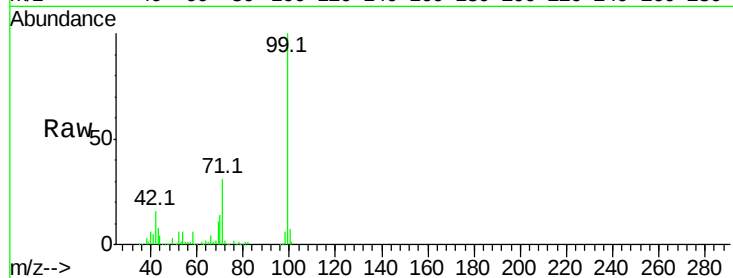

#19

n-Nitroso-di-n-propylamine

Concen: 14.985 ng

RT: 7.54 min Scan# 927

Delta R.T. 0.15 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56

Tgt Ion: 70 Resp: 98488




Ion Ratio Lower Upper


70 100

42 42.1 47.5 71.3#

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#

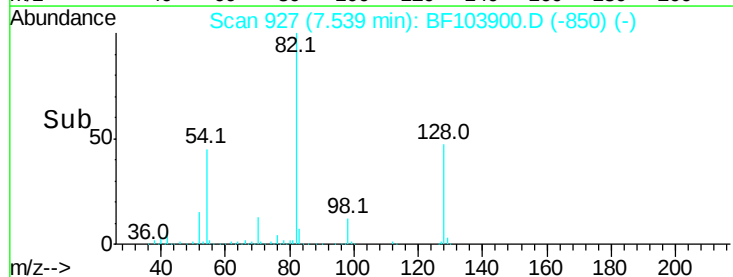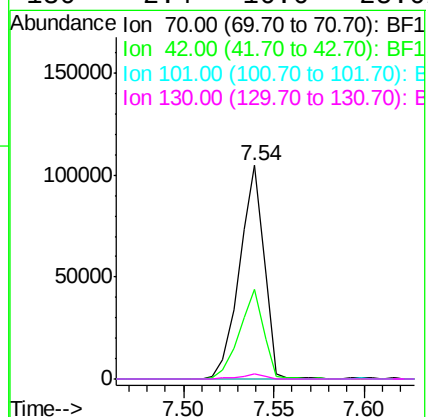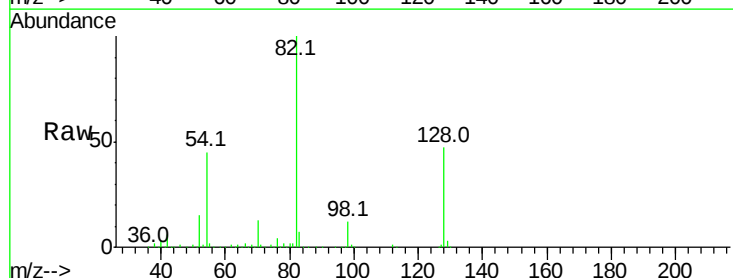


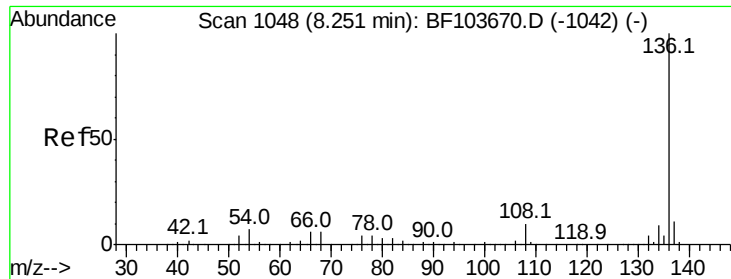




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.26 min Scan# 1049
Delta R.T. -0.00 min
Lab File: BF103900.D
Acq: 24 Mar 2018 00:56

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	473048
Ion	Ratio	Lower	Upper
136	100		
137	11.4	8.9	13.3
54	6.9	6.6	9.8
68	6.0	5.0	7.4

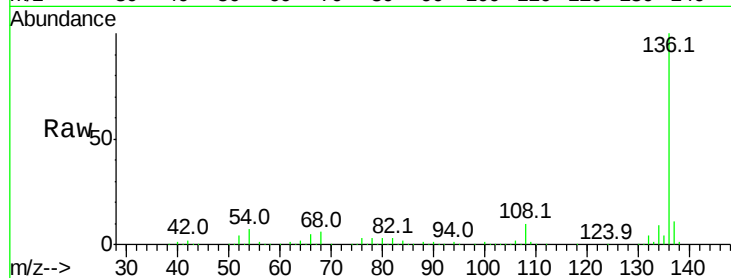


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

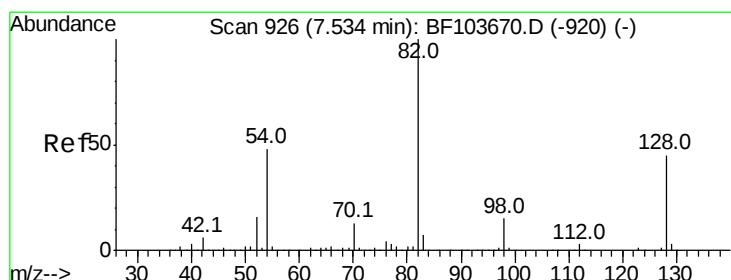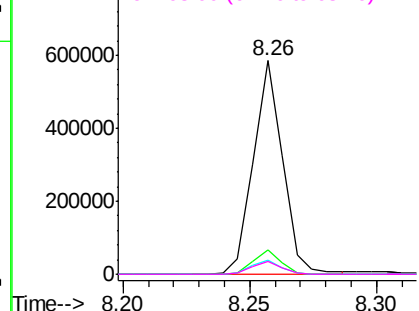
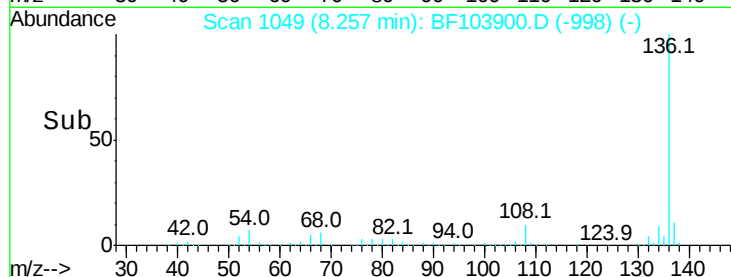



#23
Nitrobenzene-d5
Concen: 112.911 ng
RT: 7.54 min Scan# 927
Delta R.T. -0.00 min
Lab File: BF103900.D
Acq: 24 Mar 2018 00:56

Tgt Ion:	82	Resp:	765921
Ion	Ratio	Lower	Upper
82	100		
128	46.8	36.1	54.1
54	44.9	41.4	62.2

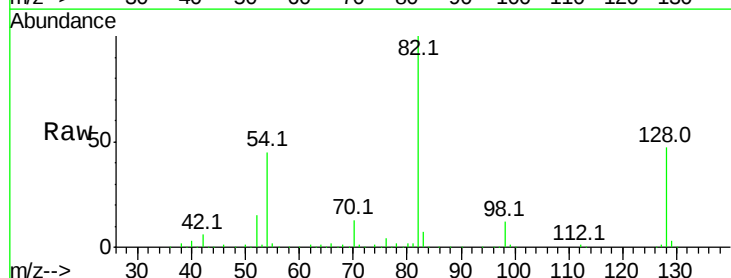

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

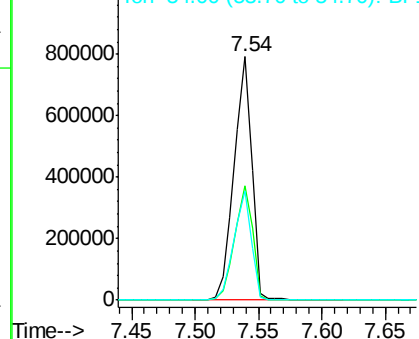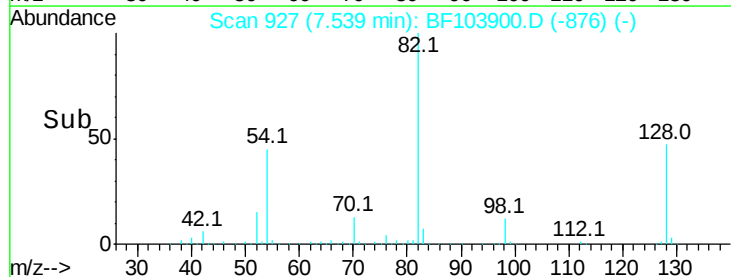

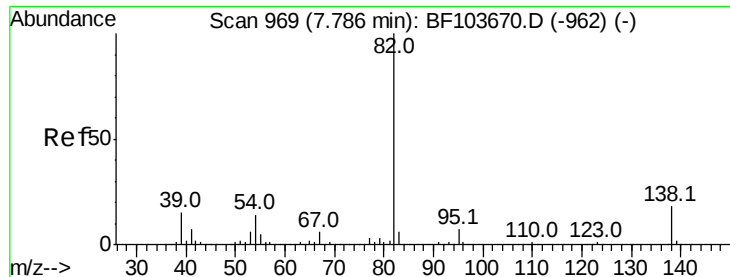

#25

Isophorone

Concen: 48.774 ng

RT: 7.54 min Scan# 927

Delta R.T. -0.25 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 765909

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

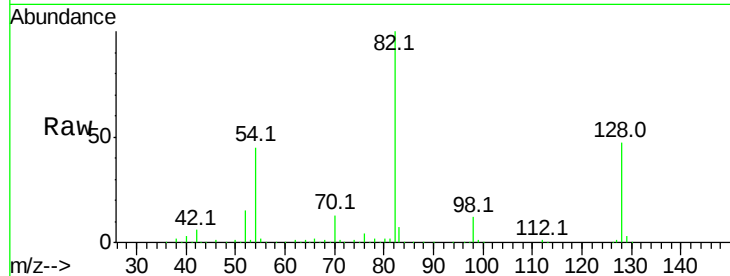

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

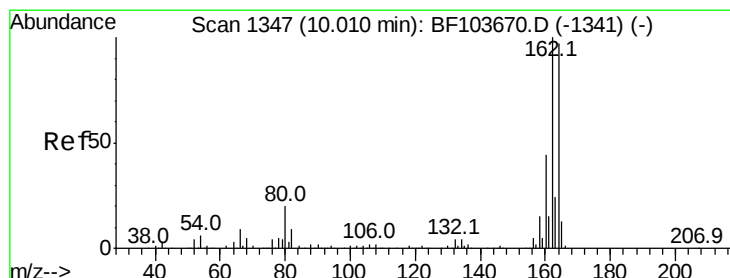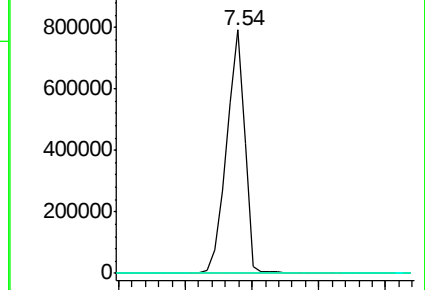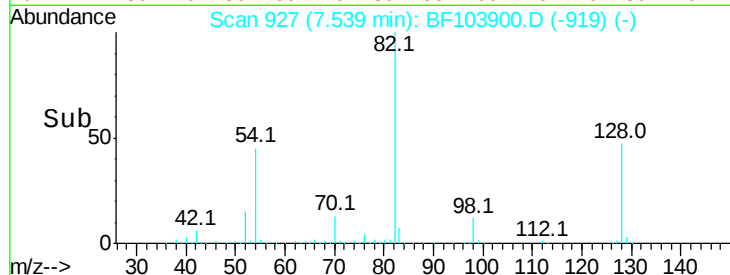

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.02 min Scan# 1348

Delta R.T. -0.01 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56


Tgt Ion:164 Resp: 200136

Ion Ratio Lower Upper

164 100

162 102.7 86.1 129.1



160 45.2 38.3 57.5

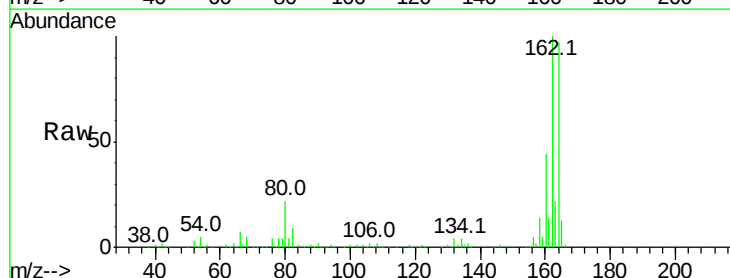


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

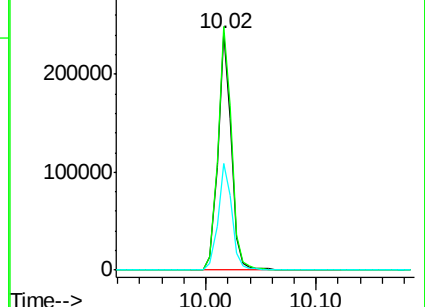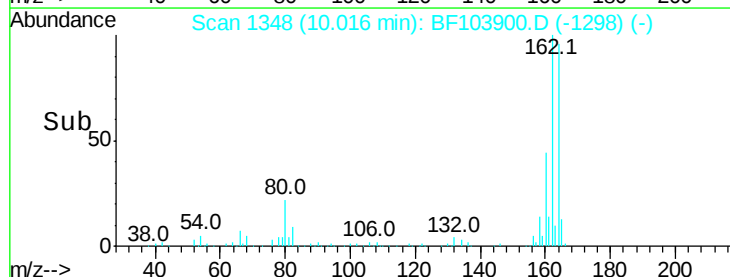


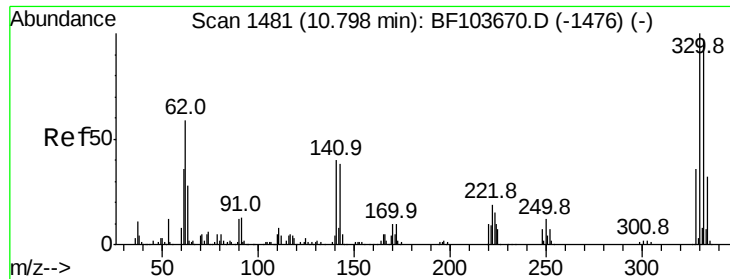




#41
 2,4,6-Tribromophenol
 Concen: 100.006 ng
 RT: 10.81 min Scan# 1483
 Delta R.T. -0.00 min
 Lab File: BF103900.D
 Acq: 24 Mar 2018 00:56

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 172088
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 32.3 29.9 44.9

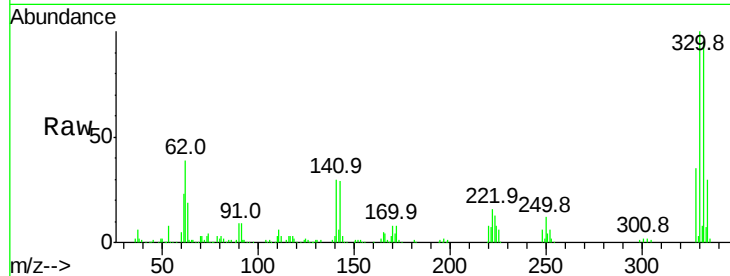


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

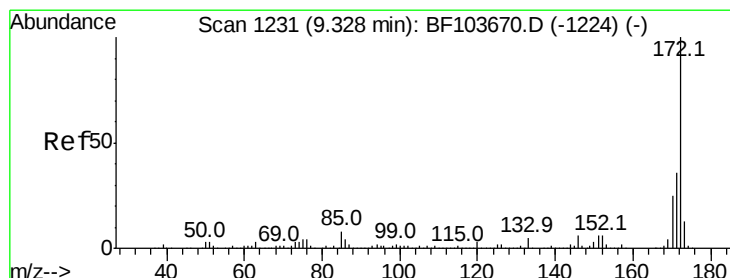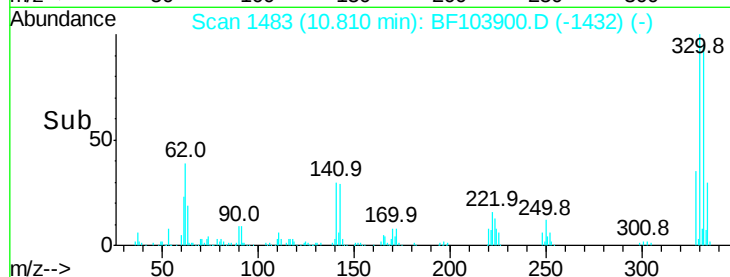
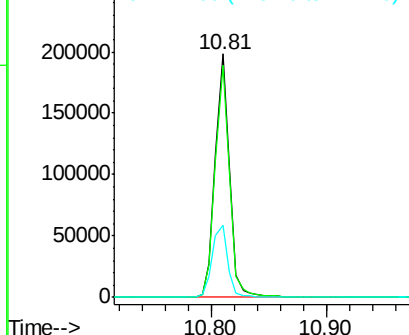



#44
 2-Fluorobiphenyl
 Concen: 104.758 ng
 RT: 9.33 min Scan# 1232
 Delta R.T. -0.00 min
 Lab File: BF103900.D
 Acq: 24 Mar 2018 00:56

Tgt Ion:172 Resp: 1314346
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.7 44.5
 170 24.1 19.6 29.4

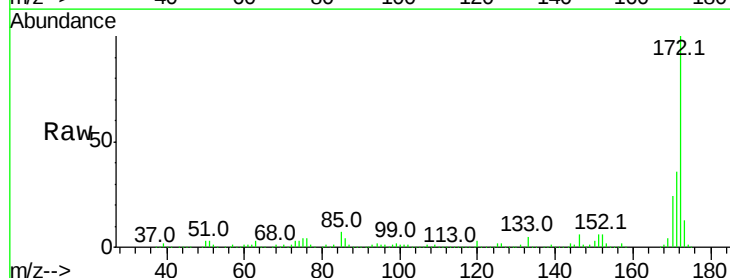

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

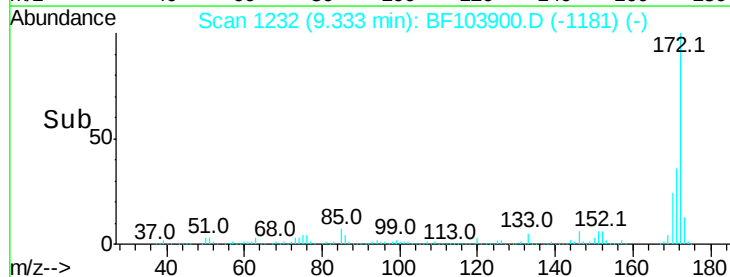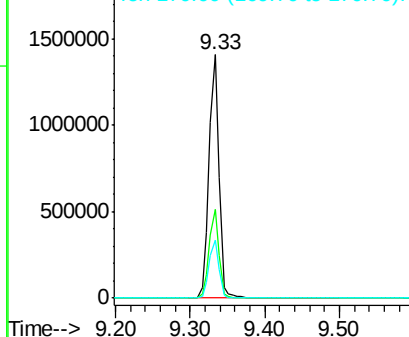

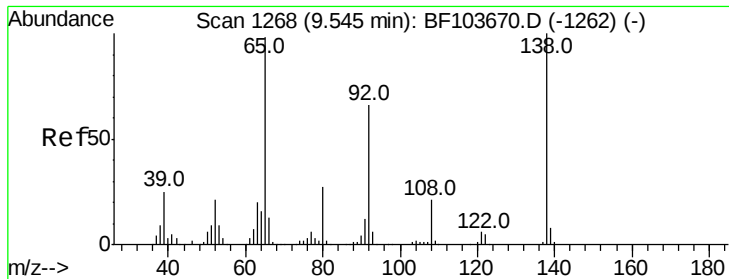

#47

2-Nitroaniline

Concen: 7.289 ng

RT: 9.33 min Scan# 1232

Delta R.T. -0.22 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56

Instrument :

BNA_F

ClientSampled :


Tot Ion: 65 Resp: 1918

Ion Ratio Lower Upper

65 100

92 207.2 55.8 83.6#




138 32.5 91.2 136.8#

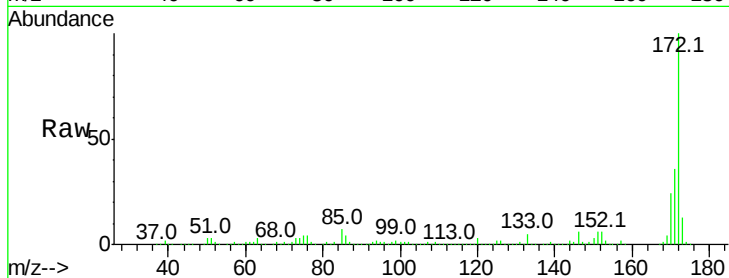

Abundance Ion 65.00 (64.70 to 65.70): BF1

Ion 92.00 (91.70 to 92.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

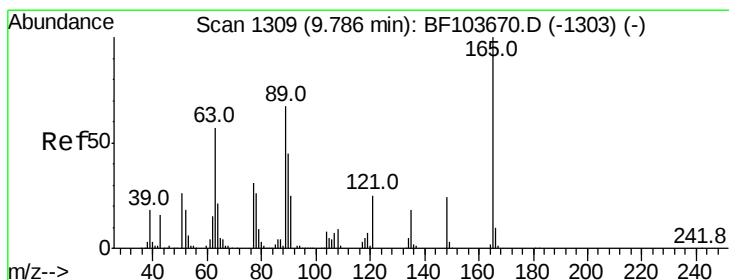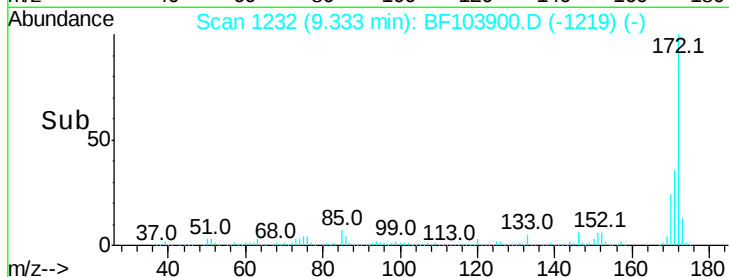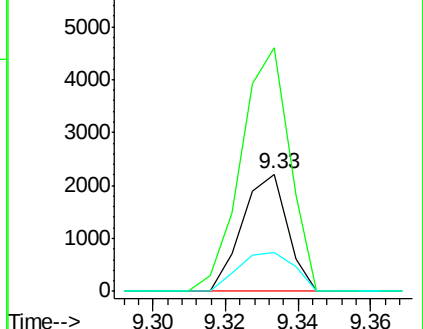

#50

2,6-Dinitrotoluene

Concen: 11.982 ng

RT: 10.02 min Scan# 1348

Delta R.T. 0.22 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56


Tgt Ion:165 Resp: 25764

Ion Ratio Lower Upper

165 100

63 1.0 44.7 67.1#



89 1.1 44.0 66.0#

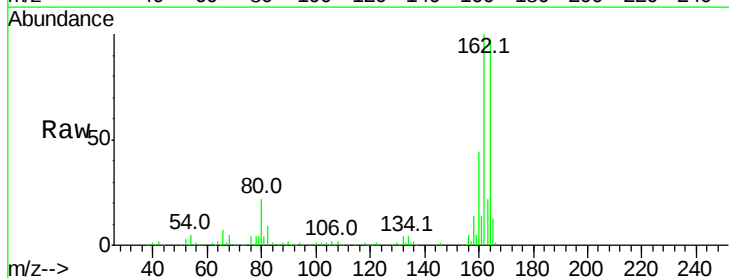


Abundance Ion 165.00 (164.70 to 165.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

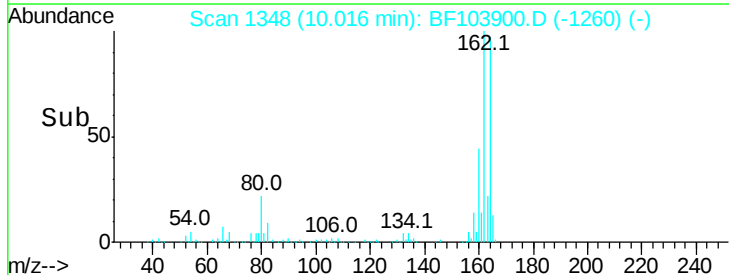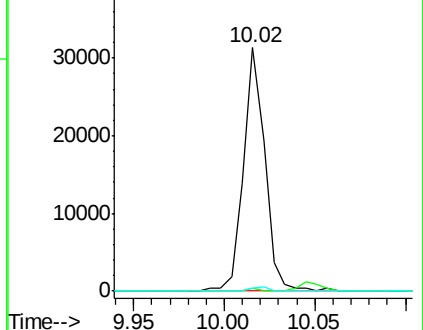


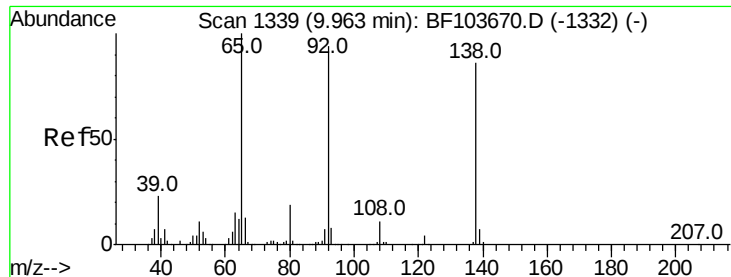


#52
3-Nitroaniline
Concen: 3.842 ng
RT: 10.22 min Scan# 1383
Delta R.T. 0.25 min
Lab File: BF103900.D
Acq: 24 Mar 2018 00:56

Instrument :
BNA_F
ClientSampleId :



Tot Ion:138 Resp: 107
Ion Ratio Lower Upper
138 100
108 0.0 9.4 14.0#
92 0.0 89.4 134.2#

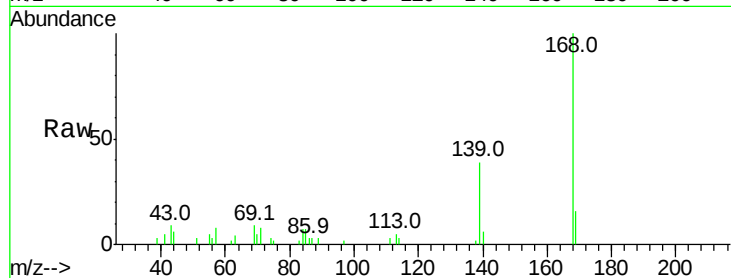

Abundance Ion 138.00 (137.70 to 138.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 92.00 (91.70 to 92.70): BF1

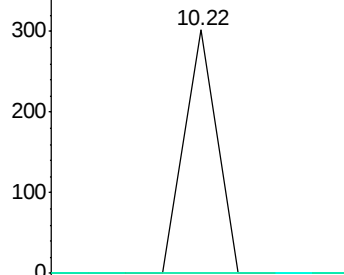


Time-->

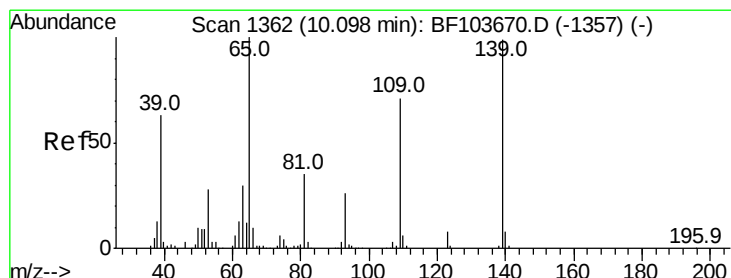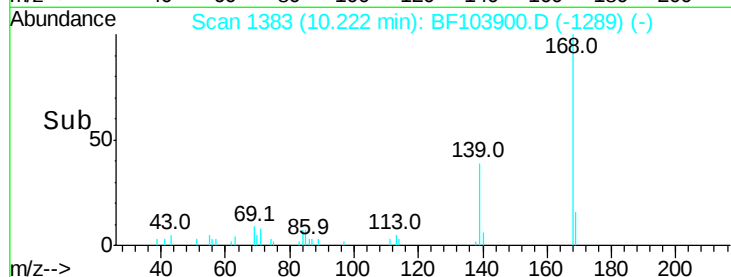


#55
4-Nitrophenol
Concen: 6.501 ng
RT: 10.22 min Scan# 1383
Delta R.T. 0.10 min
Lab File: BF103900.D
Acq: 24 Mar 2018 00:56


Tgt Ion:139 Resp: 4563
Ion Ratio Lower Upper
139 100
109 0.0 48.4 88.4#
65 0.0 72.6 112.6#

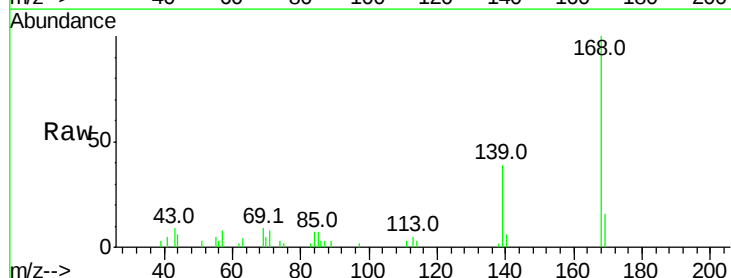


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF1

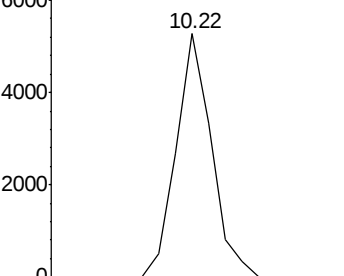

Time-->

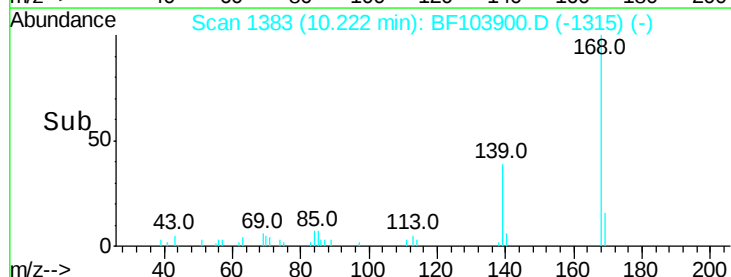


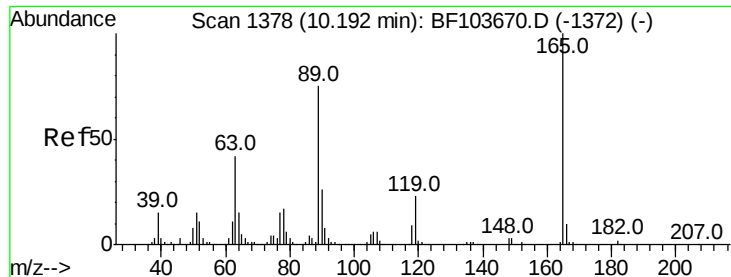




#56
 2,4-Dinitrotoluene
 Concen: 12.207 ng
 RT: 10.02 min Scan# 1348
 Delta R.T. -0.19 min
 Lab File: BF103900.D
 Acq: 24 Mar 2018 00:56

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:165 Resp: 25765
 Ion Ratio Lower Upper
 165 100
 63 1.0 36.4 54.6#
 89 1.1 57.8 86.6#
 182 0.0 1.6 2.4#

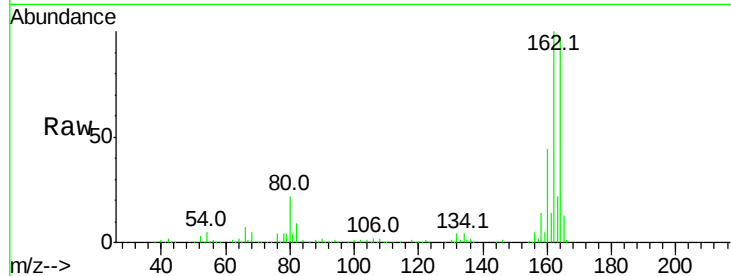


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

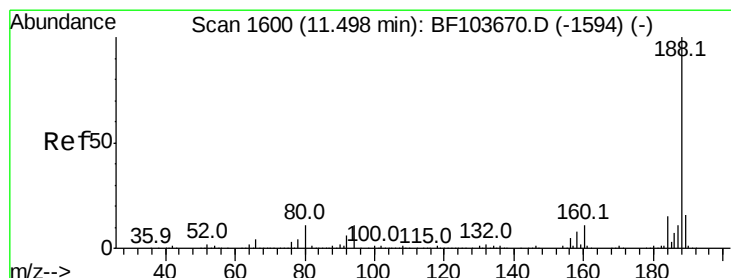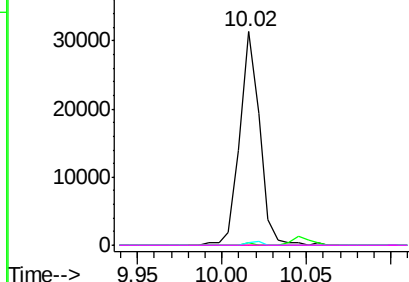
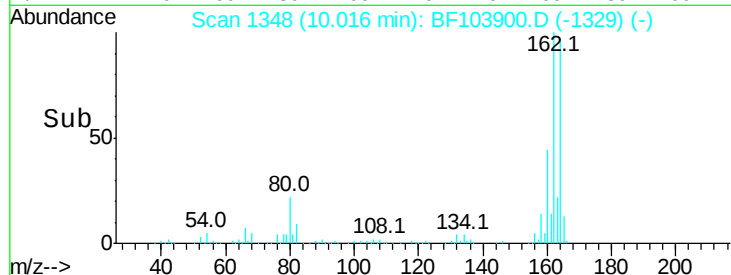



#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.51 min Scan# 1602
 Delta R.T. -0.00 min
 Lab File: BF103900.D
 Acq: 24 Mar 2018 00:56

Tgt Ion:188 Resp: 307324
 Ion Ratio Lower Upper
 188 100
 94 10.8 8.5 12.7
 80 11.1 9.2 13.8

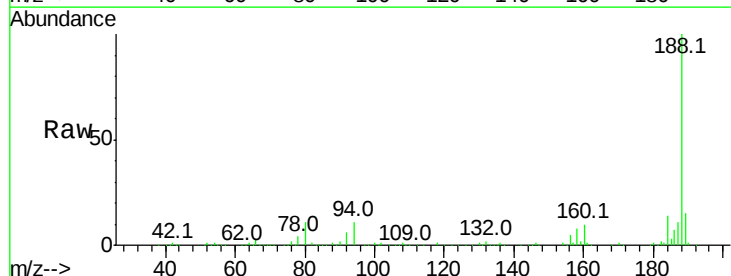

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

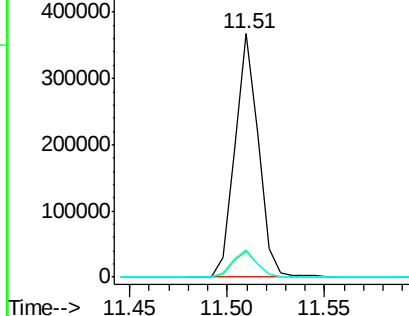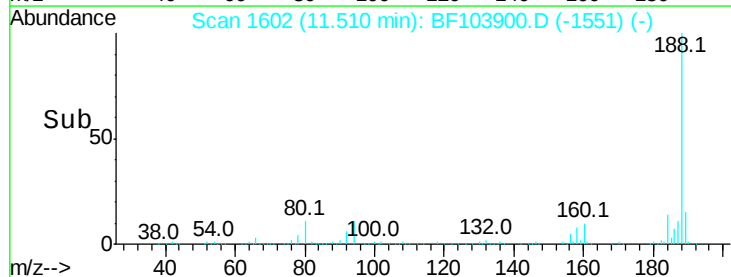

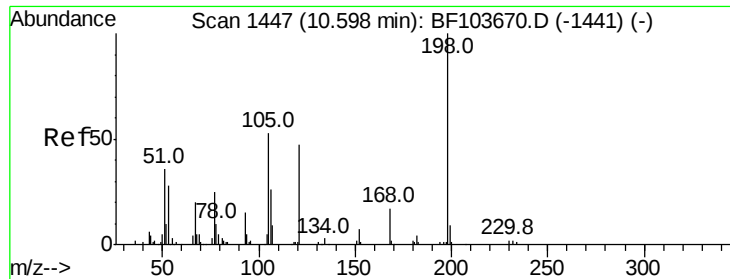

#64

4,6-Dinitro-2-methylphenol

Concen: 8.229 ng

RT: 10.81 min Scan# 1483

Delta R.T. 0.19 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion:198 Resp: 116

Ion Ratio Lower Upper

198 100

51 214.0 37.7 77.7#




105 220.1 36.3 76.3#

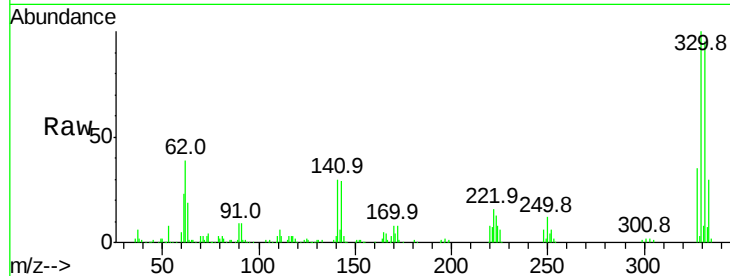

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

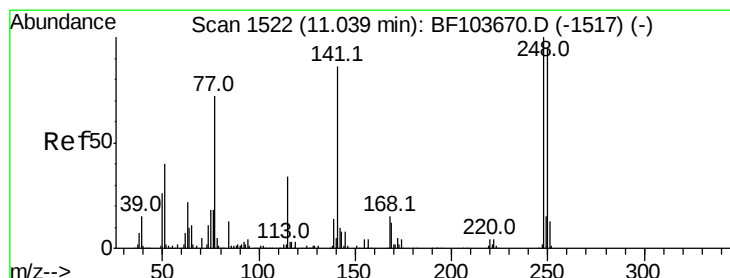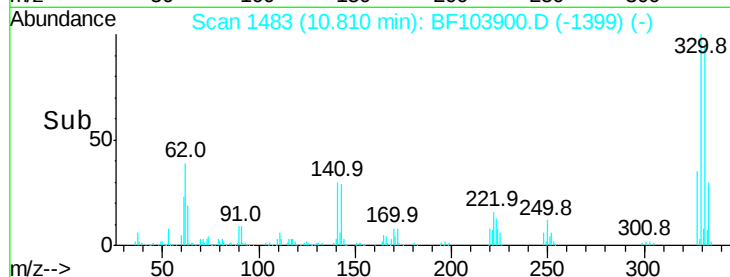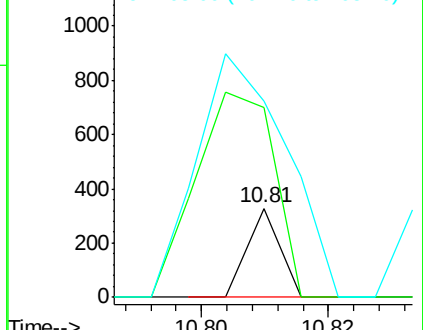

#66

4-Bromophenyl-phenylether

Concen: 3.225 ng

RT: 10.81 min Scan# 1483

Delta R.T. -0.24 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56


Tgt Ion:248 Resp: 10176

Ion Ratio Lower Upper

248 100

250 201.3 76.9 115.3#



141 509.6 74.4 111.6#

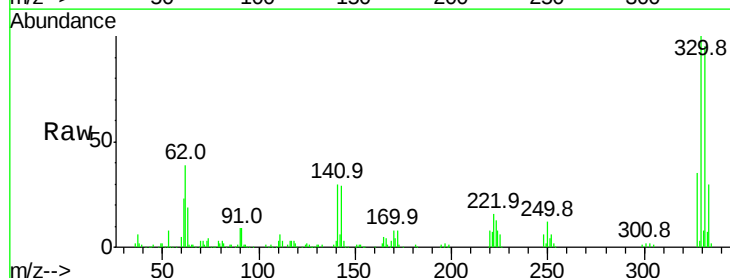


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

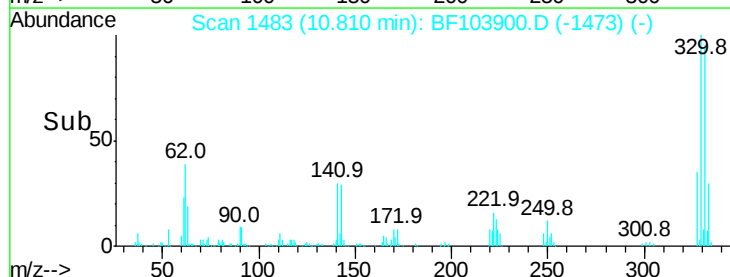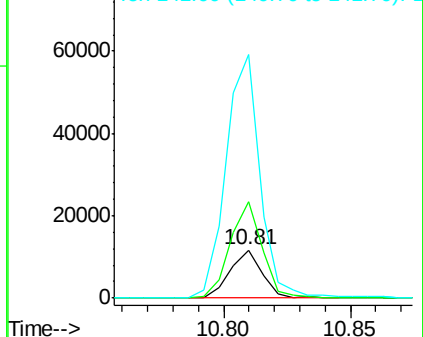

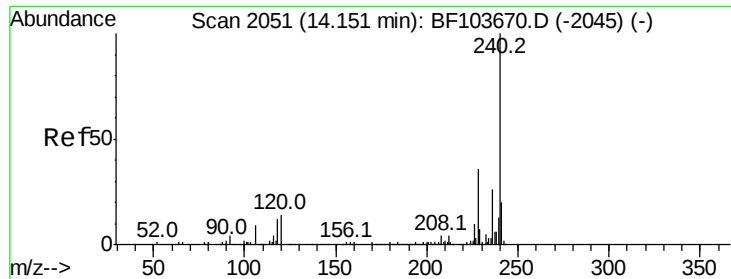

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2053

Delta R.T. -0.01 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 246672

Ion Ratio Lower Upper

240 100

120 13.5 9.5 14.3




236 25.0 20.7 31.1

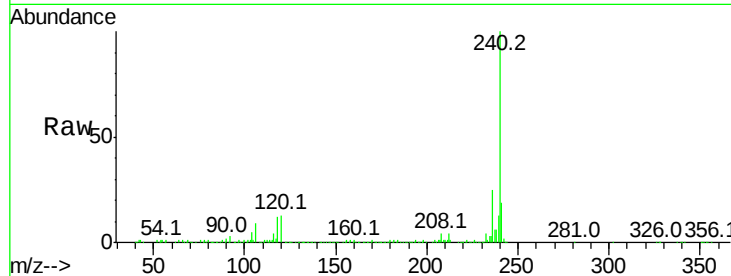

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

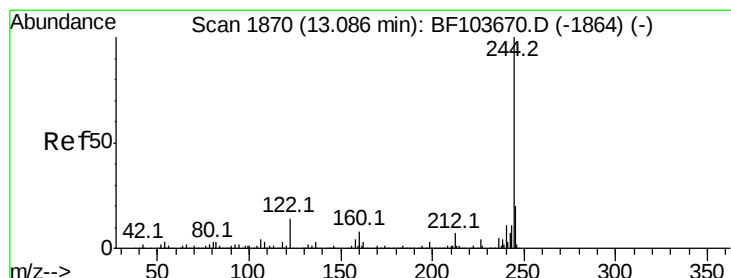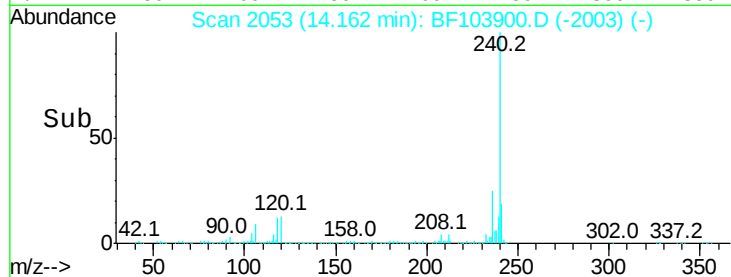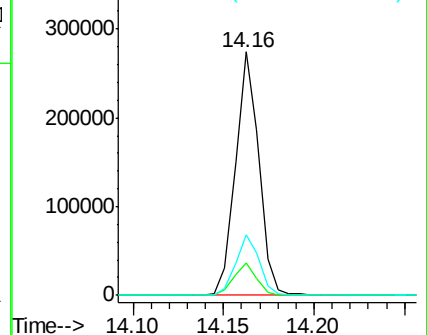

#78

Terphenyl-d14

Concen: 94.152 ng

RT: 13.10 min Scan# 1872

Delta R.T. -0.00 min

Lab File: BF103900.D

Acq: 24 Mar 2018 00:56


Tgt Ion:244 Resp: 1000565

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0



122 13.2 11.0 16.4



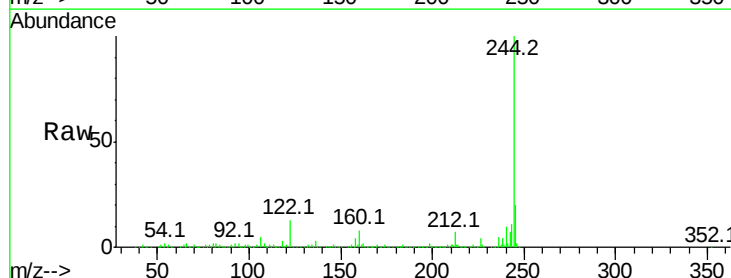


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

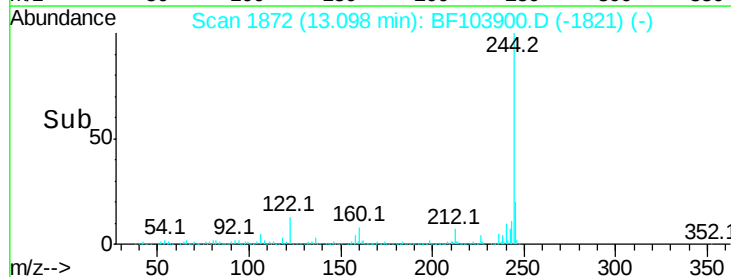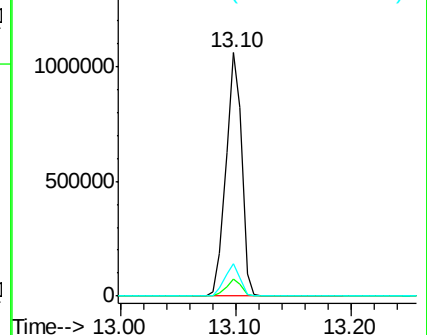

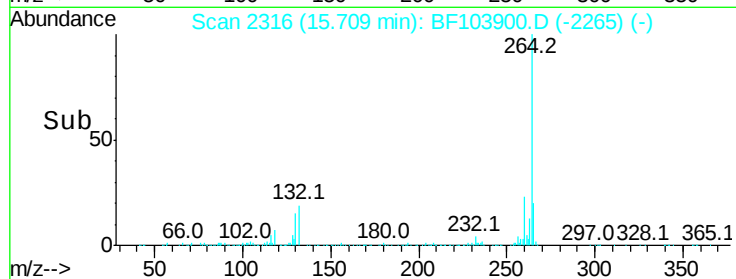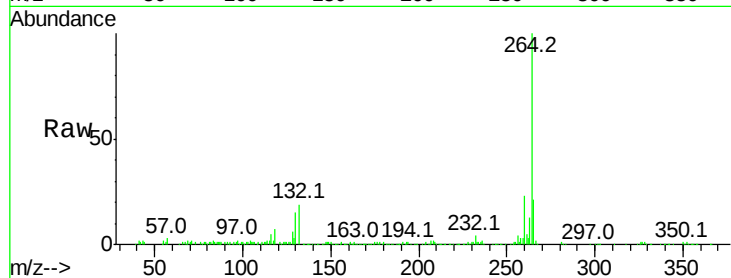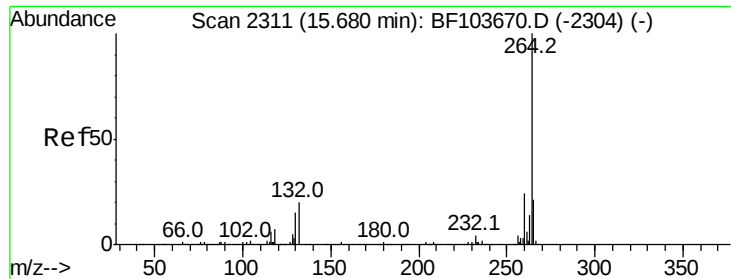

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.71 min Scan# 2316
 Delta R.T. -0.00 min
 Lab File: BF103900.D
 Acq: 24 Mar 2018 00:56

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.2	28.8
265	20.8	17.5	26.3

