


Data Path : Z:\HPCHEM1\BNA F\Data\BF032318\
 Data File : BF103865.D
 Acq On : 23 Mar 2018 8:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 13:26:17 2018

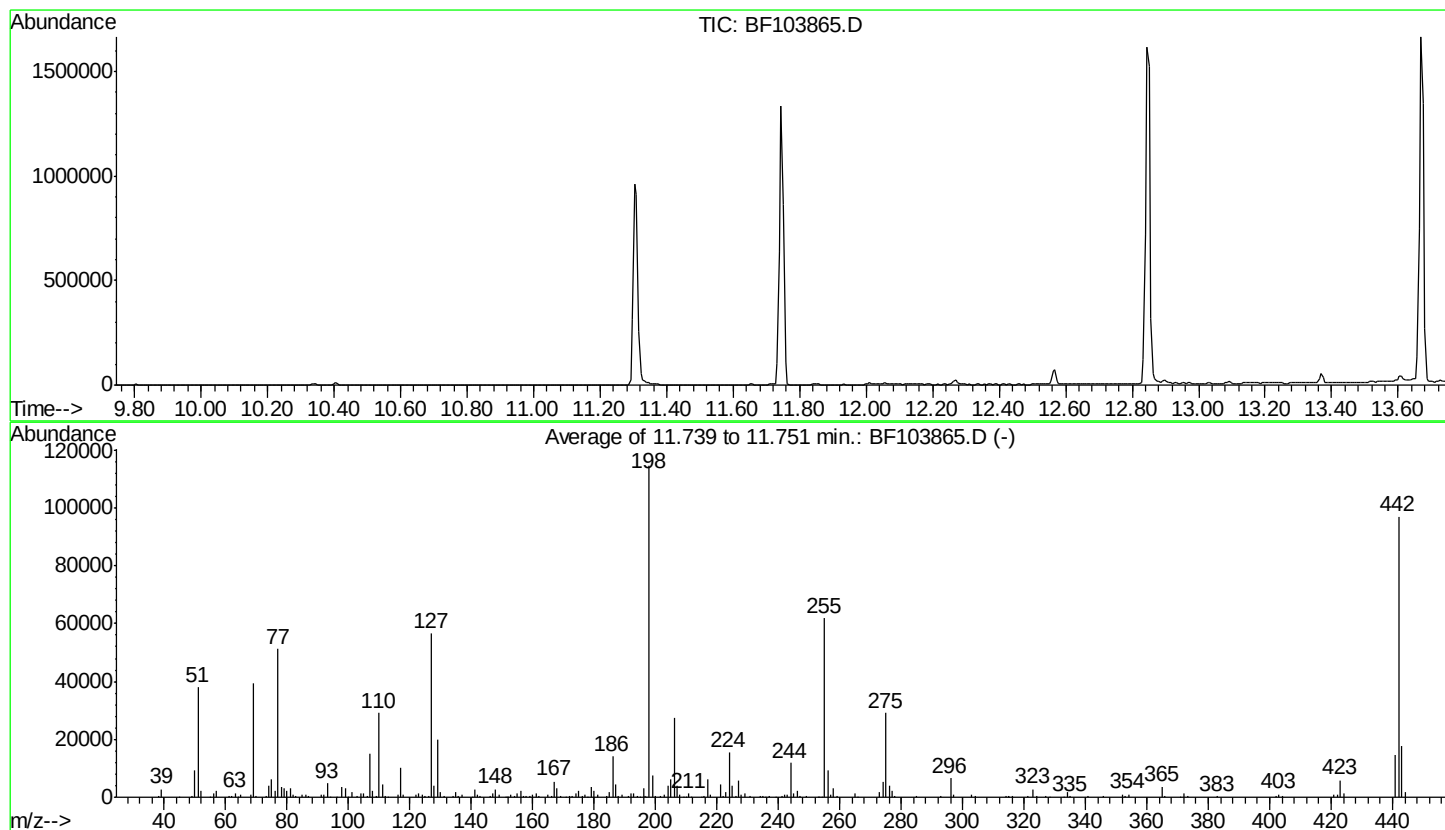

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	37984	PASS
68	69	0.00	2	2.0	798	PASS
69	198	0.00	100	34.4	39367	PASS
70	69	0.00	2	0.6	237	PASS
127	198	10	80	49.4	56610	PASS
197	198	0.00	2	0.3	358	PASS
198	198	100	100	100.0	114586	PASS
199	198	5	9	6.6	7556	PASS
275	198	10	60	25.5	29181	PASS
365	198	1	100	3.3	3733	PASS
441	443	0.01	100	83.4	14821	PASS
442	198	50	100	84.6	96930	PASS
443	442	15	24	18.3	17769	PASS