


Data Path : Z:\HPCHEM1\BNA F\Data\BF032318\
Data File : BF103892.D
Acq On : 23 Mar 2018 21:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 23 13:26:17 2018

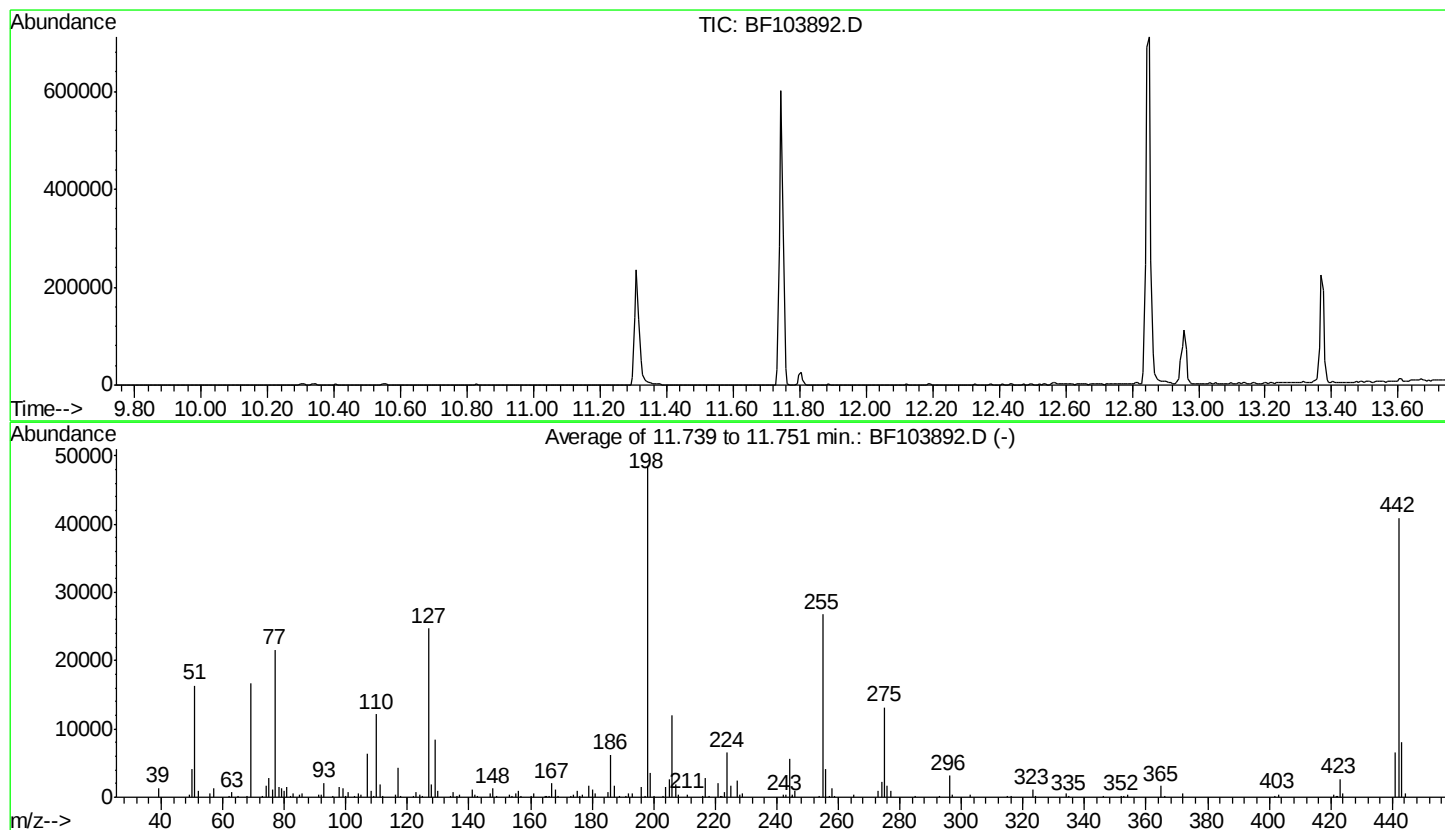

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	16396	PASS
68	69	0.00	2	0.9	156	PASS
69	198	0.00	100	34.4	16705	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	24697	PASS
197	198	0.00	2	0.4	205	PASS
198	198	100	100	100.0	48552	PASS
199	198	5	9	7.2	3488	PASS
275	198	10	60	27.2	13200	PASS
365	198	1	100	3.4	1654	PASS
441	443	0.01	100	81.0	6567	PASS
442	198	50	100	84.2	40875	PASS
443	442	15	24	19.8	8106	PASS