


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032319\
 Data File : BF113253.D
 Acq On : 23 Mar 2019 10:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

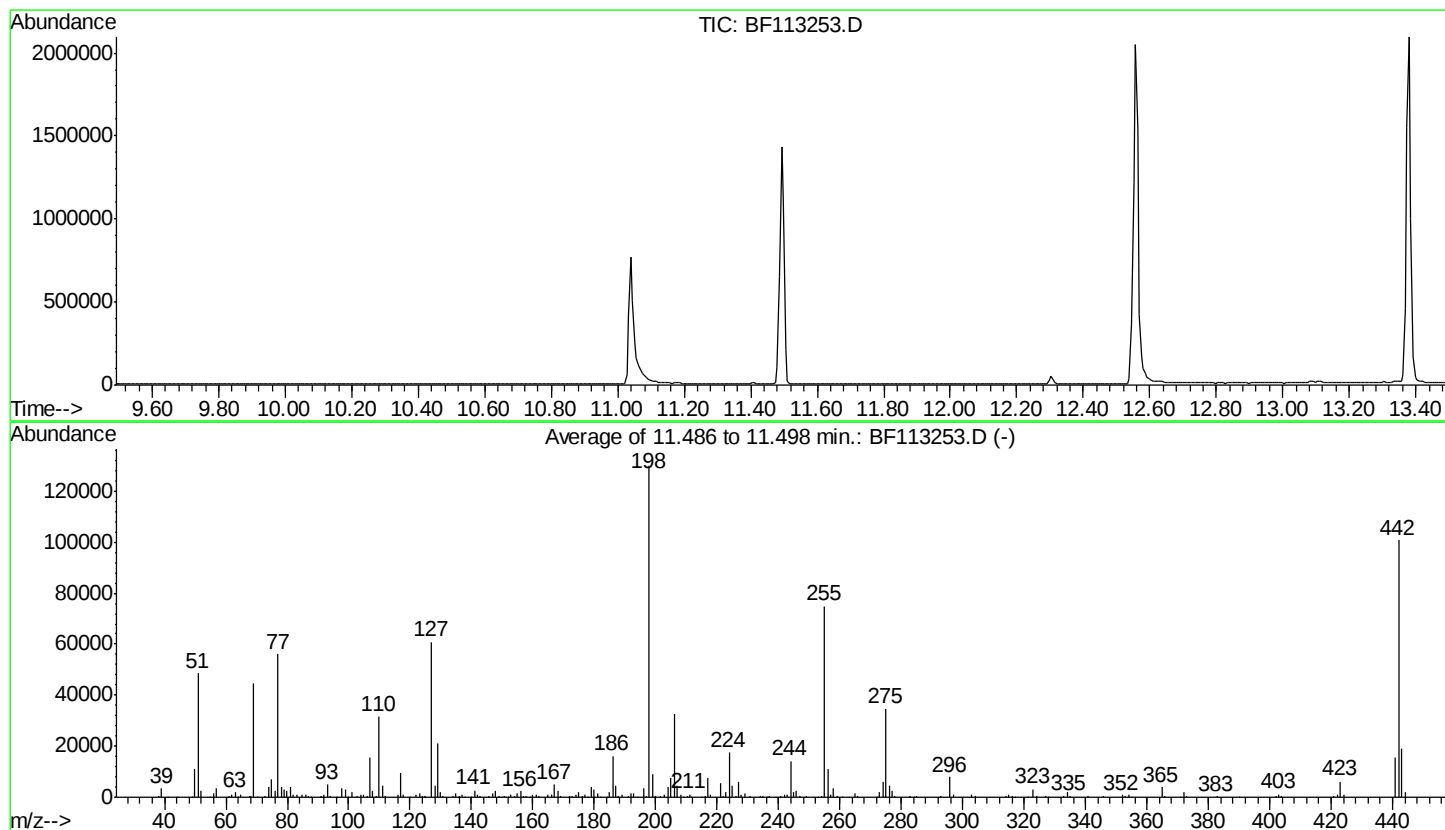

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	48530	PASS
68	69	0.00	2	0.8	366	PASS
69	198	0.00	100	34.5	44890	PASS
70	69	0.00	2	0.3	143	PASS
127	198	10	80	46.7	60752	PASS
197	198	0.00	2	0.5	682	PASS
198	198	100	100	100.0	129994	PASS
199	198	5	9	6.9	8908	PASS
275	198	10	60	26.8	34781	PASS
365	198	1	100	3.1	3992	PASS
441	198	0.01	100	12.1	15689	PASS
442	198	50	100	77.6	100829	PASS
443	442	15	24	19.1	19260	PASS