
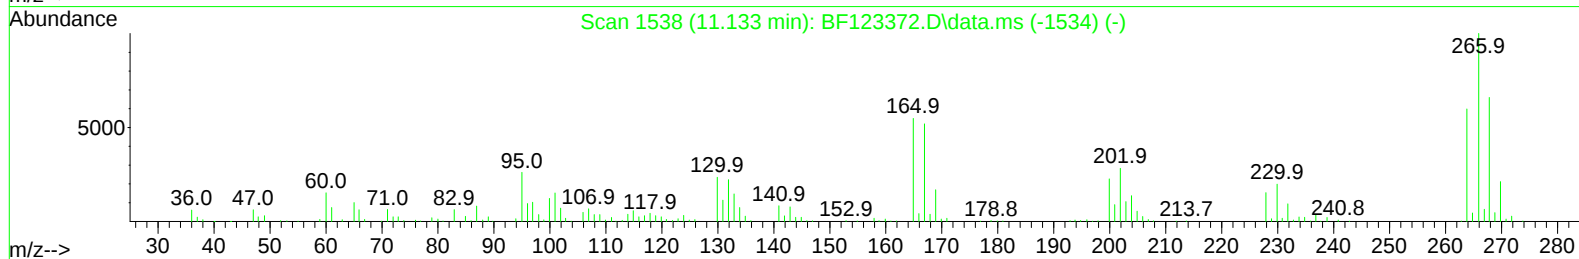
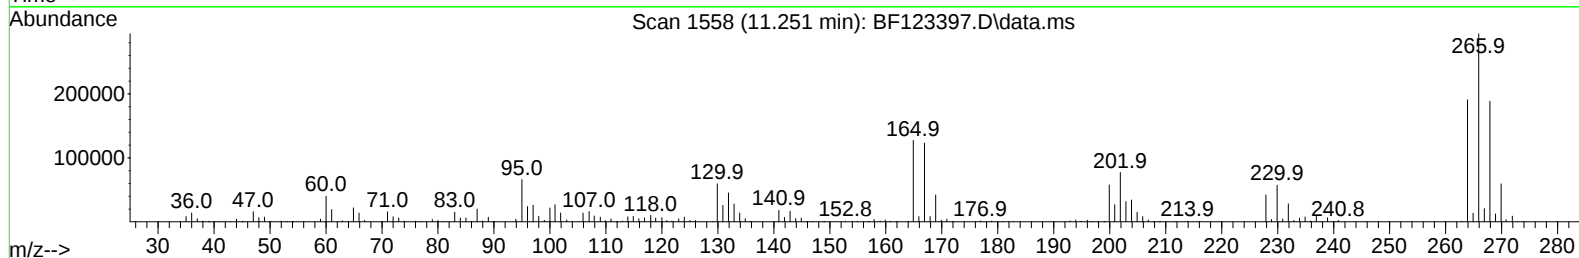


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
Data File : BF123397.D
Acq On : 23 Mar 2021 10:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 13:05:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 11:55:52 2021
Response via : Initial Calibration

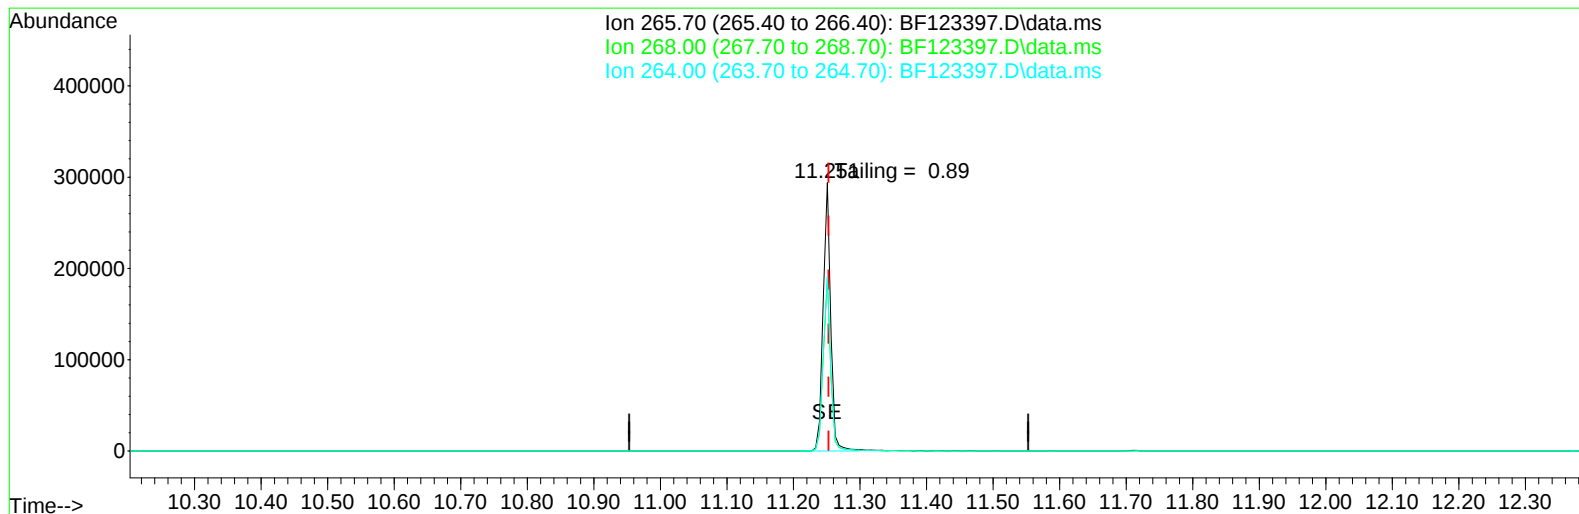

TIC: BF123397.D\data.ms

(70) Pentachlorophenol (C)




11.251min (-0.002) 45288.10 ng

response 237146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.15
264.00	62.30	64.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
Data File : BF123397.D
Acq On : 23 Mar 2021 10:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 13:05:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 11:55:52 2021
Response via : Initial Calibration

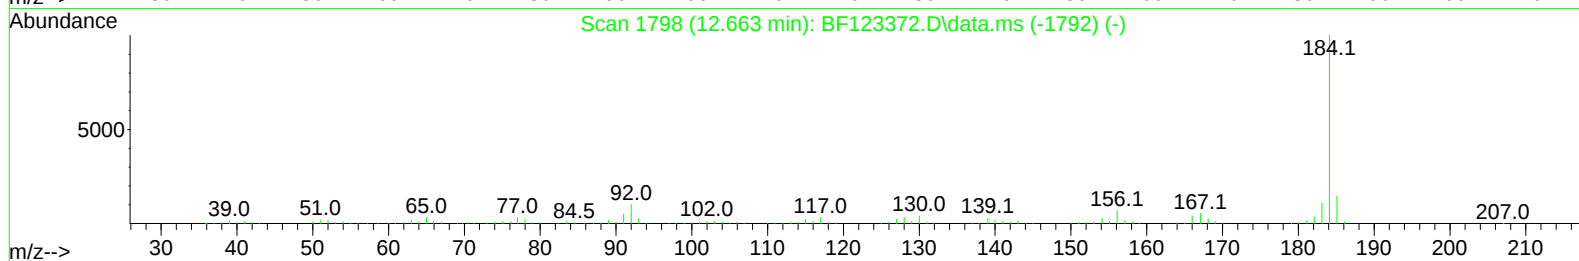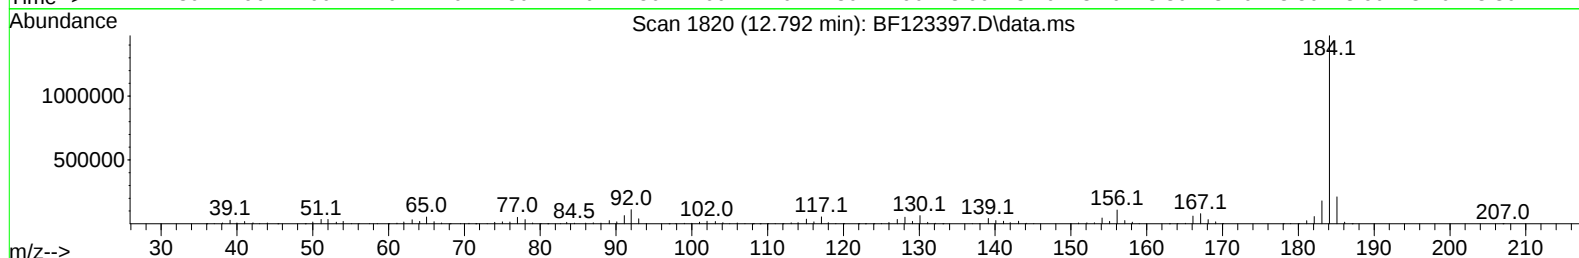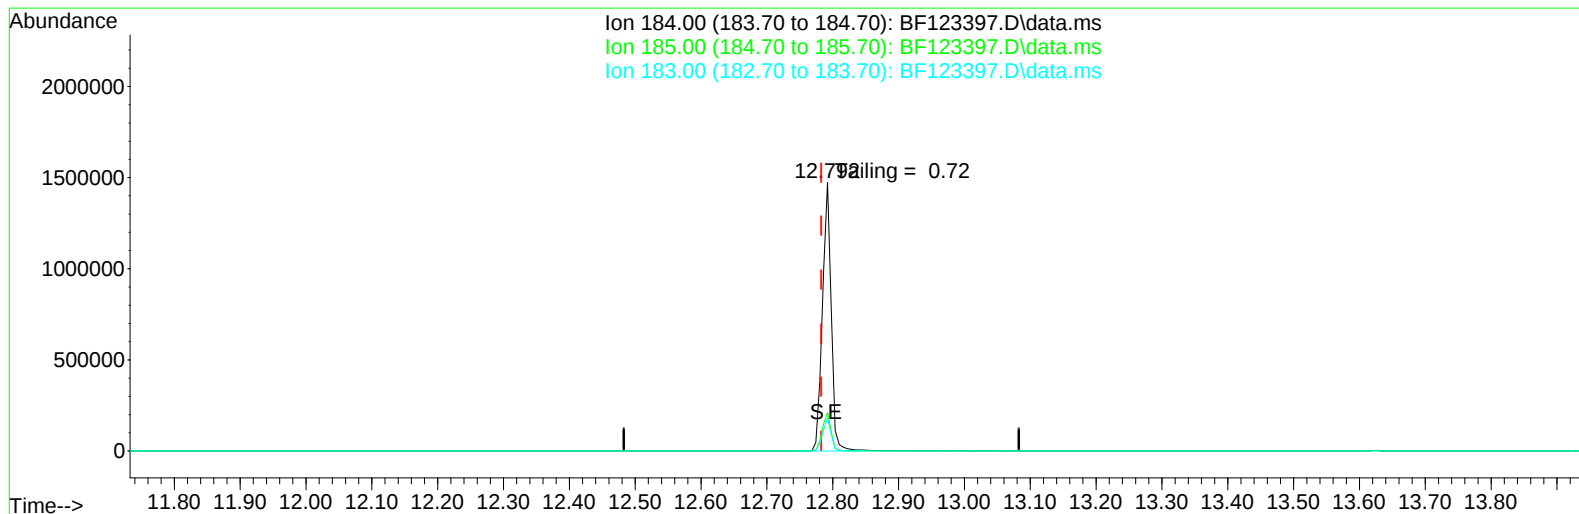

TIC: BF123397.D\data.ms

(77) Benzidine

12.792min (+ 0.009) 0.00 ng

response 1379154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.31
183.00	12.10	12.16
0.00	0.00	0.00