

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
 Data File : BF123416.D
 Acq On : 23 Mar 2021 22:02
 Operator : JU/CG
 Sample : M1739-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HP-627

Quant Time: Mar 24 00:27:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 15:58:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	268698	20.00	ng	0.00
21) Naphthalene-d8	8.198	136	953604	20.00	ng	# 0.00
39) Acenaphthene-d10	9.963	164	499442	20.00	ng	0.00
64) Phenanthrene-d10	11.451	188	774491	20.00	ng	0.00
76) Chrysene-d12	14.098	240	398718	20.00	ng	0.00
86) Perylene-d12	15.609	264	441344	20.00	ng	# 0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	596423	36.31	ng	0.00
7) Phenol-d6	6.528	99	461561	21.11	ng	0.00
23) Nitrobenzene-d5	7.481	82	1702786	96.37	ng	0.00
42) 2,4,6-Tribromophenol	10.757	330	467569	83.74	ng	0.00
45) 2-Fluorobiphenyl	9.280	172	2880100	82.38	ng	0.00
79) Terphenyl-d14	13.051	244	2334036	99.21	ng	0.00
Target Compounds						
10) Phenol	6.539	94	50053	2.23	ng	96
74) Di-n-butylphthalate	12.015	149	301827	6.52	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
Data File : BF123416.D
Acq On : 23 Mar 2021 22:02
Operator : JU/CG
Sample : M1739-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HP-627

Quant Time: Mar 24 00:27:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 15:58:35 2021
Response via : Initial Calibration




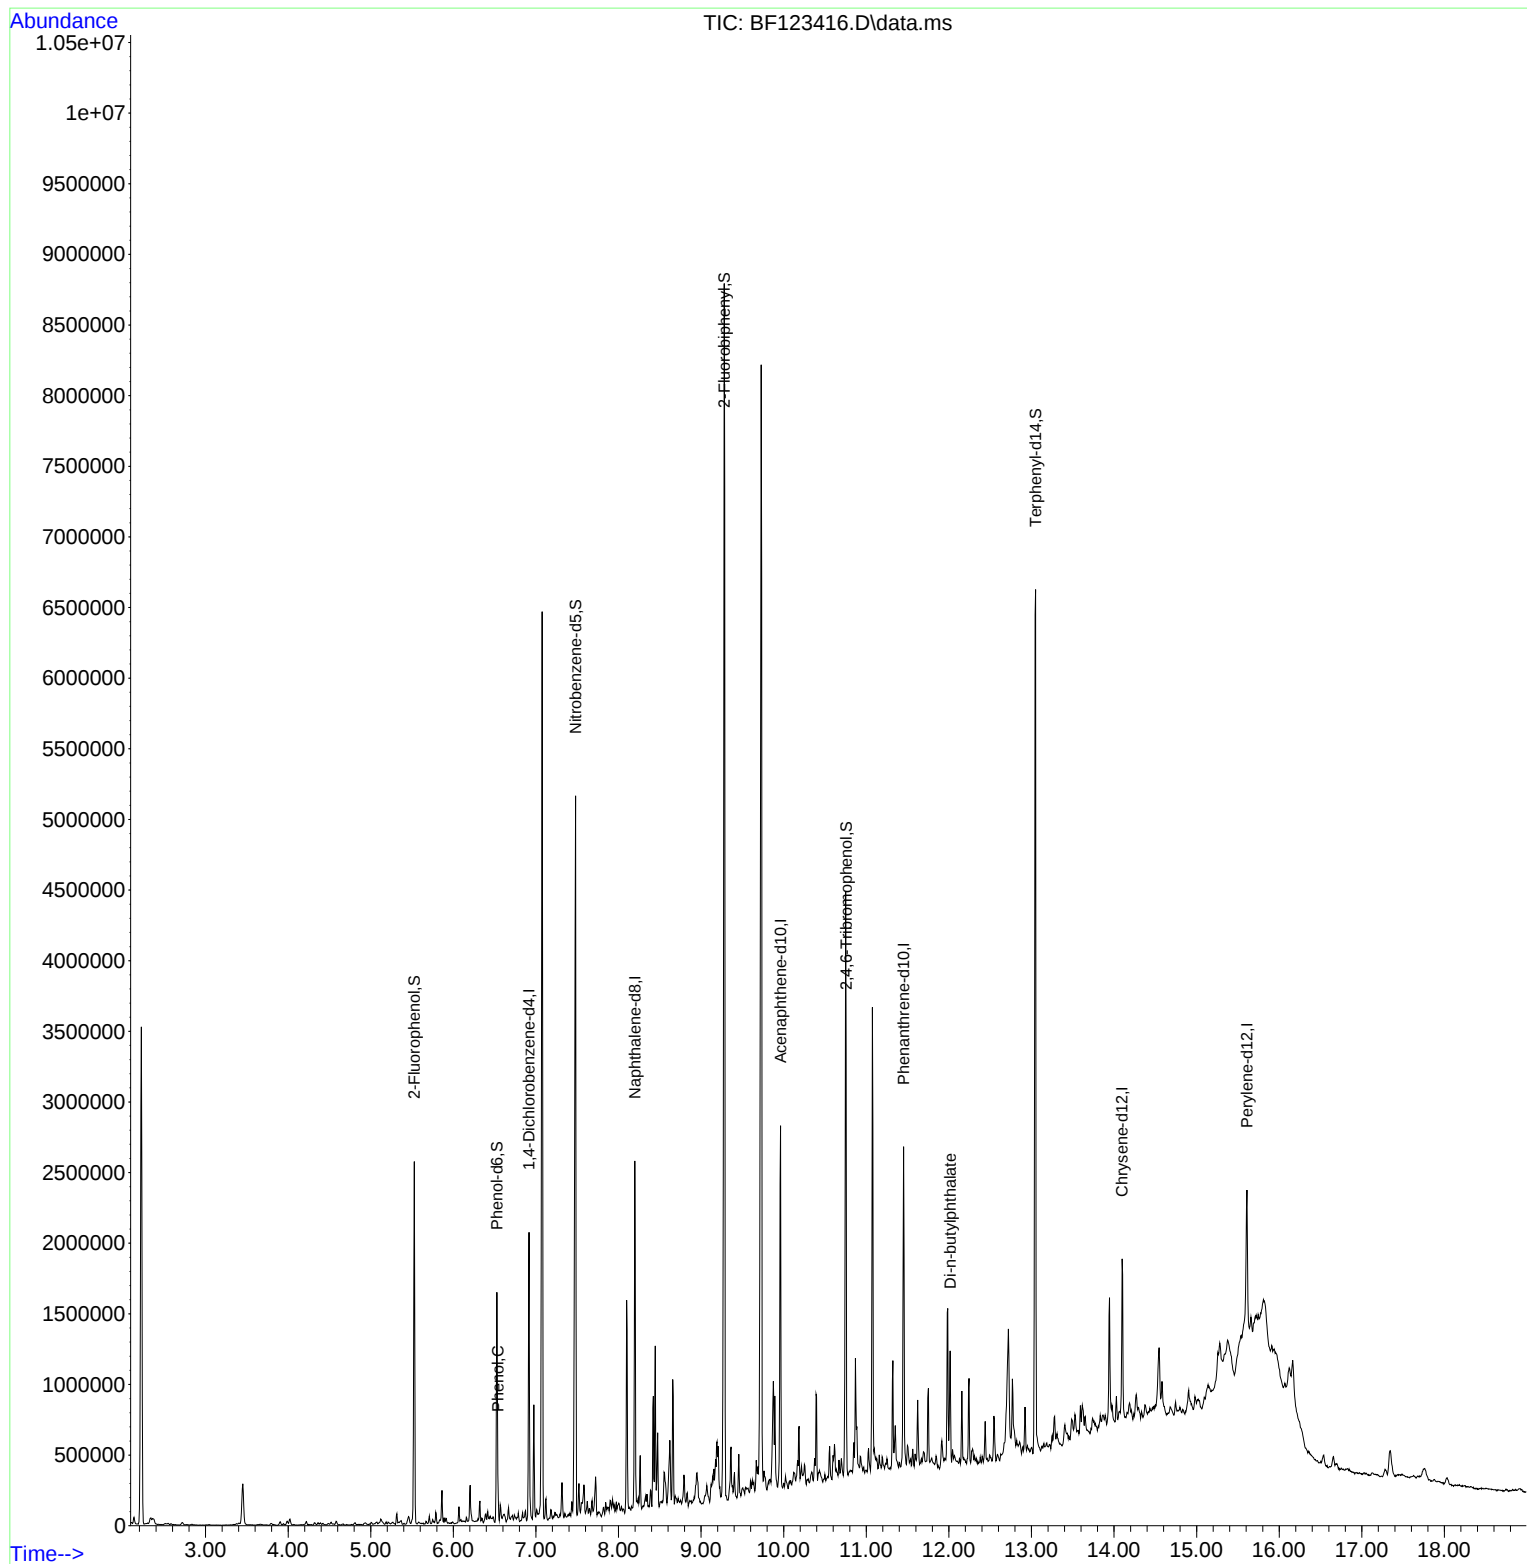




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.916 min Scan# 821
Delta R.T. -0.000 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02




Instrument :
BNA_F
ClientSampleId :
HP-627


Tgt Ion:152 Resp: 268698
Ion Ratio Lower Upper
152 100
150 147.7 125.8 188.6
115 61.6 49.3 73.9

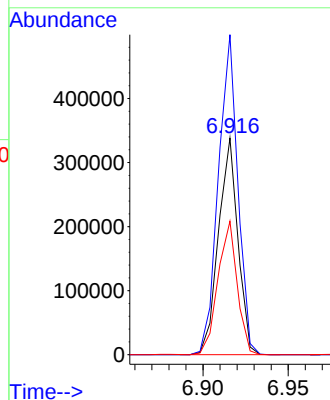

#5
2-Fluorophenol
Concen: 36.31 ng
RT: 5.528 min Scan# 585
Delta R.T. 0.006 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02

Tgt Ion:112 Resp: 596423
Ion Ratio Lower Upper
112 100
64 69.9 46.9 70.3
63 36.2 24.5 36.7


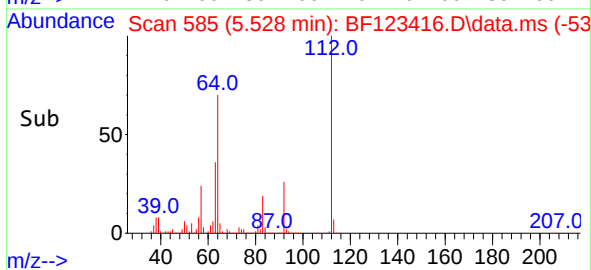
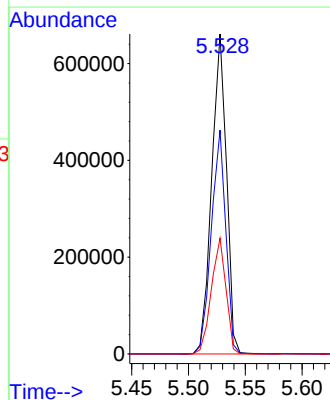





#7
Phenol-d6
Concen: 21.11 ng
RT: 6.528 min Scan# 755
Delta R.T. -0.006 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02




Instrument :
BNA_F
ClientSampleId :
HP-627


Tgt Ion: 99 Resp: 461561
Ion Ratio Lower Upper
99 100
42 23.8 13.8 20.6#
71 34.8 26.9 40.3

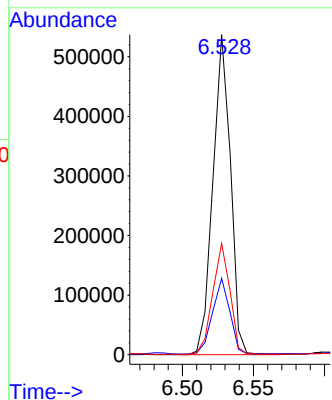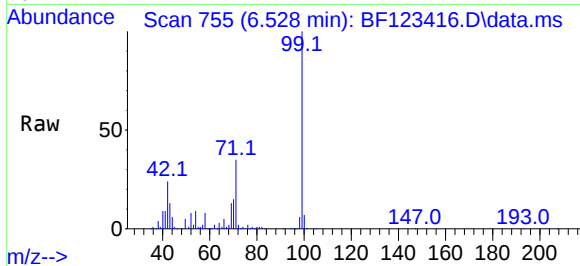

#10
Phenol
Concen: 2.23 ng
RT: 6.539 min Scan# 757
Delta R.T. -0.012 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02

Tgt Ion: 94 Resp: 50053
Ion Ratio Lower Upper
94 100
65 34.0 11.2 51.2
66 43.6 25.8 65.8

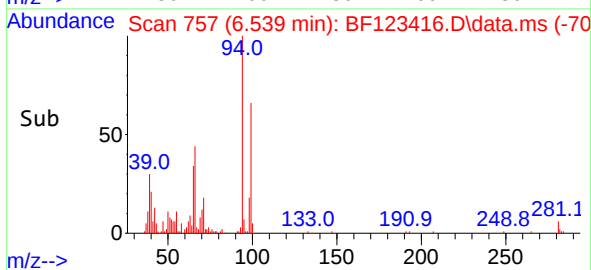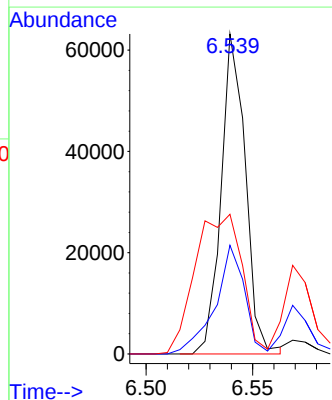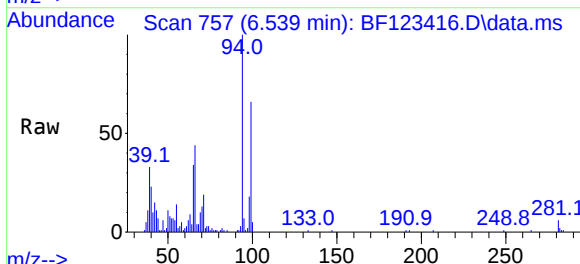







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.198 min Scan# 1039
Delta R.T. -0.006 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02

Instrument :
BNA_F
ClientSampleId :
HP-627

Tgt Ion:136 Resp: 953604




Ion	Ratio	Lower	Upper
136	100		
137	11.4	8.8	13.2
54	12.6	5.5	8.3#
68	6.7	4.6	6.8

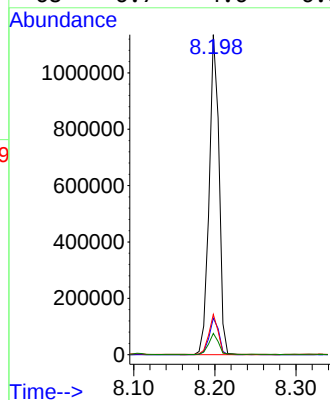


#23
Nitrobenzene-d5
Concen: 96.37 ng
RT: 7.481 min Scan# 917
Delta R.T. -0.000 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02

Tgt Ion: 82 Resp: 1702786

Ion	Ratio	Lower	Upper
82	100		
128	42.0	37.0	55.4
54	66.5	38.4	57.6#


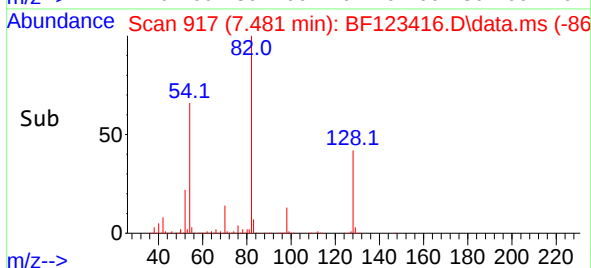
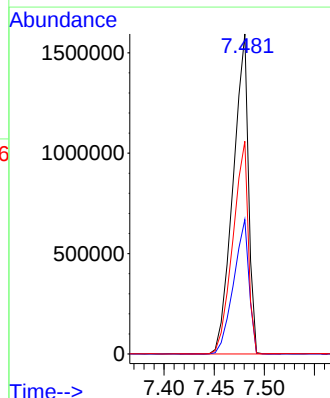





#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.963 min Scan# 1339
Delta R.T. -0.000 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02




Instrument :
BNA_F
ClientSampleId :
HP-627


Tgt Ion:164 Resp: 499442
Ion Ratio Lower Upper
164 100
162 104.2 80.8 121.2
160 44.8 35.4 53.0

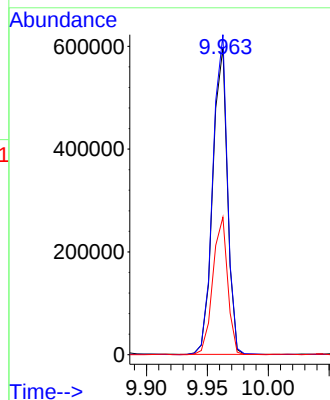

#42
2,4,6-Tribromophenol
Concen: 83.74 ng
RT: 10.757 min Scan# 1474
Delta R.T. -0.000 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02

Tgt Ion:330 Resp: 467569
Ion Ratio Lower Upper
330 100
332 96.5 77.5 116.3
141 32.7 23.8 35.8


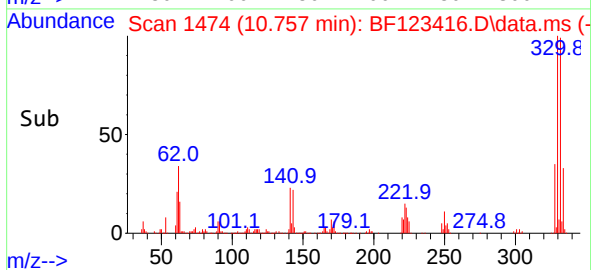
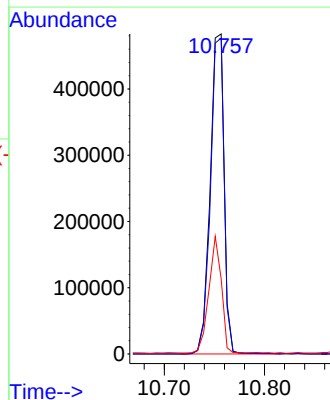





#45
2-Fluorobiphenyl
Concen: 82.38 ng
RT: 9.280 min Scan# 1223
Delta R.T. -0.001 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02




Instrument :
BNA_F
ClientSampleId :
HP-627


Tgt Ion:172 Resp: 2880100
Ion Ratio Lower Upper
172 100
171 36.7 29.6 44.4
170 25.0 19.5 29.3

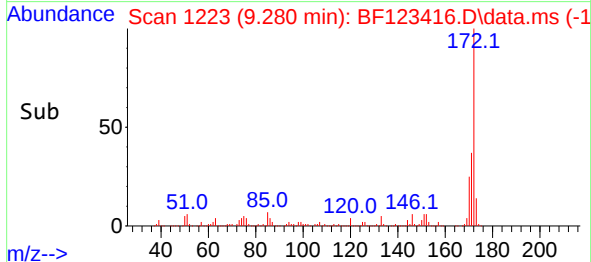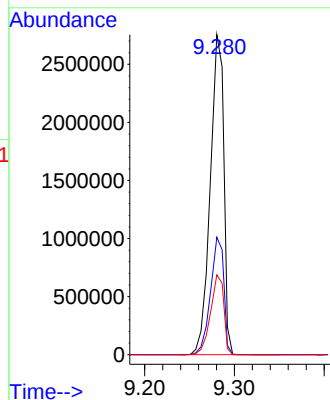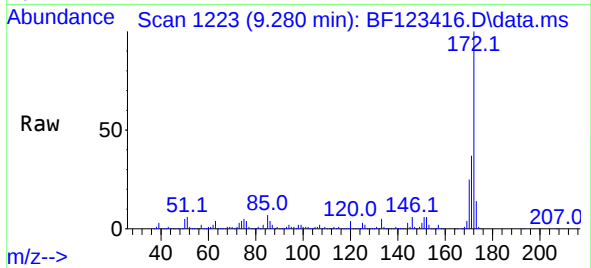

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.451 min Scan# 1592
Delta R.T. -0.000 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02

Tgt Ion:188 Resp: 774491
Ion Ratio Lower Upper
188 100
94 9.9 7.4 11.2
80 10.7 8.2 12.4


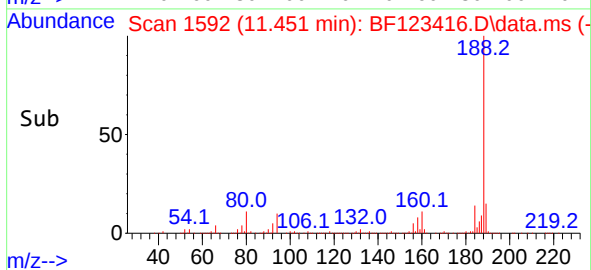
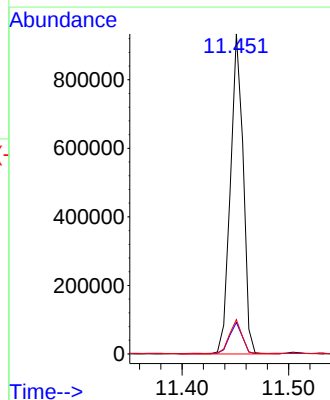





#74
Di-n-butylphthalate
Concen: 6.52 ng
RT: 12.015 min Scan# 1688
Delta R.T. -0.000 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02




Instrument :
BNA_F
ClientSampleId :
HP-627


Tgt Ion:149 Resp: 301827
Ion Ratio Lower Upper
149 100
150 8.7 7.8 11.6
104 5.0 4.2 6.4

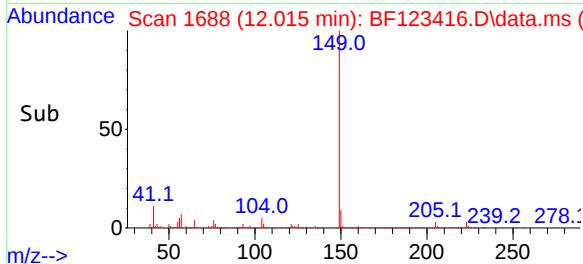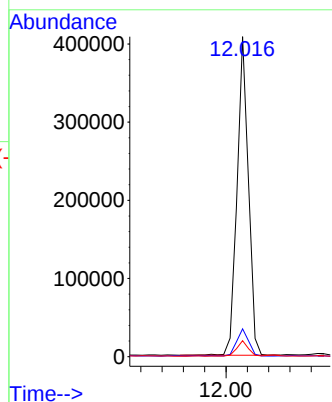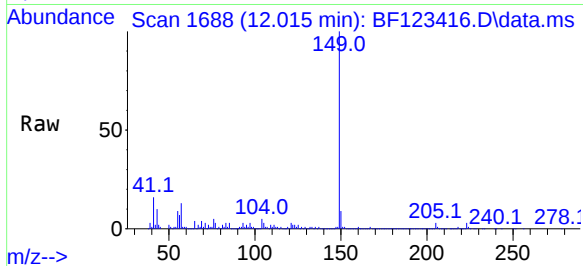

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.098 min Scan# 2042
Delta R.T. -0.006 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02


Tgt Ion:240 Resp: 398718
Ion Ratio Lower Upper
240 100
120 11.8 8.6 12.8
236 25.3 20.3 30.5

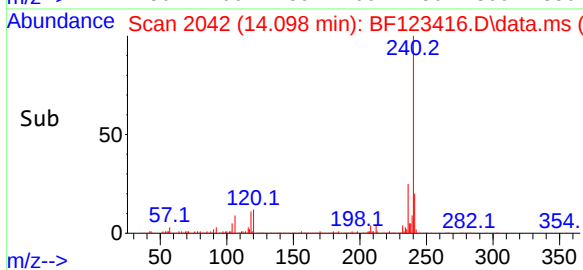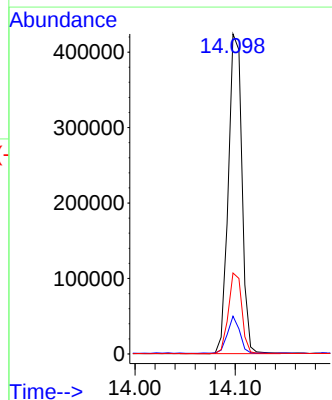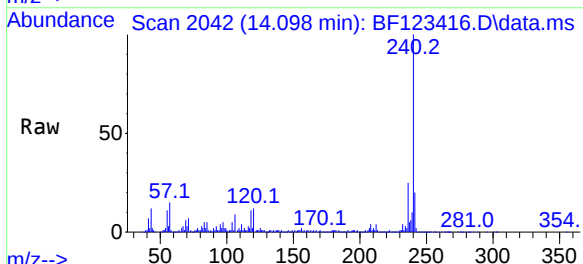






#79
Terphenyl-d14
Concen: 99.21 ng
RT: 13.051 min Scan# 1864
Delta R.T. 0.006 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02


Instrument :
BNA_F
ClientSampleId :
HP-627

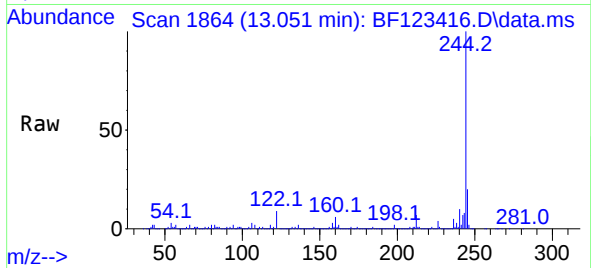

Tgt Ion:244 Resp: 2334036
Ion Ratio Lower Upper
244 100
212 7.1 5.7 8.5
122 8.9 8.3 12.5

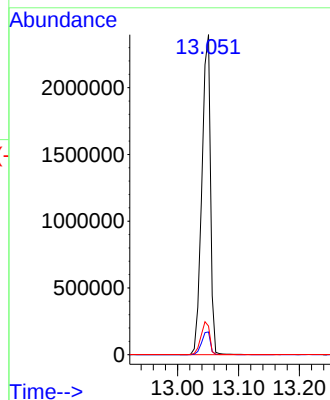

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.609 min Scan# 2299
Delta R.T. 0.006 min
Lab File: BF123416.D
Acq: 23 Mar 2021 22:02



Tgt Ion:264 Resp: 441344
Ion Ratio Lower Upper
264 100
260 22.0 18.6 28.0
265 30.5 17.0 25.6#

