
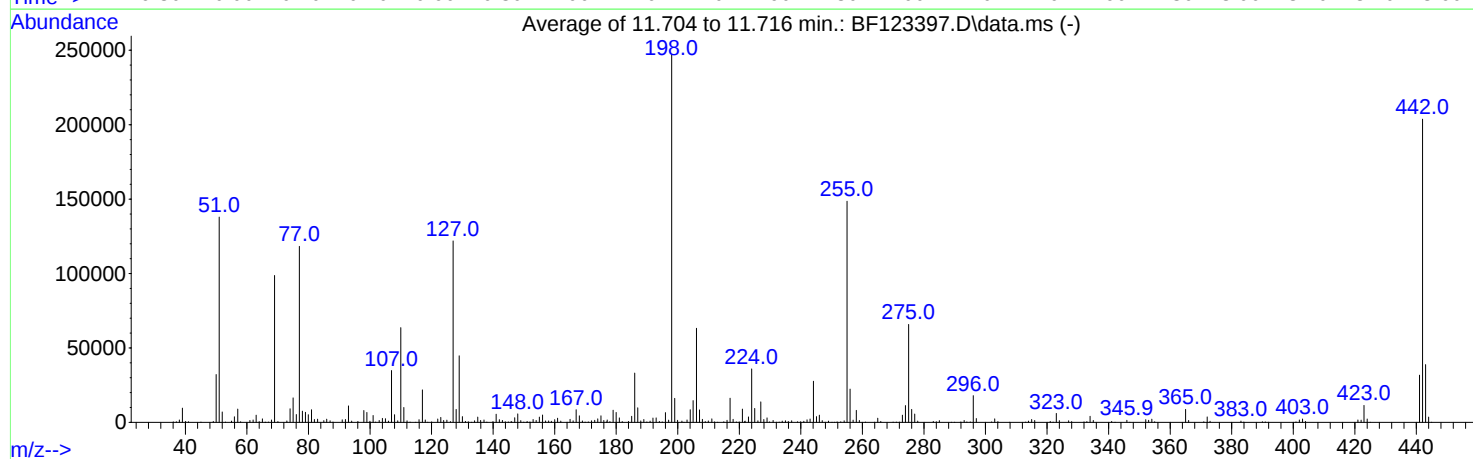


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
 Data File : BF123397.D
 Acq On : 23 Mar 2021 10:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 24 12:51:15 2021

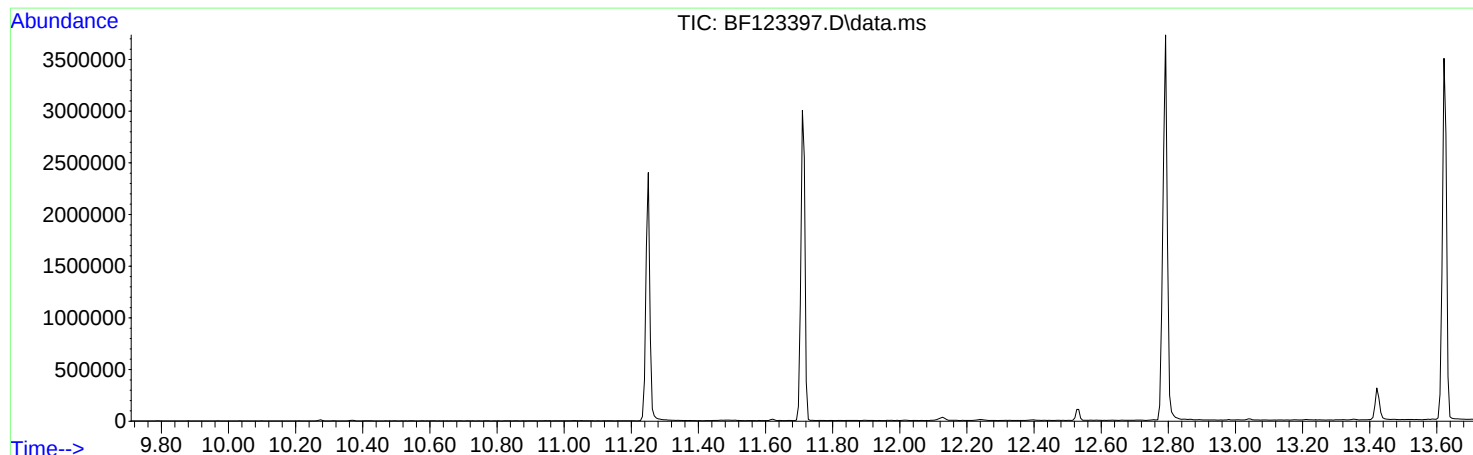




AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.8	137875	PASS
68	69	0.00	2	1.7	1658	PASS
69	198	0.00	100	39.9	98691	PASS
70	69	0.00	2	0.5	527	PASS
127	198	10	80	49.3	121936	PASS
197	198	0.00	2	0.6	1551	PASS
198	198	100	100	100.0	247144	PASS
199	198	5	9	6.5	16130	PASS
275	198	10	60	26.6	65819	PASS
365	198	1	100	3.5	8744	PASS
441	198	0.01	100	12.8	31666	PASS
442	442	50	100	100.0	203755	PASS
443	442	15	24	19.1	38862	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
Data File : BF123397.D
Acq On : 23 Mar 2021 10:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 23 13:05:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 11:55:52 2021
Response via : Initial Calibration

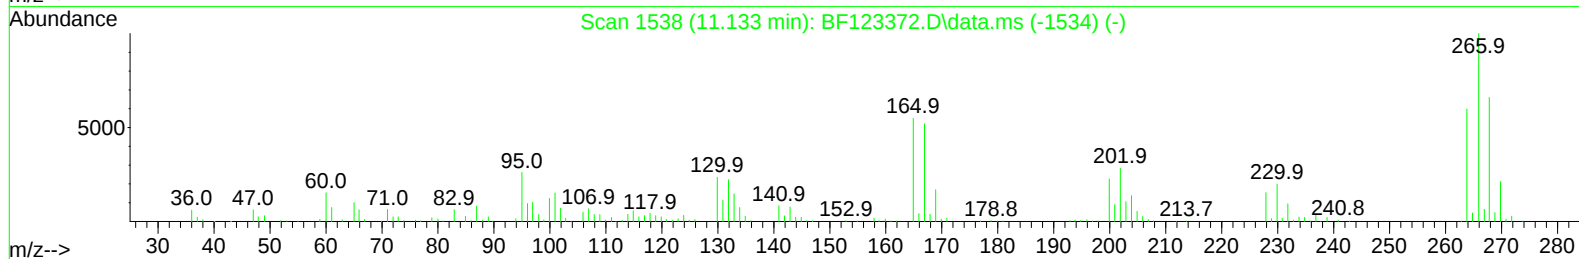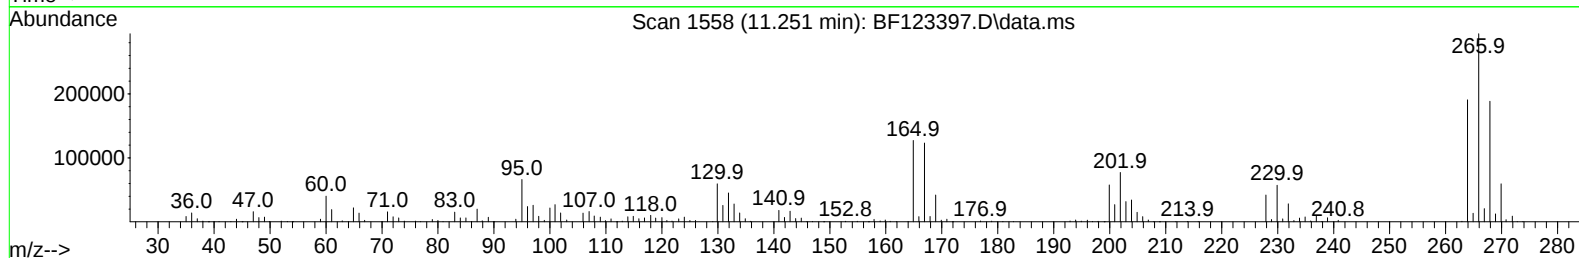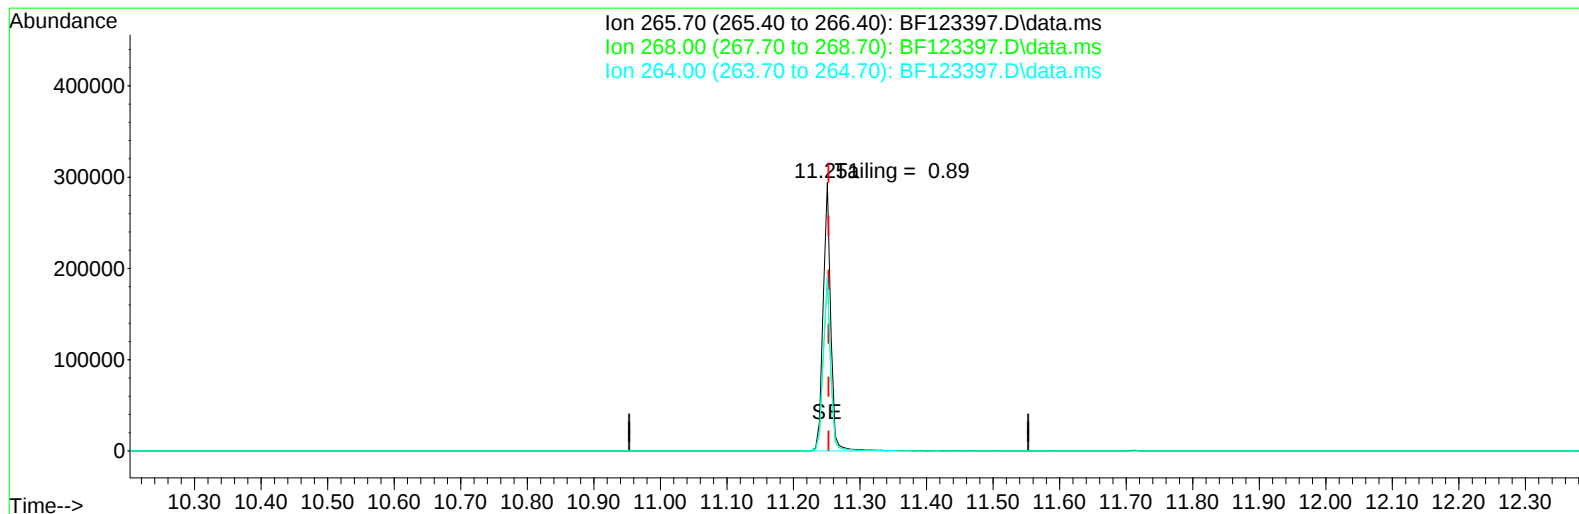

TIC: BF123397.D\data.ms

(70) Pentachlorophenol (C)

11.251min (-0.002) 45288.10 ng




response 237146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.15
264.00	62.30	64.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032321\
 Data File : BF123397.D
 Acq On : 23 Mar 2021 10:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 13:05:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 11:55:52 2021
 Response via : Initial Calibration

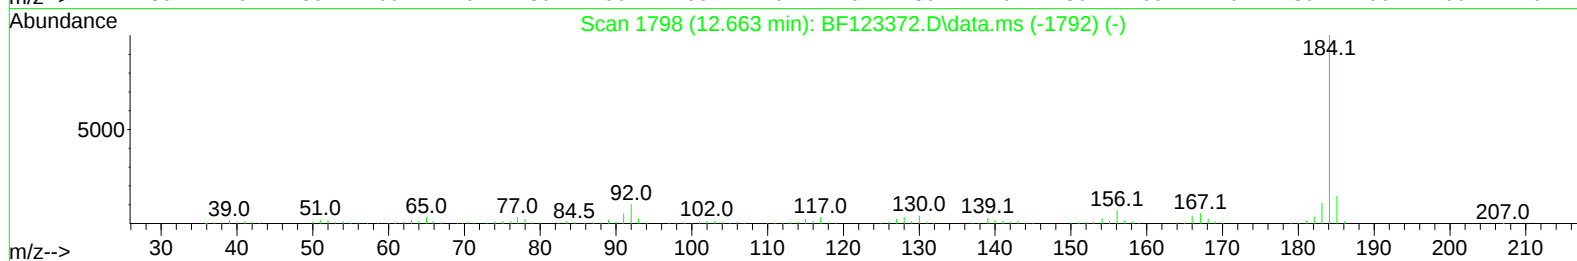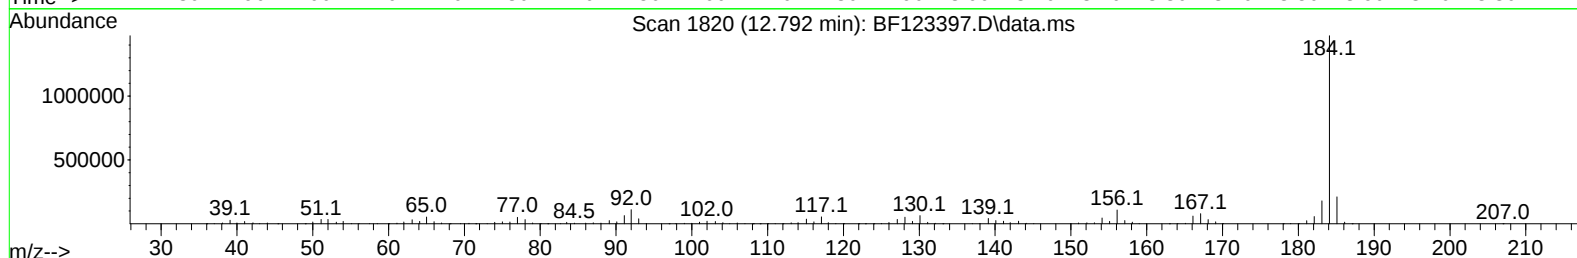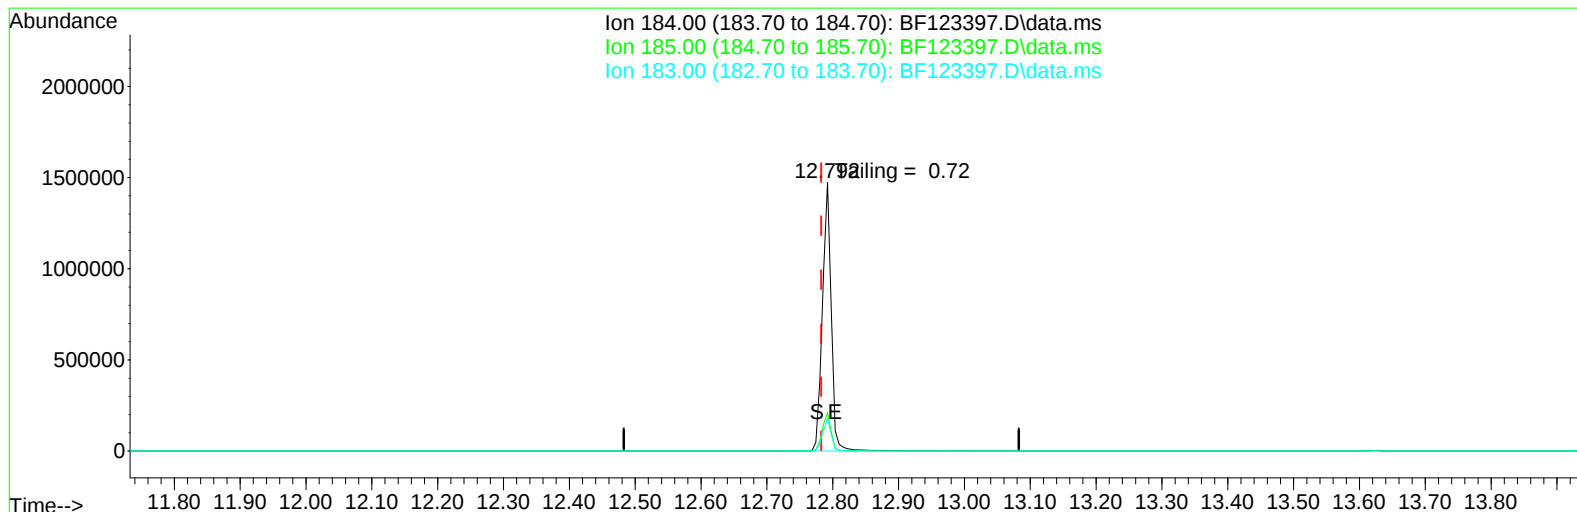

TIC: BF123397.D\data.ms

(77) Benzidine

12.792min (+ 0.009) 0.00 ng

response 1379154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.31
183.00	12.10	12.16
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/23/2021	BNA_F	<u>BF123397.D</u>
Compound Name	Response	Retention Time
DDT	547041	13.62
DDD	404	13.32
DDE	830	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1234	548275	0.23