

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
 Data File : BF077923.D
 Acq On : 24 Mar 2015 20:47
 Operator : TP/IZ
 Sample : G1613-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-11

Quant Time: Mar 25 00:12:19 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 25 00:51:55 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.12	152	50461	20.00	ng	0.00
21) Naphthalene-d8	8.69	136	210051	20.00	ng	0.00
38) Acenaphthene-d10	10.86	164	101558	20.00	ng	0.00
63) Phenanthrene-d10	12.69	188	208017	20.00	ng	0.00
75) Chrysene-d12	15.97	240	222461	20.00	ng	0.00
86) Perylene-d12	17.73	264	205876	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	254612	88.07	ng	0.00
7) Phenol-d6	6.69	99	324832	90.95	ng	0.00
23) Nitrobenzene-d5	7.81	82	176512	55.08	ng	0.00
41) 2,4,6-Tribromophenol	11.84	330	75750	77.96	ng	0.00
44) 2-Fluorobiphenyl	10.04	172	404648	58.56	ng	0.00
78) Terphenyl-d14	14.69	244	479851	52.69	ng	0.00
Target Compounds						
2) 1,4-Dioxane	1.77	88	27903	21.26	ng	# 100
19) n-Nitroso-di-n-propylamine	7.81	70	22544	9.12	ng	# 78
50) 2,6-Dinitrotoluene	10.86	165	12158	7.79	ng	# 24
56) 2,4-Dinitrotoluene	10.86	165	12158	5.97	ng	# 11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
Data File : BF077923.D
Acq On : 24 Mar 2015 20:47
Operator : TP/IZ
Sample : G1613-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-11

Quant Time: Mar 25 00:12:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 25 00:51:55 2015
Response via : Initial Calibration

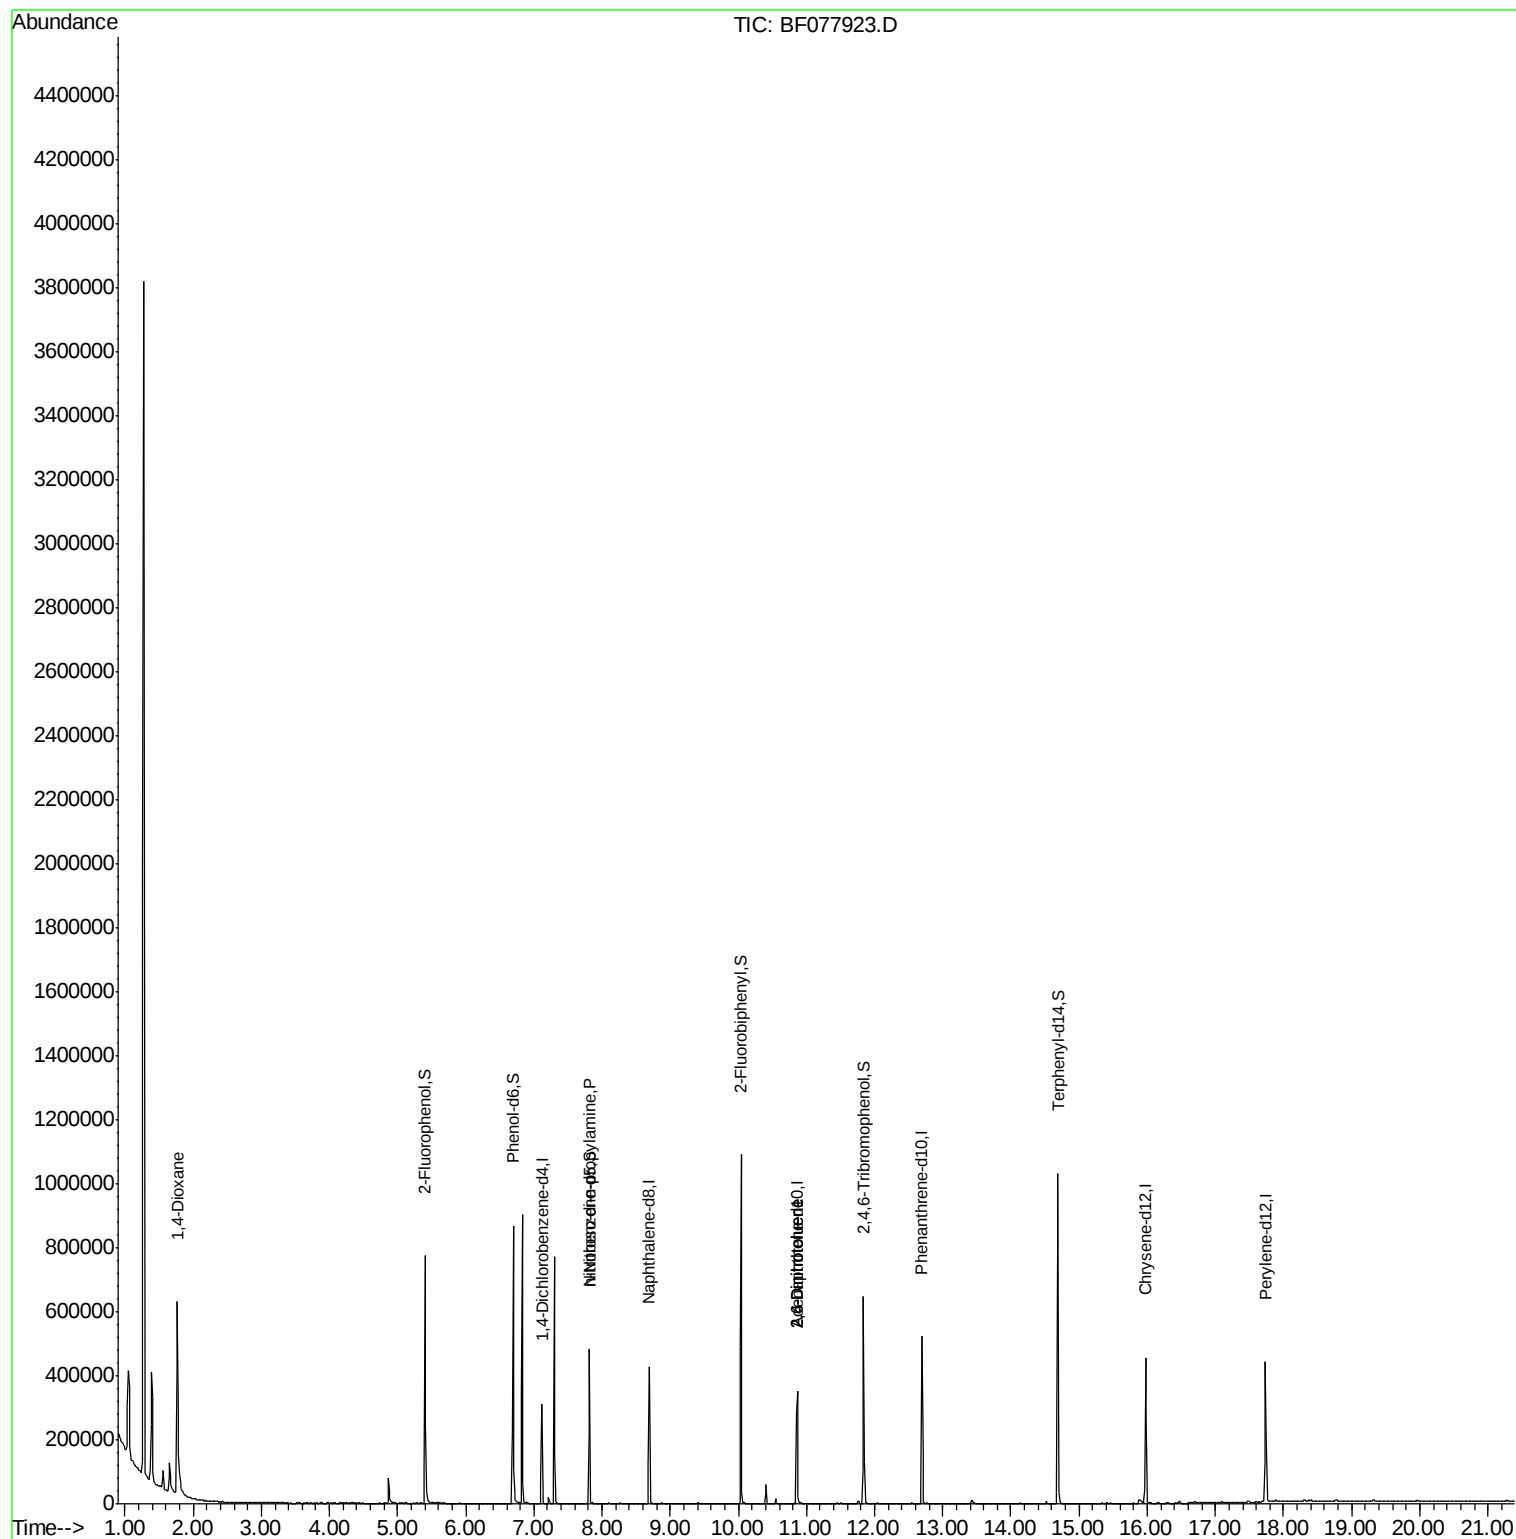

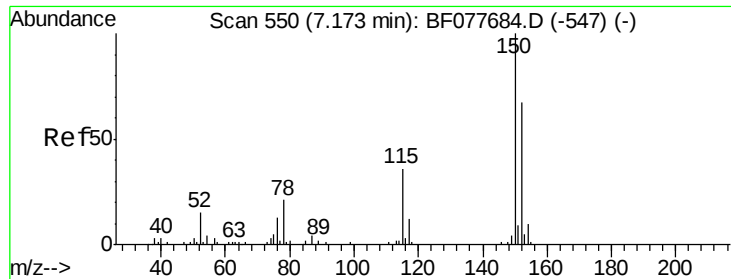


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.12 min Scan# 545
Delta R.T. -0.00 min
Lab File: BF077923.D
Acq: 24 Mar 2015 20:47

Instrument :
BNA_F
ClientSampleId :
SB-11

Tgt Ion:152 Resp: 50461
Ion Ratio Lower Upper
152 100
150 159.9 119.5 179.3
115 60.1 43.0 64.4

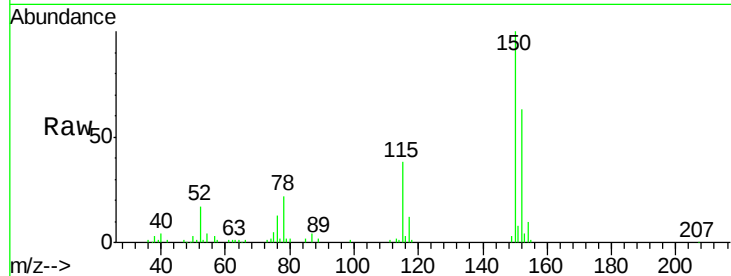


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

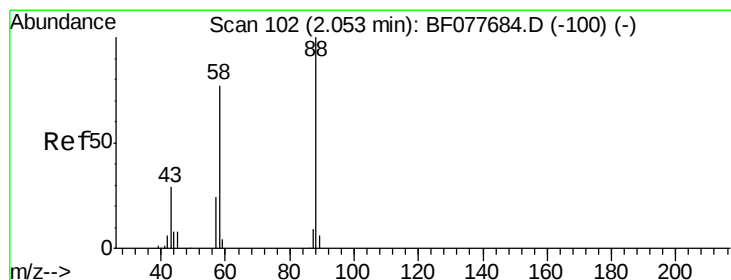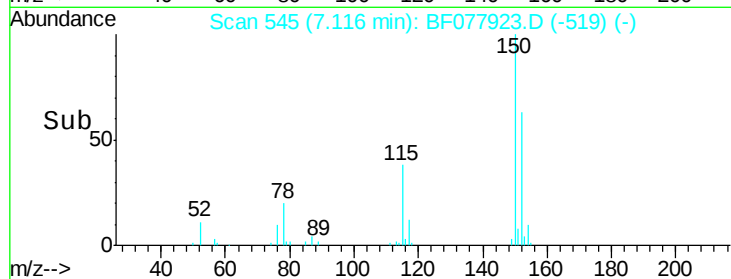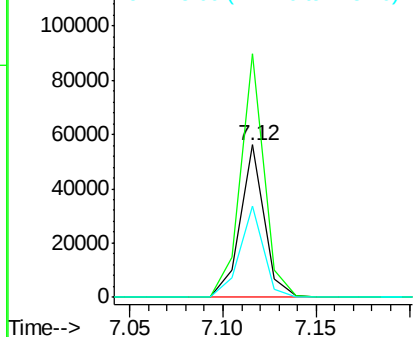



#2


1,4-Dioxane
Concen: 21.26 ng
RT: 1.77 min Scan# 77
Delta R.T. -0.22 min
Lab File: BF077923.D
Acq: 24 Mar 2015 20:47

Tgt Ion: 88 Resp: 27903
Ion Ratio Lower Upper
88 100
58 0.0 0.0 0.0
43 0.0 0.0 0.0



Abundance Ion 88.00 (87.70 to 88.70): BF0
Ion 58.00 (57.70 to 58.70): BF0
Ion 43.00 (42.70 to 43.70): BF0

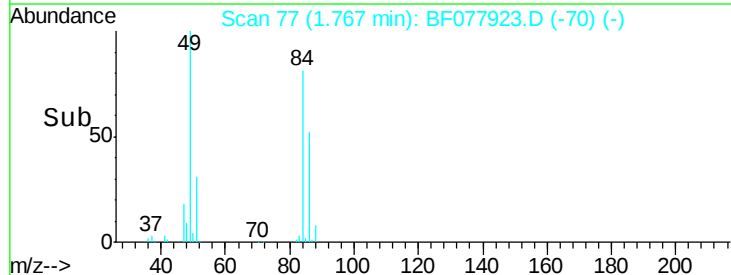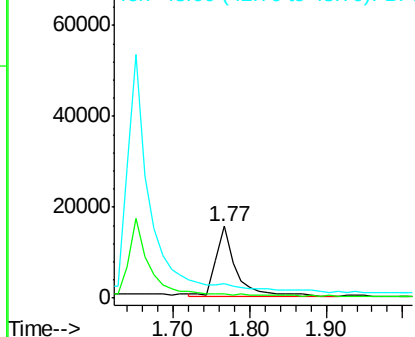



#5

2-Fluorophenol

Concen: 88.07 ng

RT: 5.40 min Scan# 395

Delta R.T. -0.00 min

Lab File: BF077923.D

Acq: 24 Mar 2015 20:47

Instrument :

BNA_F

ClientSampleId :

SB-11


Tgt Ion: 112 Resp: 254612

Ion Ratio Lower Upper

112 100

64 56.6 38.6 57.8




63 28.7 19.3 28.9

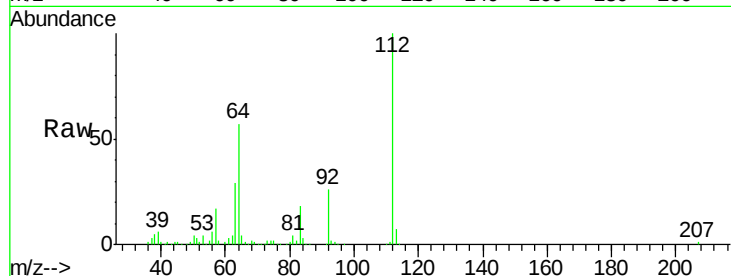

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

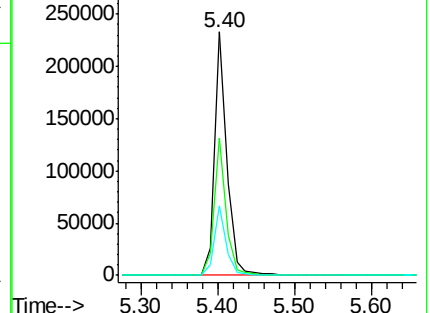

#7

Phenol-d6

Concen: 90.95 ng

RT: 6.69 min Scan# 508

Delta R.T. -0.00 min

Lab File: BF077923.D

Acq: 24 Mar 2015 20:47


Tgt Ion: 99 Resp: 324832

Ion Ratio Lower Upper

99 100

42 15.4 11.0 16.4



71 31.0 23.4 35.2




Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



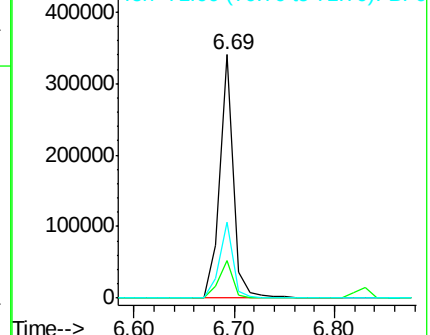





#19
n-Nitroso-di-n-propylamine
Concen: 9.12 ng
RT: 7.81 min Scan# 606
Delta R.T. 0.17 min
Lab File: BF077923.D
Acq: 24 Mar 2015 20:47




Instrument :
BNA_F
ClientSampleId :
SB-11


Tgt Ion: 70 Resp: 22544
Ion Ratio Lower Upper
70 100
42 43.4 44.5 66.7#
101 0.0 7.4 11.2#
130 2.3 15.3 22.9#

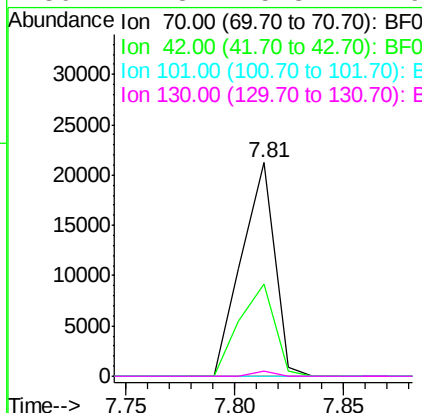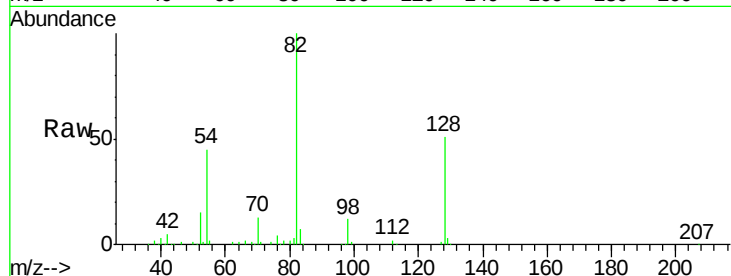

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.69 min Scan# 683
Delta R.T. -0.00 min
Lab File: BF077923.D
Acq: 24 Mar 2015 20:47

Tgt Ion: 136 Resp: 210051
Ion Ratio Lower Upper
136 100
137 10.7 8.7 13.1
54 6.2 4.6 6.8
68 5.2 3.7 5.5


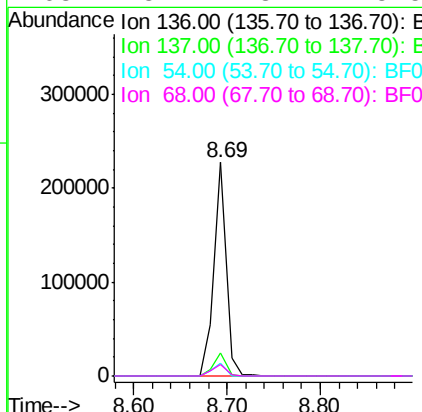




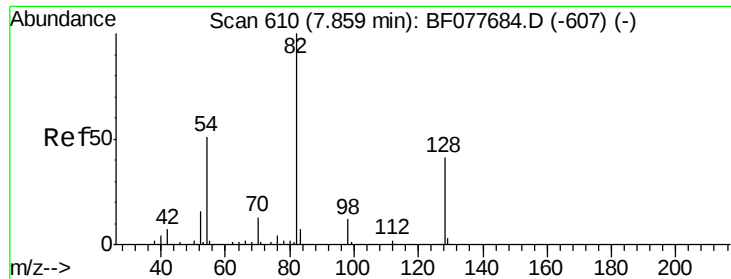

#23
 Nitrobenzene-d5
 Concen: 55.08 ng
 RT: 7.81 min Scan# 606
 Delta R.T. -0.00 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47




Instrument :
 BNA_F
 ClientSampleId :
 SB-11


Tgt Ion: 82 Resp: 176512
 Ion Ratio Lower Upper
 82 100
 128 51.2 32.8 49.2#
 54 44.8 40.6 60.8

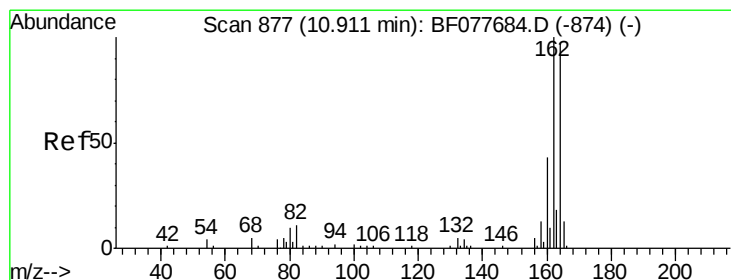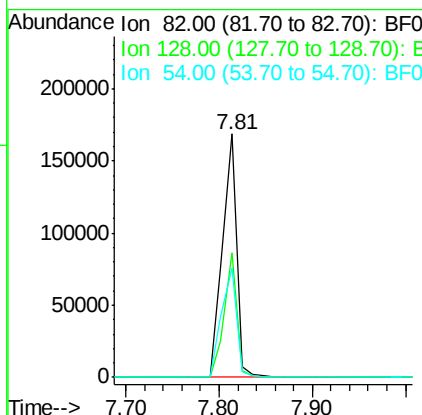

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.86 min Scan# 873
 Delta R.T. -0.00 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47

Tgt Ion: 164 Resp: 101558
 Ion Ratio Lower Upper
 164 100
 162 108.6 82.4 123.6
 160 47.3 35.8 53.6

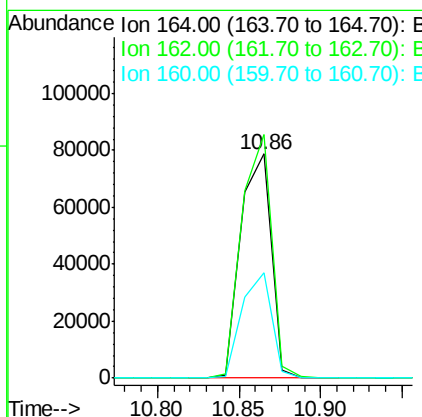


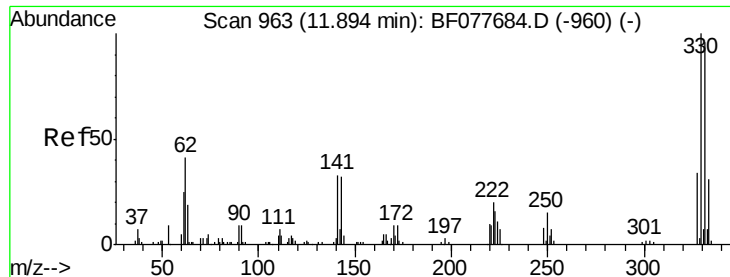




#41
 2,4,6-Tribromophenol
 Concen: 77.96 ng
 RT: 11.84 min Scan# 958
 Delta R.T. -0.00 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47

Instrument :
 BNA_F
 ClientSampled :
 SB-11

Tgt Ion:330 Resp: 75750
 Ion Ratio Lower Upper
 330 100
 332 94.6 0.0 0.0#
 141 40.6 0.0 0.0#

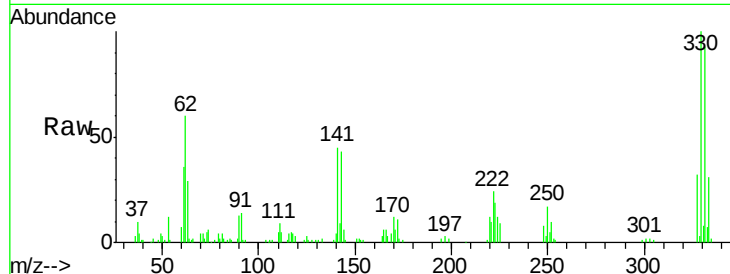


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

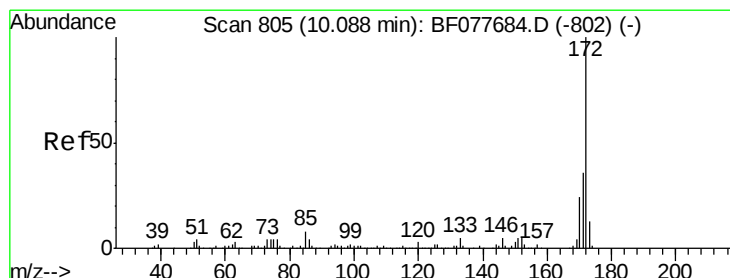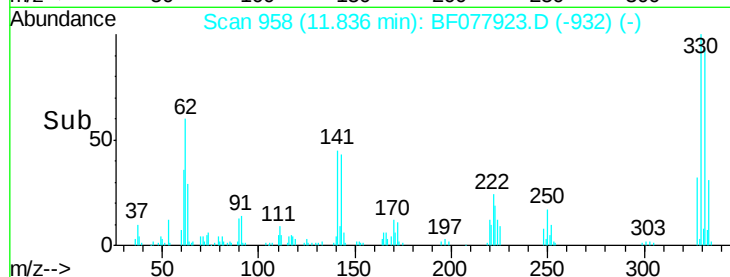
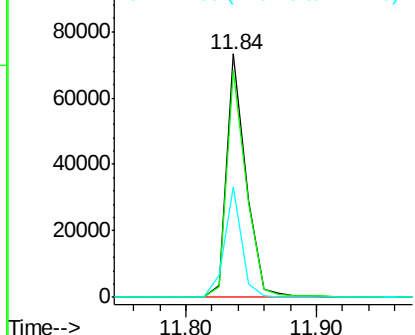



#44
 2-Fluorobiphenyl
 Concen: 58.56 ng
 RT: 10.04 min Scan# 801
 Delta R.T. -0.00 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47

Tgt Ion:172 Resp: 404648
 Ion Ratio Lower Upper
 172 100
 171 34.1 28.5 42.7
 170 23.3 18.8 28.2

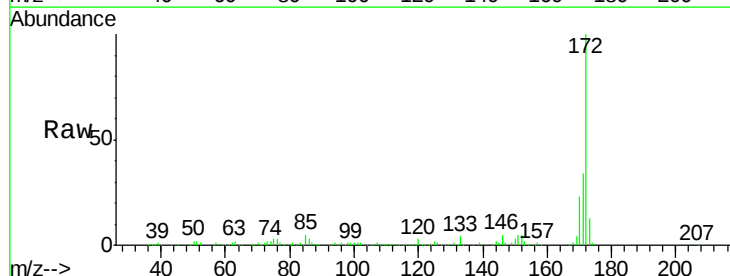

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



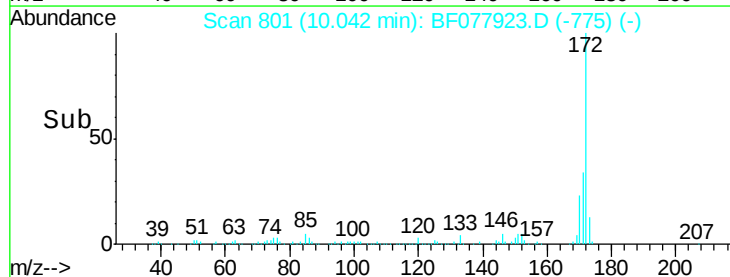
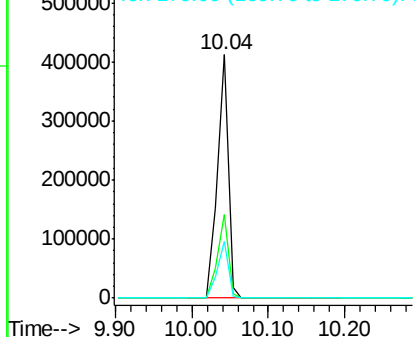


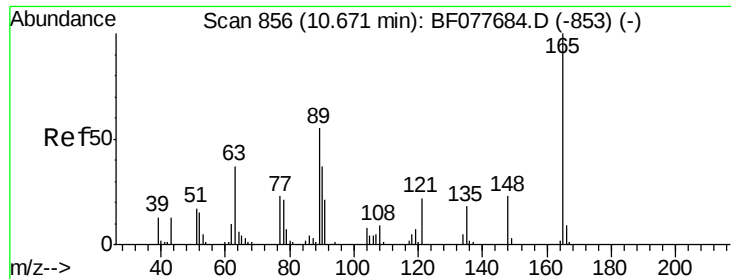

#50
 2,6-Dinitrotoluene
 Concen: 7.79 ng
 RT: 10.86 min Scan# 873
 Delta R.T. 0.24 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47




Instrument :
 BNA_F
 ClientSampleId :
 SB-11


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.1	66.1#
89	0.0	44.3	66.5#

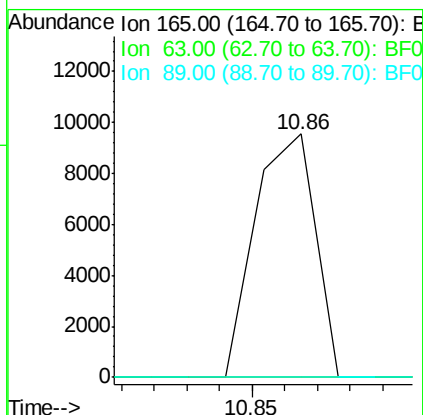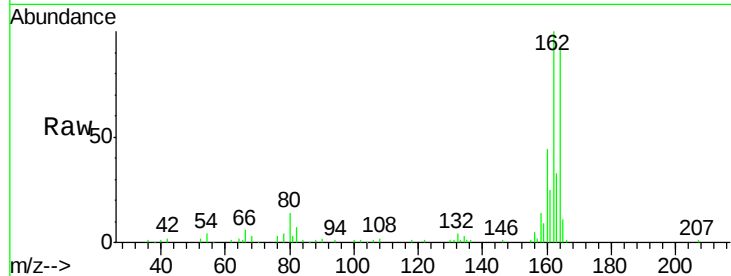

#56
 2,4-Dinitrotoluene
 Concen: 5.97 ng
 RT: 10.86 min Scan# 873
 Delta R.T. -0.25 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	52.4	78.6#
89	0.0	72.4	108.6#
182	0.0	2.0	3.0#

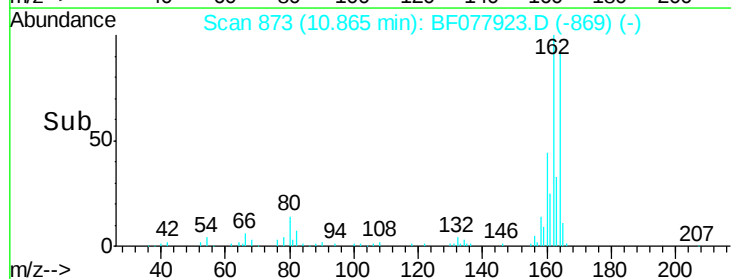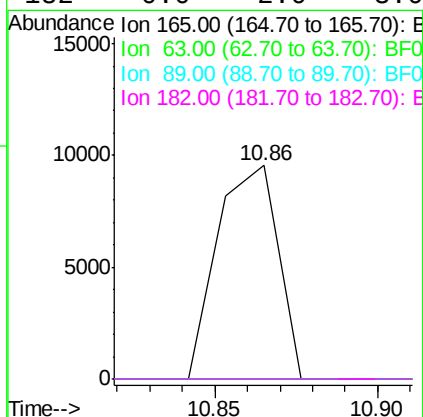


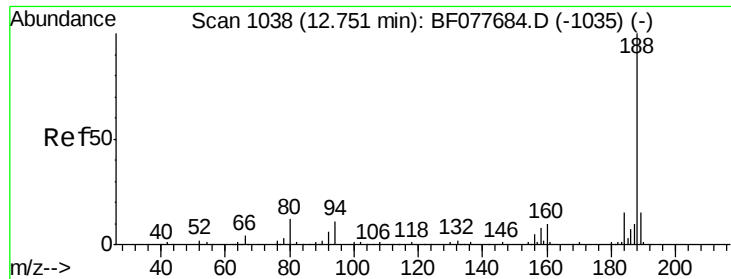




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.69 min Scan# 1033
Delta R.T. -0.00 min
Lab File: BF077923.D
Acq: 24 Mar 2015 20:47

Instrument :
BNA_F
ClientSampled :
SB-11

Tgt Ion:188 Resp: 208017
Ion Ratio Lower Upper
188 100
94 11.0 8.7 13.1
80 10.9 9.3 13.9




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


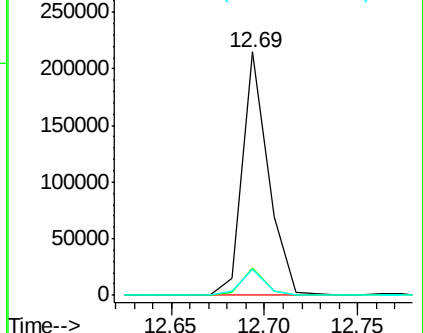



#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.97 min Scan# 1320
Delta R.T. -0.00 min
Lab File: BF077923.D
Acq: 24 Mar 2015 20:47

Tgt Ion:240 Resp: 222461
Ion Ratio Lower Upper
240 100
120 14.8 8.2 12.2#
236 25.6 20.0 30.0



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



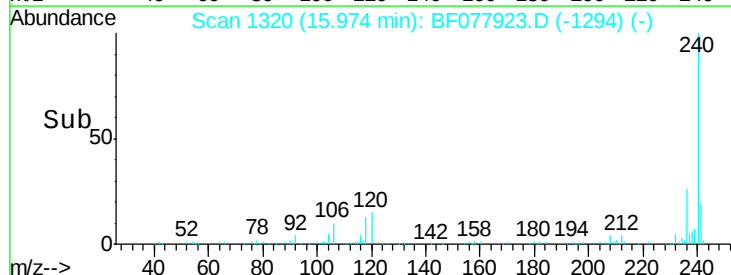
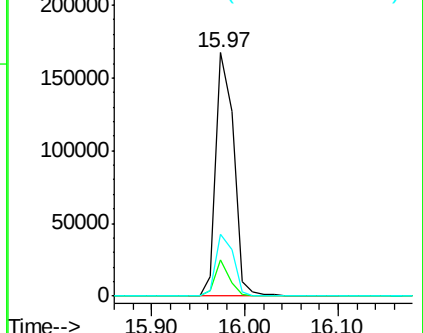


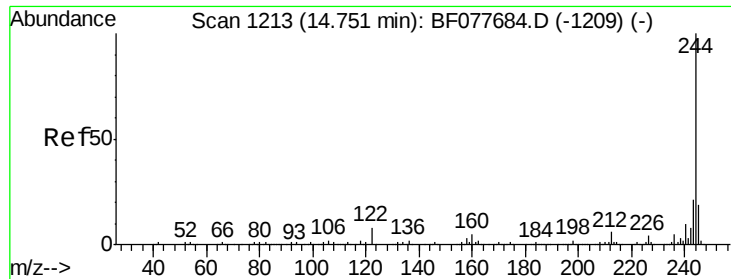

#78
 Terphenyl-d14
 Concen: 52.69 ng
 RT: 14.69 min Scan# 1208
 Delta R.T. -0.00 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-11

Tgt Ion:244 Resp: 479851
 Ion Ratio Lower Upper
 244 100
 212 6.0 4.9 7.3
 122 7.9 6.2 9.4

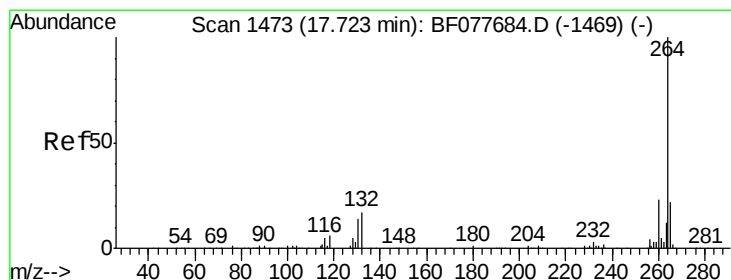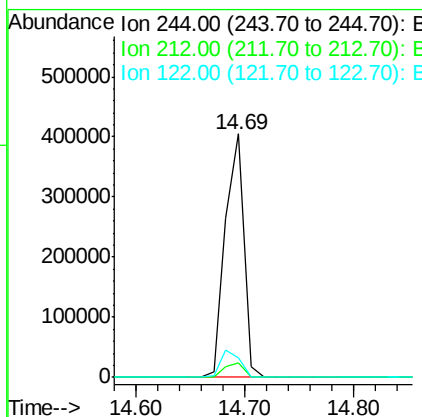

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.73 min Scan# 1474
 Delta R.T. 0.03 min
 Lab File: BF077923.D
 Acq: 24 Mar 2015 20:47

Tgt Ion:264 Resp: 205876
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.6 27.8
 265 21.4 17.3 25.9

