


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
 Data File : BF077928.D
 Acq On : 25 Mar 2015 00:46
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 25 00:51:55 2015

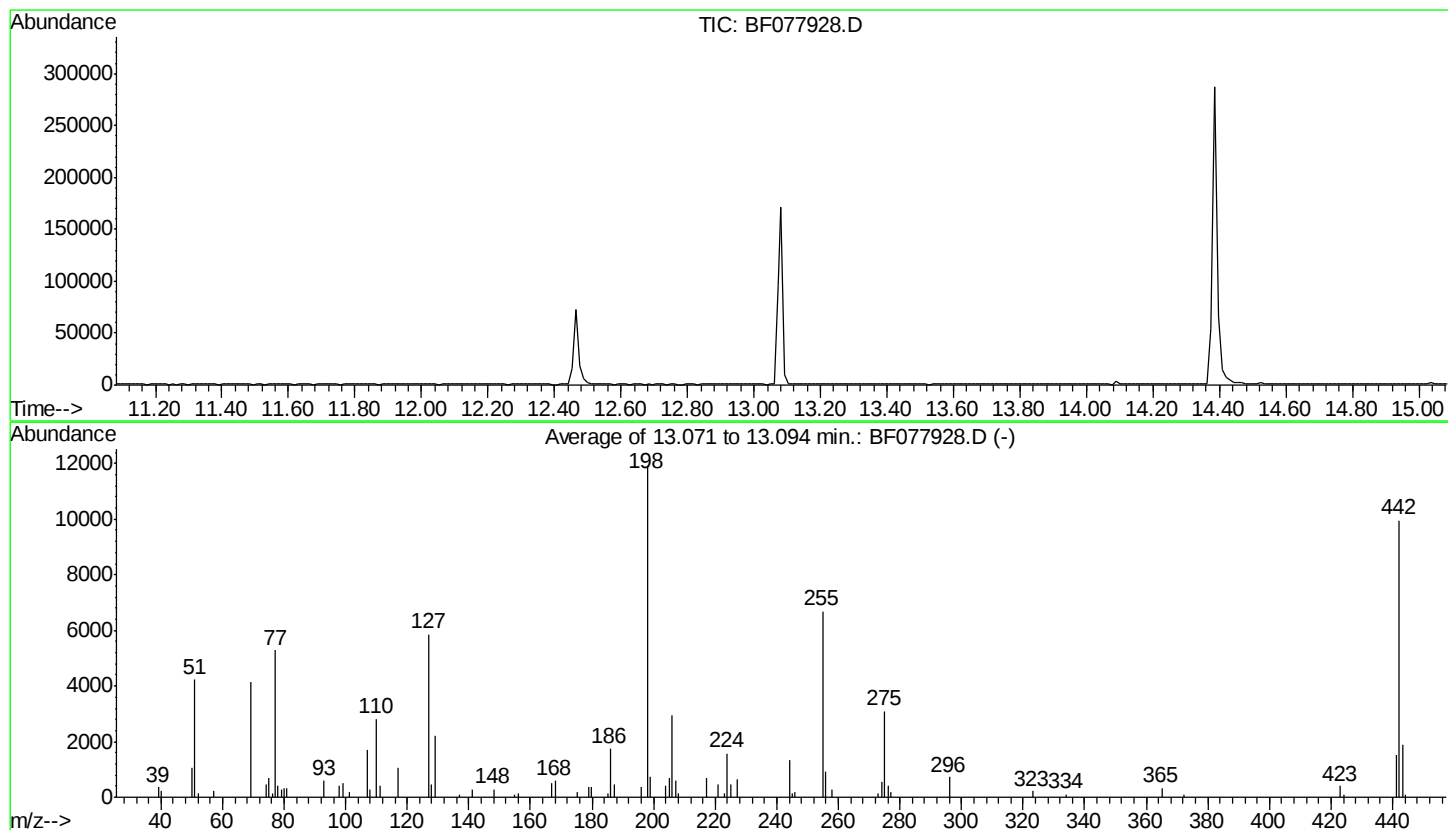

AutoFind: Scans 1066, 1067, 1068; Background Corrected with Scan 1063

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	4214	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	4123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	5861	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11925	PASS
199	198	5	9	6.1	723	PASS
275	198	10	60	26.0	3099	PASS
365	198	1	100	2.7	325	PASS
441	442	0.01	24	15.2	1518	PASS
442	198	50	100	83.5	9957	PASS
443	442	15	24	19.1	1899	PASS