
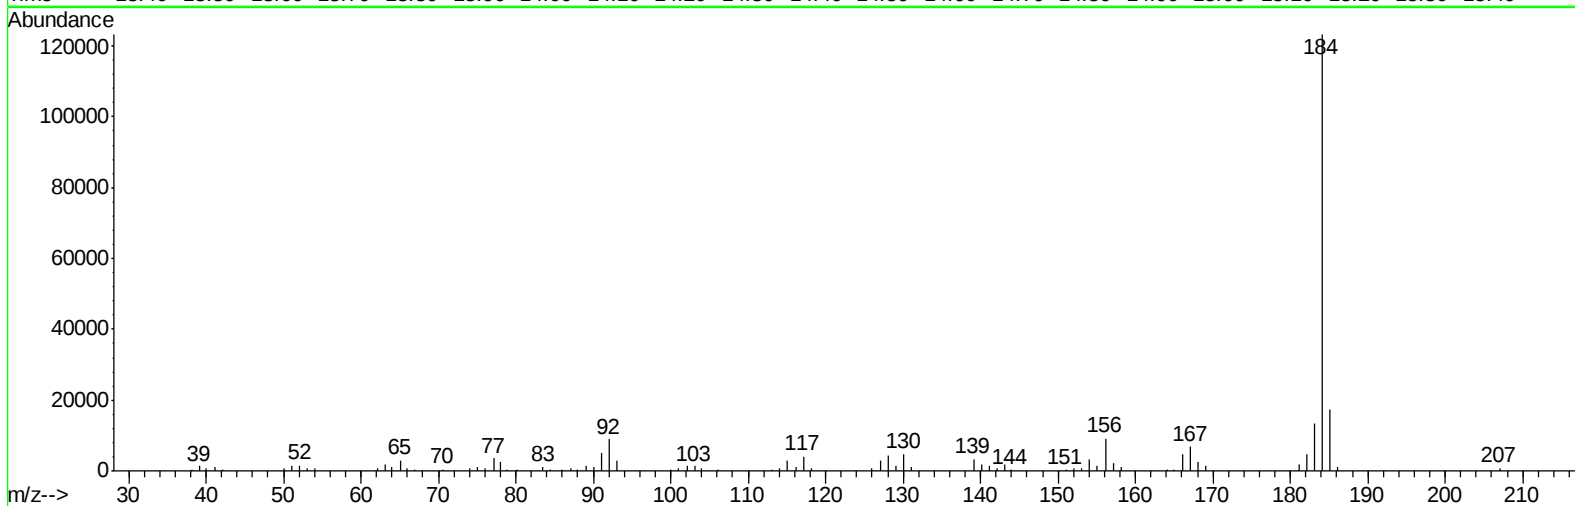


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
Data File : BF077928.D
Acq On : 25 Mar 2015 00:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 07:47:26 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 19 02:09:19 2015
Response via : Initial Calibration

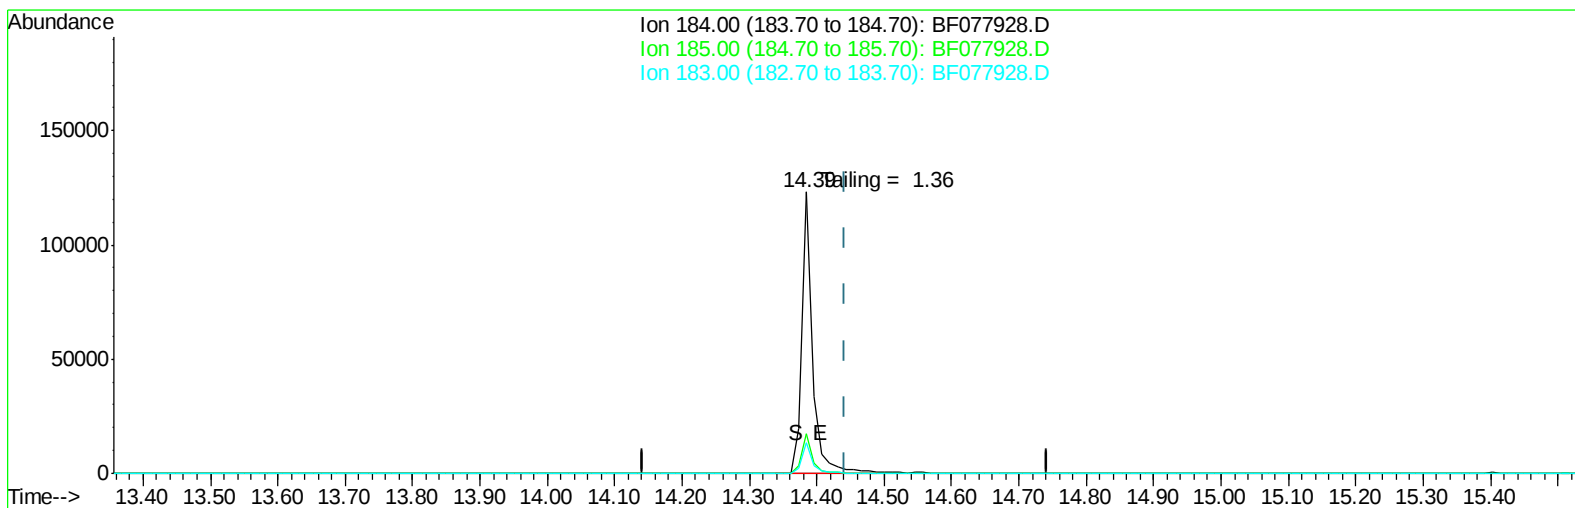

TIC: BF077928.D

(76) Benzidine



14.385min (-0.057) 0.00ng

response 137248

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.18
183.00	11.10	10.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
Data File : BF077928.D
Acq On : 25 Mar 2015 00:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 07:47:26 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 19 02:09:19 2015
Response via : Initial Calibration

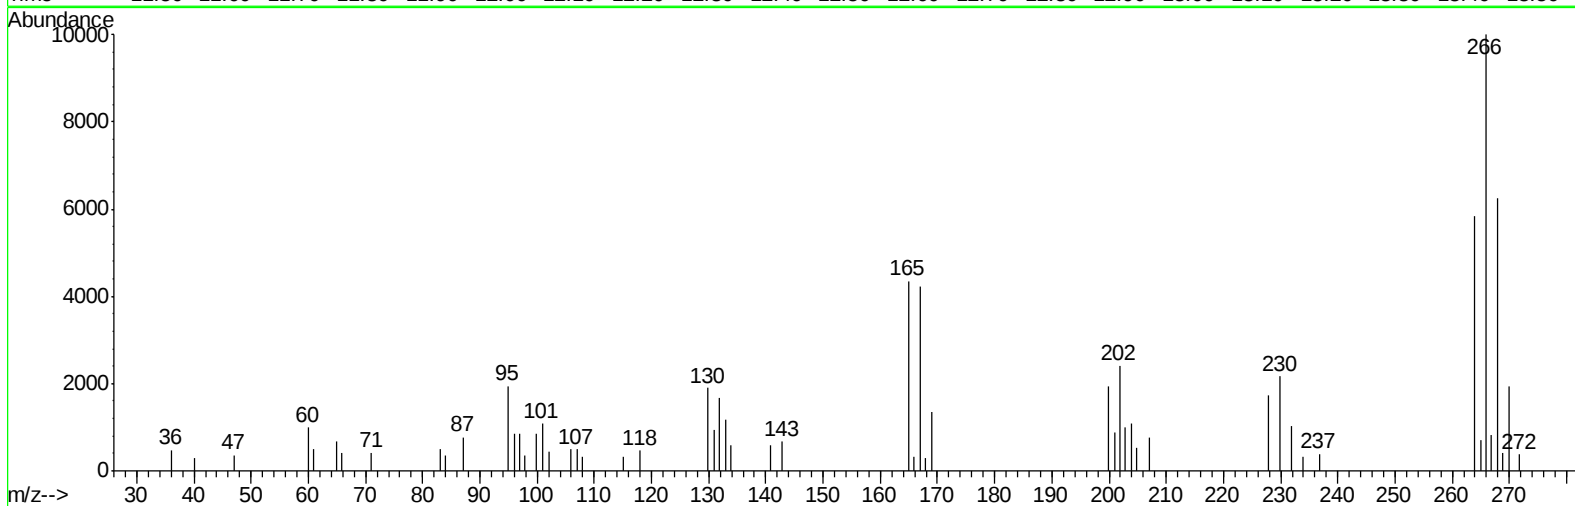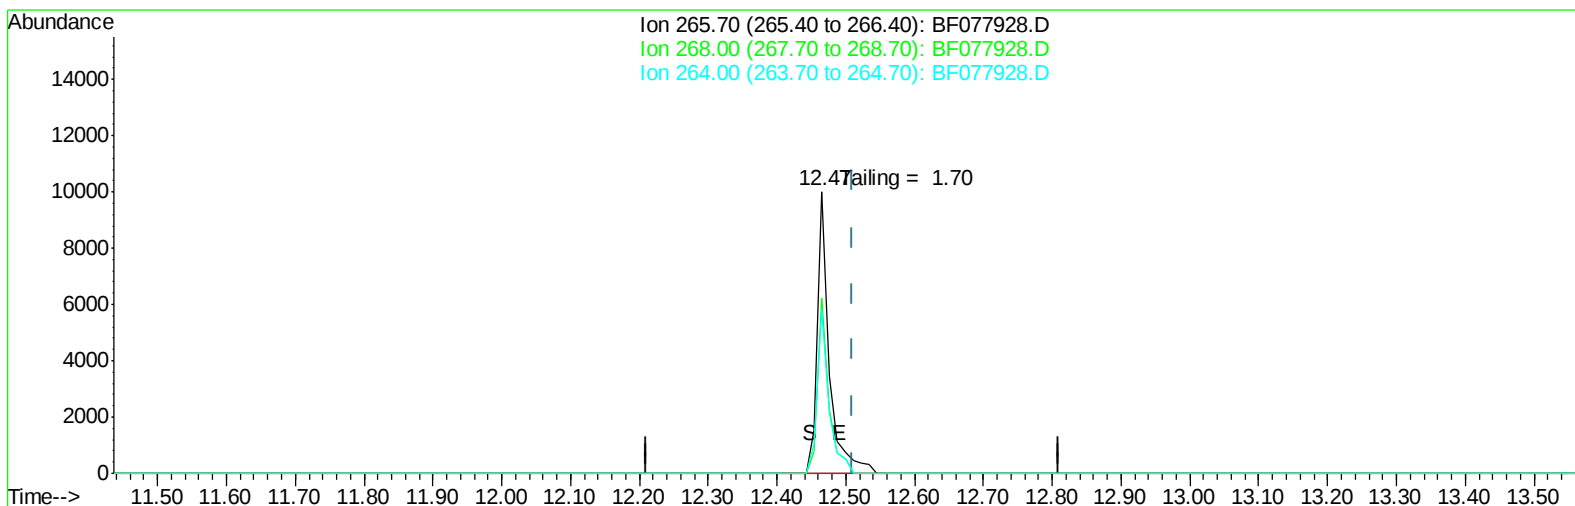

TIC: BF077928.D

(69) Pentachlorophenol (C)

12.465min (-0.046) 0.00ng

response 12343

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.42
264.00	61.20	58.35
0.00	0.00	0.00