

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
 Data File : BF077926.D
 Acq On : 24 Mar 2015 22:13
 Operator : TP/IZ
 Sample : G1613-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-5-2

Quant Time: Mar 25 02:04:11 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 25 00:51:55 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.12	152	43233	20.00	ng	0.00
21) Naphthalene-d8	8.69	136	180995	20.00	ng	0.00
38) Acenaphthene-d10	10.86	164	90573	20.00	ng	0.00
63) Phenanthrene-d10	12.69	188	178325	20.00	ng	0.00
75) Chrysene-d12	16.00	240	198182	20.00	ng	0.02
86) Perylene-d12	17.81	264	182535	20.00	ng	0.11
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	246419	99.49	ng	0.00
7) Phenol-d6	6.69	99	322544	105.40	ng	0.00
23) Nitrobenzene-d5	7.81	82	172738	62.56	ng	0.00
41) 2,4,6-Tribromophenol	11.84	330	72777	83.98	ng	0.00
44) 2-Fluorobiphenyl	10.04	172	415006	67.34	ng	0.00
78) Terphenyl-d14	14.69	244	502575	61.94	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
Data File : BF077926.D
Acq On : 24 Mar 2015 22:13
Operator : TP/IZ
Sample : G1613-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-5-2

Quant Time: Mar 25 02:04:11 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 25 00:51:55 2015
Response via : Initial Calibration

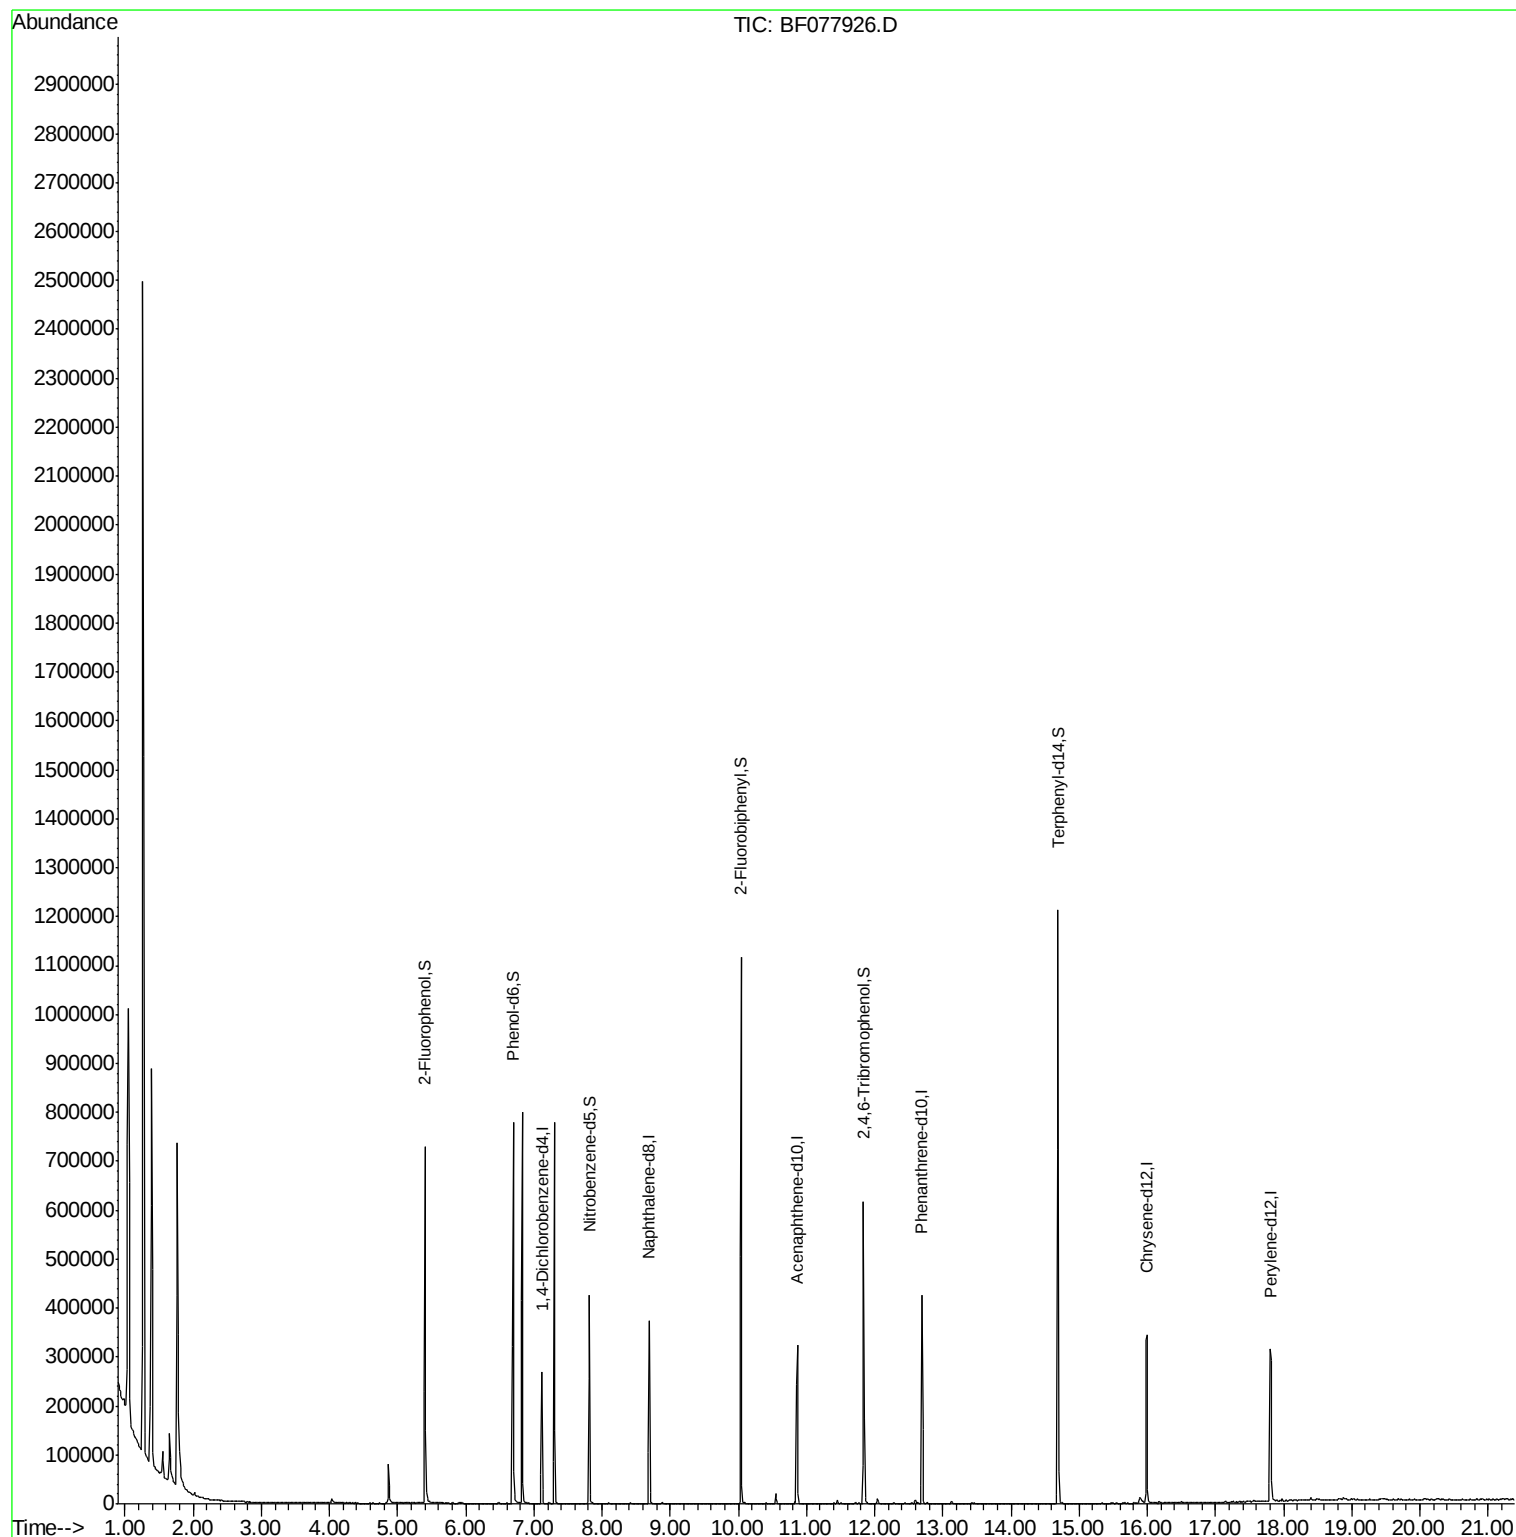

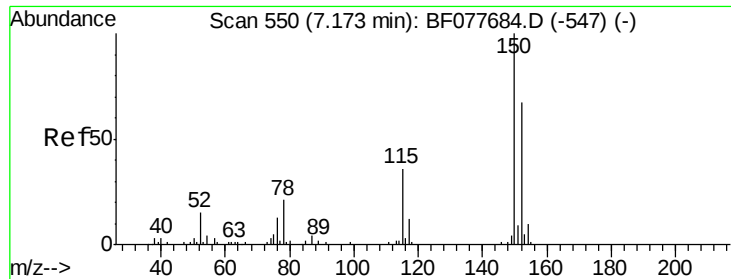


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.12 min Scan# 545
Delta R.T. -0.00 min
Lab File: BF077926.D
Acq: 24 Mar 2015 22:13

Instrument :
BNA_F
ClientSampleId :
SB-5-2

Tgt Ion:152 Resp: 43233
Ion Ratio Lower Upper
152 100
150 156.4 119.5 179.3
115 57.0 43.0 64.4

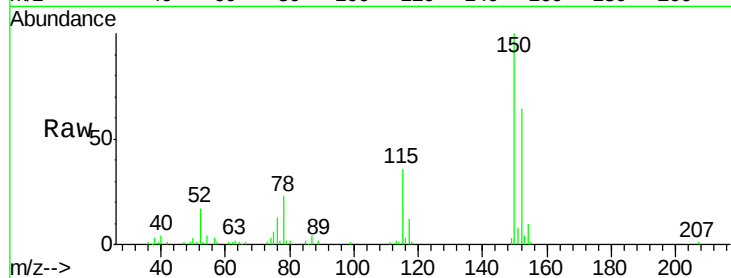


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

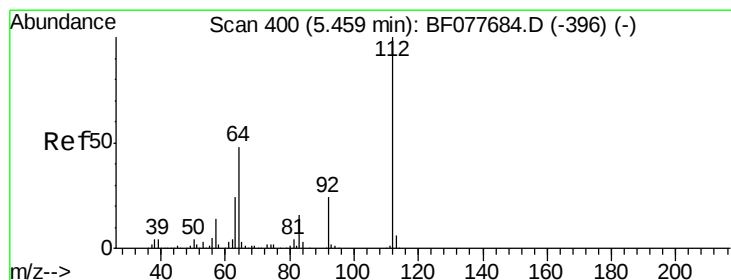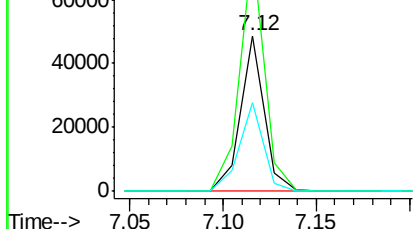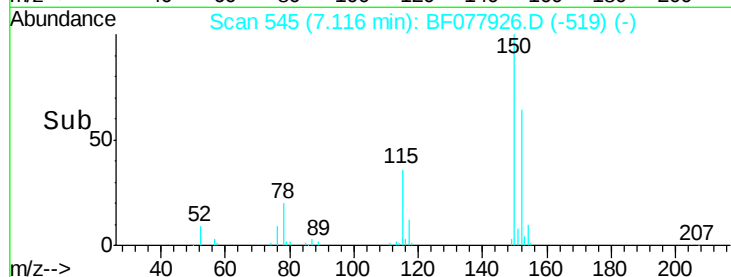



#5


2-Fluorophenol
Concen: 99.49 ng
RT: 5.40 min Scan# 395
Delta R.T. -0.00 min
Lab File: BF077926.D
Acq: 24 Mar 2015 22:13

Tgt Ion:112 Resp: 246419
Ion Ratio Lower Upper
112 100
64 52.5 38.6 57.8
63 26.7 19.3 28.9

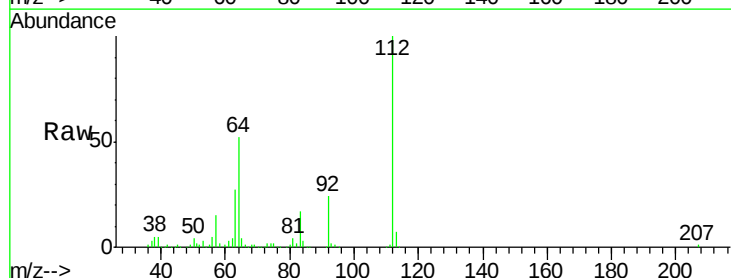

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

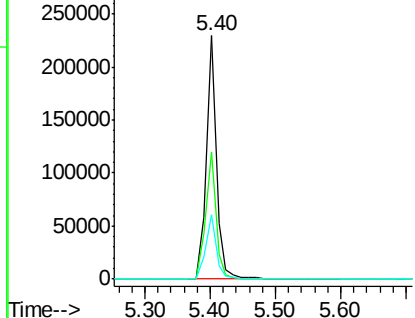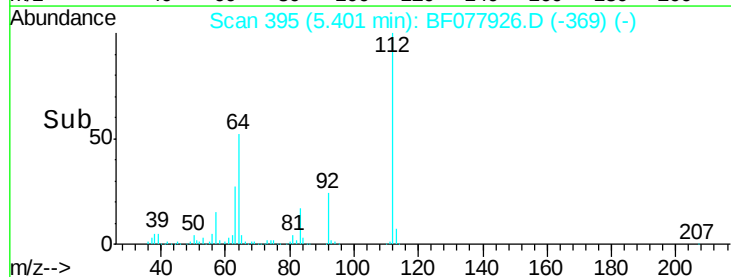

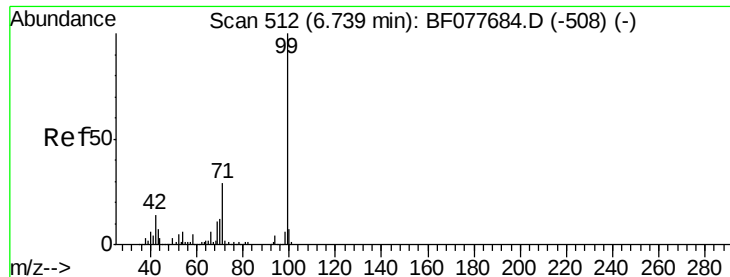

#7

Phenol-d6

Concen: 105.40 ng

RT: 6.69 min Scan# 508

Delta R.T. -0.00 min

Lab File: BF077926.D

Acq: 24 Mar 2015 22:13

Instrument :

BNA_F

ClientSampleId :

SB-5-2


Tgt Ion: 99 Resp: 322544

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.4

71 29.6 23.4 35.2



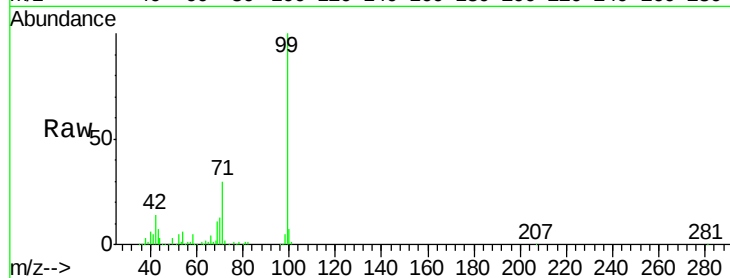


Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

Time-->

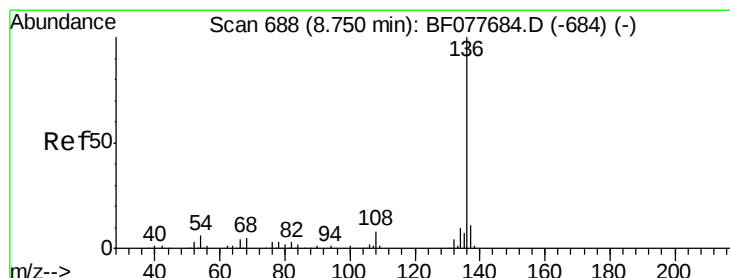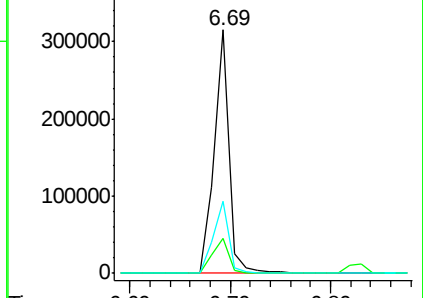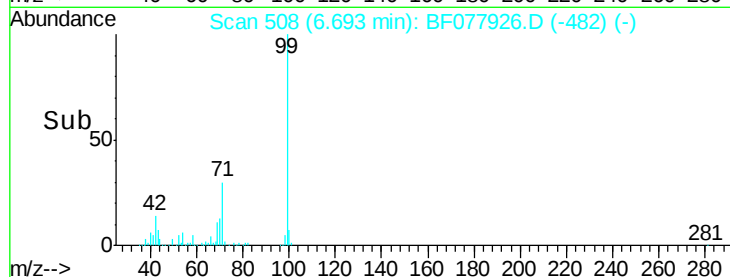

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.69 min Scan# 683

Delta R.T. -0.00 min

Lab File: BF077926.D

Acq: 24 Mar 2015 22:13

Tgt Ion: 136 Resp: 180995


Ion Ratio Lower Upper

136 100

137 10.6 8.7 13.1

54 6.1 4.6 6.8

68 5.2 3.7 5.5

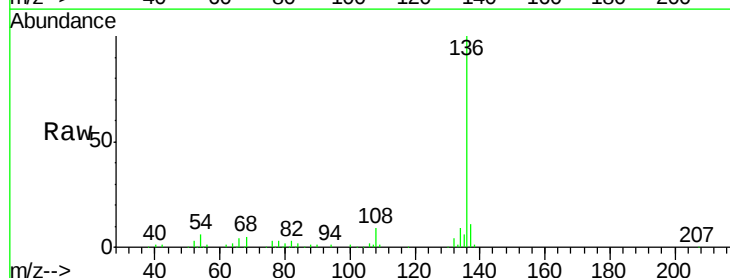



Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

Time-->



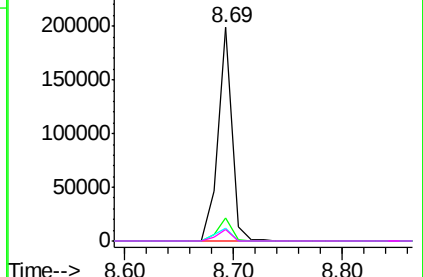
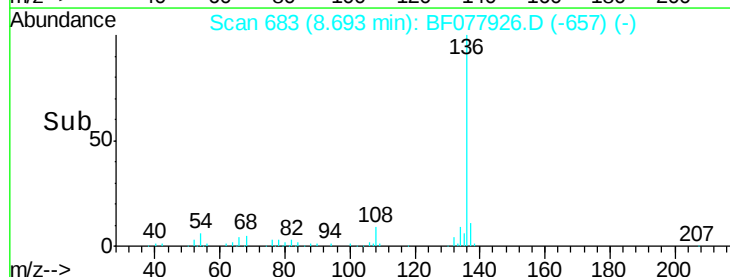


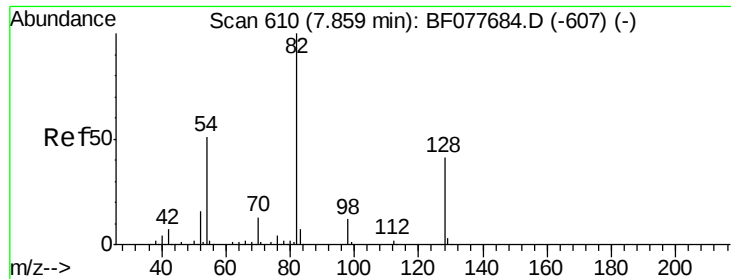

#23
 Nitrobenzene-d5
 Concen: 62.56 ng
 RT: 7.81 min Scan# 606
 Delta R.T. -0.00 min
 Lab File: BF077926.D
 Acq: 24 Mar 2015 22:13




Instrument :
 BNA_F
 ClientSampleId :
 SB-5-2

Tgt Ion: 82 Resp: 172738
 Ion Ratio Lower Upper
 82 100
 128 52.5 32.8 49.2#
 54 43.1 40.6 60.8

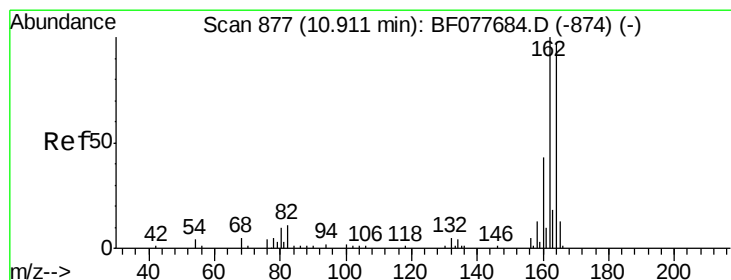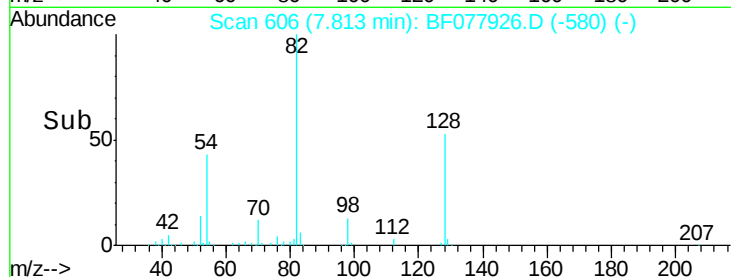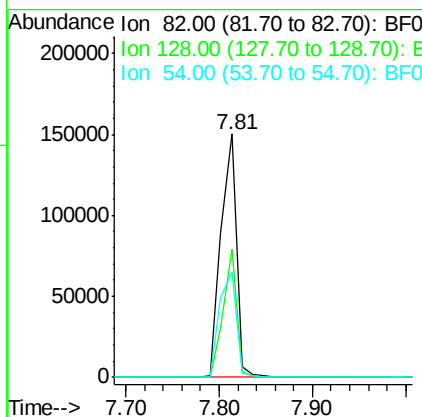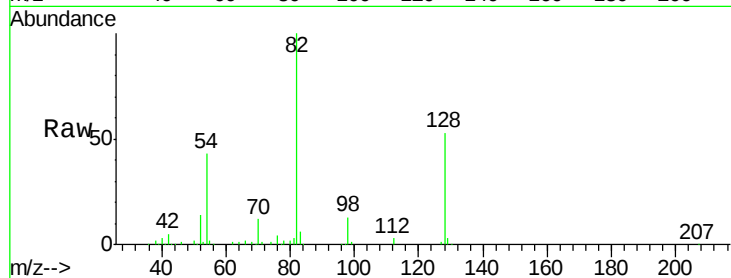

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.86 min Scan# 873
 Delta R.T. -0.00 min
 Lab File: BF077926.D
 Acq: 24 Mar 2015 22:13

Tgt Ion: 164 Resp: 90573
 Ion Ratio Lower Upper
 164 100
 162 106.7 82.4 123.6
 160 45.1 35.8 53.6

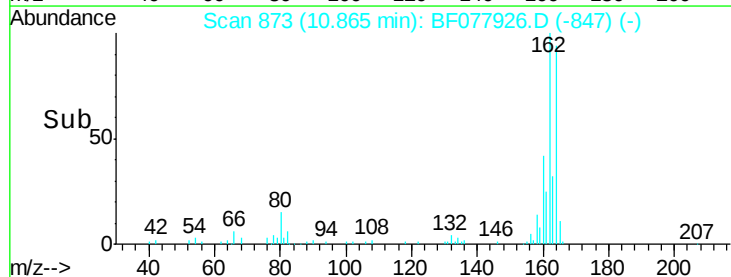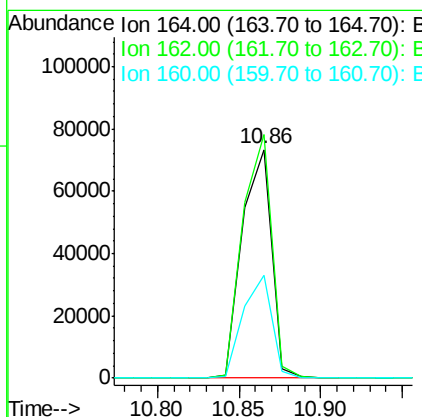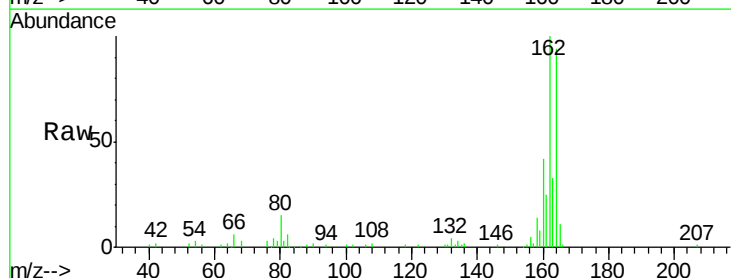







#41
 2,4,6-Tribromophenol
 Concen: 83.98 ng
 RT: 11.84 min Scan# 958
 Delta R.T. -0.00 min
 Lab File: BF077926.D
 Acq: 24 Mar 2015 22:13

Instrument :
 BNA_F
 ClientSampleId :
 SB-5-2

Tgt Ion:330 Resp: 72777
 Ion Ratio Lower Upper
 330 100
 332 96.6 0.0 0.0#
 141 40.4 0.0 0.0#

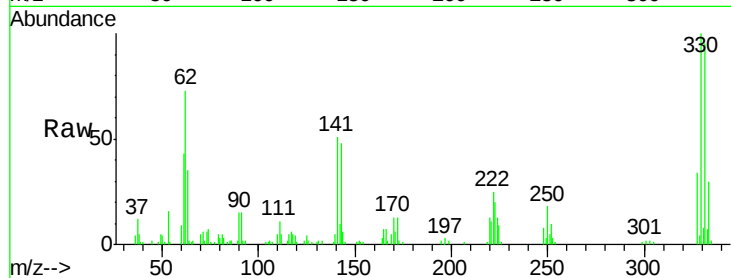


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

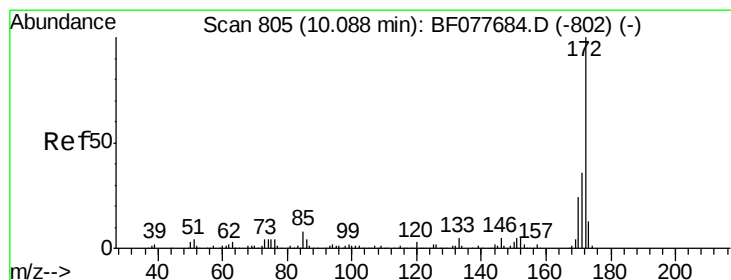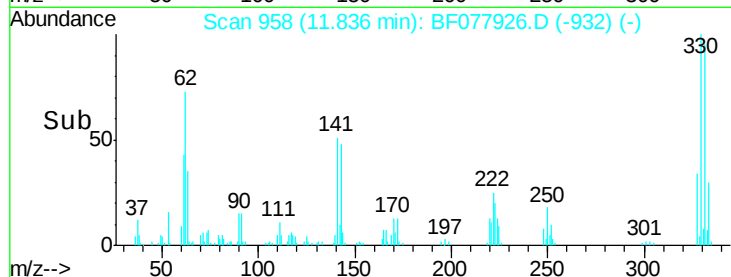
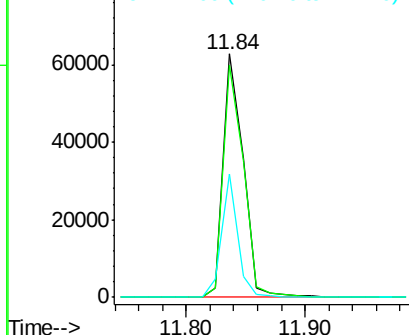



#44
 2-Fluorobiphenyl
 Concen: 67.34 ng
 RT: 10.04 min Scan# 801
 Delta R.T. -0.00 min
 Lab File: BF077926.D
 Acq: 24 Mar 2015 22:13

Tgt Ion:172 Resp: 415006
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.5 42.7
 170 23.5 18.8 28.2

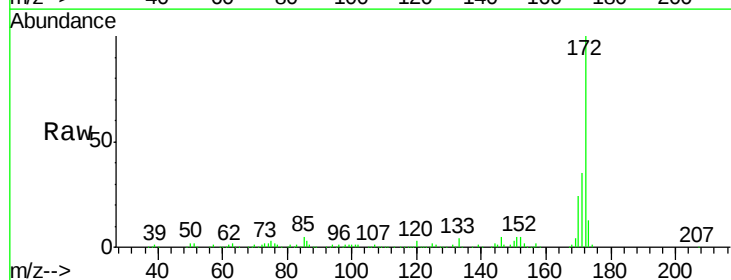

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



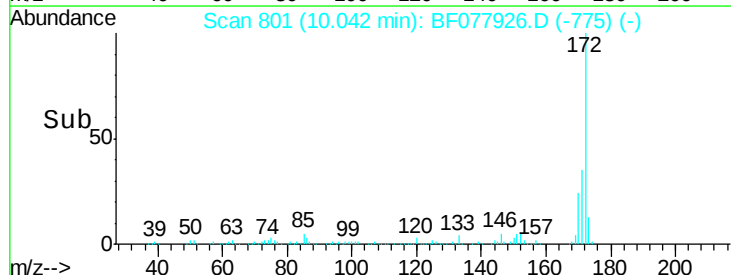
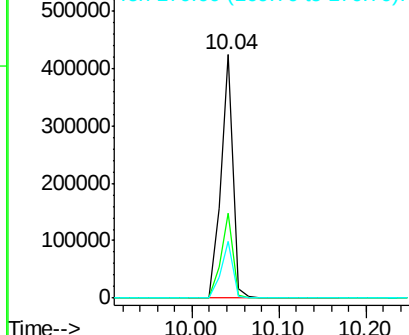


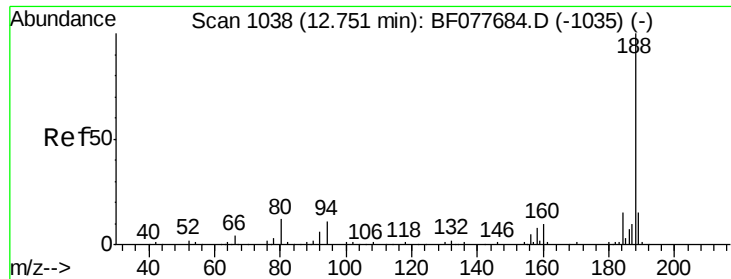

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.69 min Scan# 1033
Delta R.T. -0.00 min
Lab File: BF077926.D
Acq: 24 Mar 2015 22:13




Instrument :
BNA_F
ClientSampleId :
SB-5-2


Tgt Ion:188 Resp: 178325
Ion Ratio Lower Upper
188 100
94 10.6 8.7 13.1
80 11.7 9.3 13.9

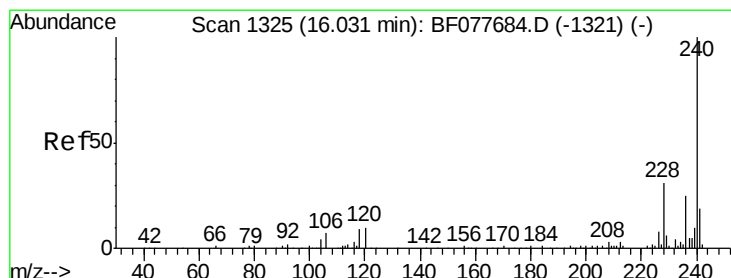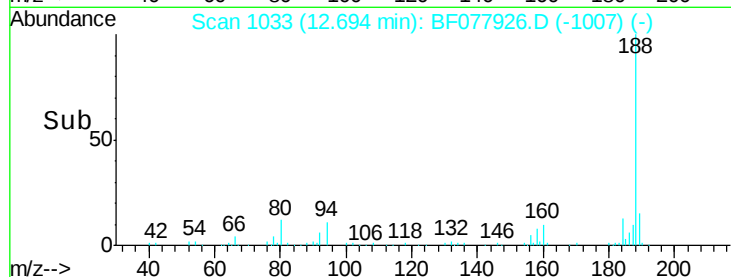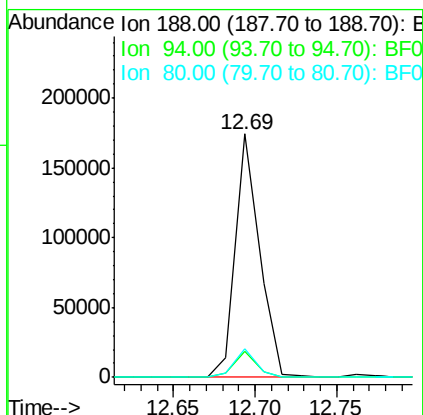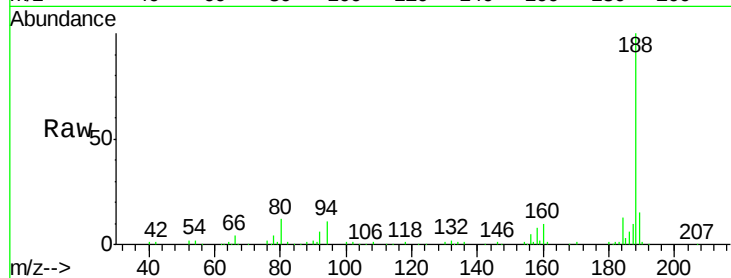

#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.00 min Scan# 1322
Delta R.T. 0.02 min
Lab File: BF077926.D
Acq: 24 Mar 2015 22:13

Tgt Ion:240 Resp: 198182
Ion Ratio Lower Upper
240 100
120 8.8 8.2 12.2
236 25.1 20.0 30.0


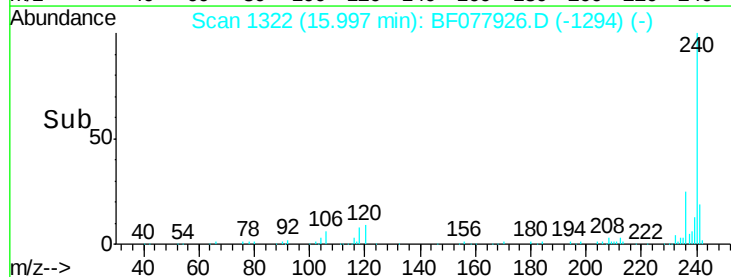
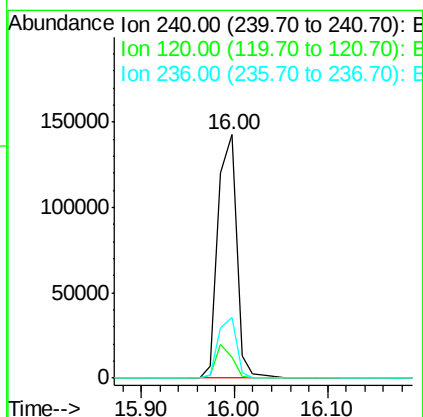
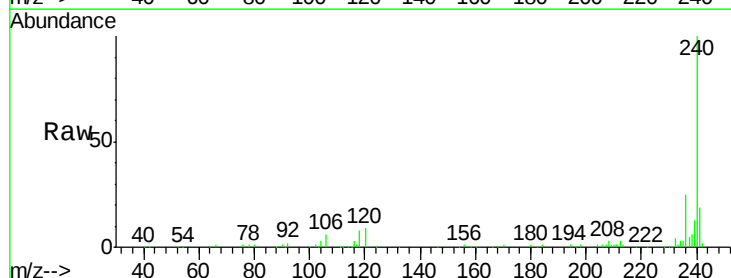


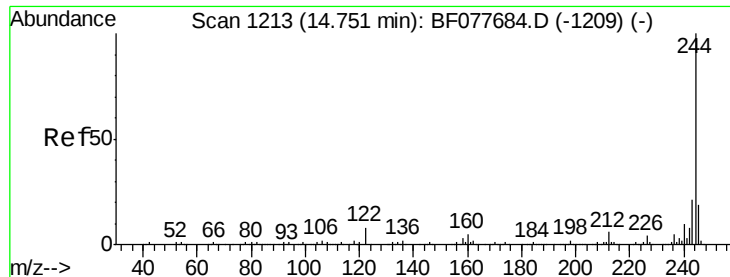

#78
 Terphenyl-d14
 Concen: 61.94 ng
 RT: 14.69 min Scan# 1208
 Delta R.T. -0.00 min
 Lab File: BF077926.D
 Acq: 24 Mar 2015 22:13

Instrument :
 BNA_F
 ClientSampleId :
 SB-5-2

Tgt Ion: 244 Resp: 502575
 Ion Ratio Lower Upper
 244 100
 212 6.2 4.9 7.3
 122 9.1 6.2 9.4

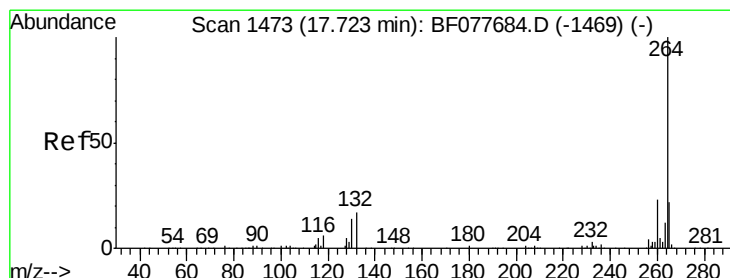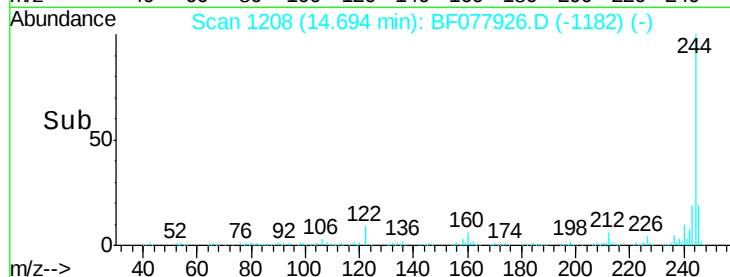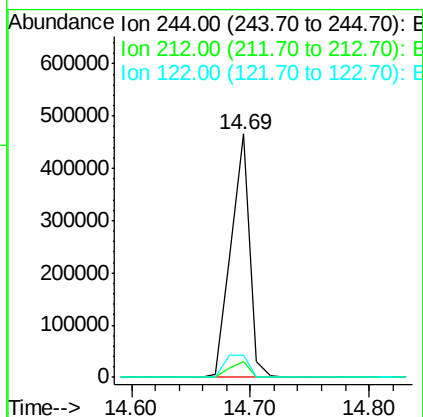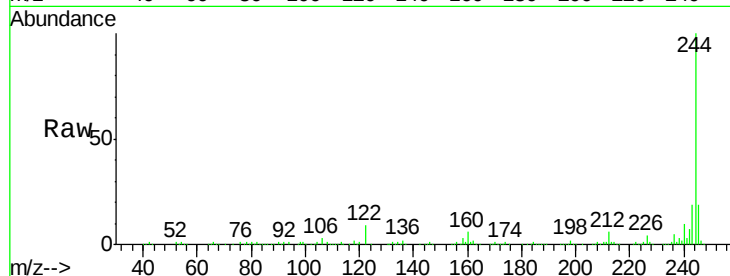

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.81 min Scan# 1481
 Delta R.T. 0.11 min
 Lab File: BF077926.D
 Acq: 24 Mar 2015 22:13

Tgt Ion: 264 Resp: 182535
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.6 27.8
 265 20.7 17.3 25.9

