

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
 Data File : BF077948.D
 Acq On : 25 Mar 2015 10:45
 Operator : TP/IZ
 Sample : G1613-20
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-14

Quant Time: Mar 25 11:37:19 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 25 11:05:58 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.12	152	43488	20.00	ng	0.00
21) Naphthalene-d8	8.69	136	183894	20.00	ng	0.00
38) Acenaphthene-d10	10.87	164	91087	20.00	ng	0.00
63) Phenanthrene-d10	12.71	188	174083	20.00	ng	0.01
75) Chrysene-d12	15.97	240	192799	20.00	ng	-0.01
86) Perylene-d12	17.70	264	191694	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	220918	88.67	ng	0.01
7) Phenol-d6	6.70	99	289604	94.08	ng	0.01
23) Nitrobenzene-d5	7.81	82	162476	57.92	ng	0.00
41) 2,4,6-Tribromophenol	11.85	330	71649	82.21	ng	0.01
44) 2-Fluorobiphenyl	10.04	172	367944	59.36	ng	0.00
78) Terphenyl-d14	14.69	244	428696	54.31	ng	0.00
Target Compounds						
49) Dimethylphthalate	10.56	163	21766	3.22	ng	# 96
83) Bis(2-ethylhexyl)phthalate	16.03	149	16346	2.26	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
Data File : BF077948.D
Acq On : 25 Mar 2015 10:45
Operator : TP/IZ
Sample : G1613-20
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-14

Quant Time: Mar 25 11:37:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 25 11:05:58 2015
Response via : Initial Calibration

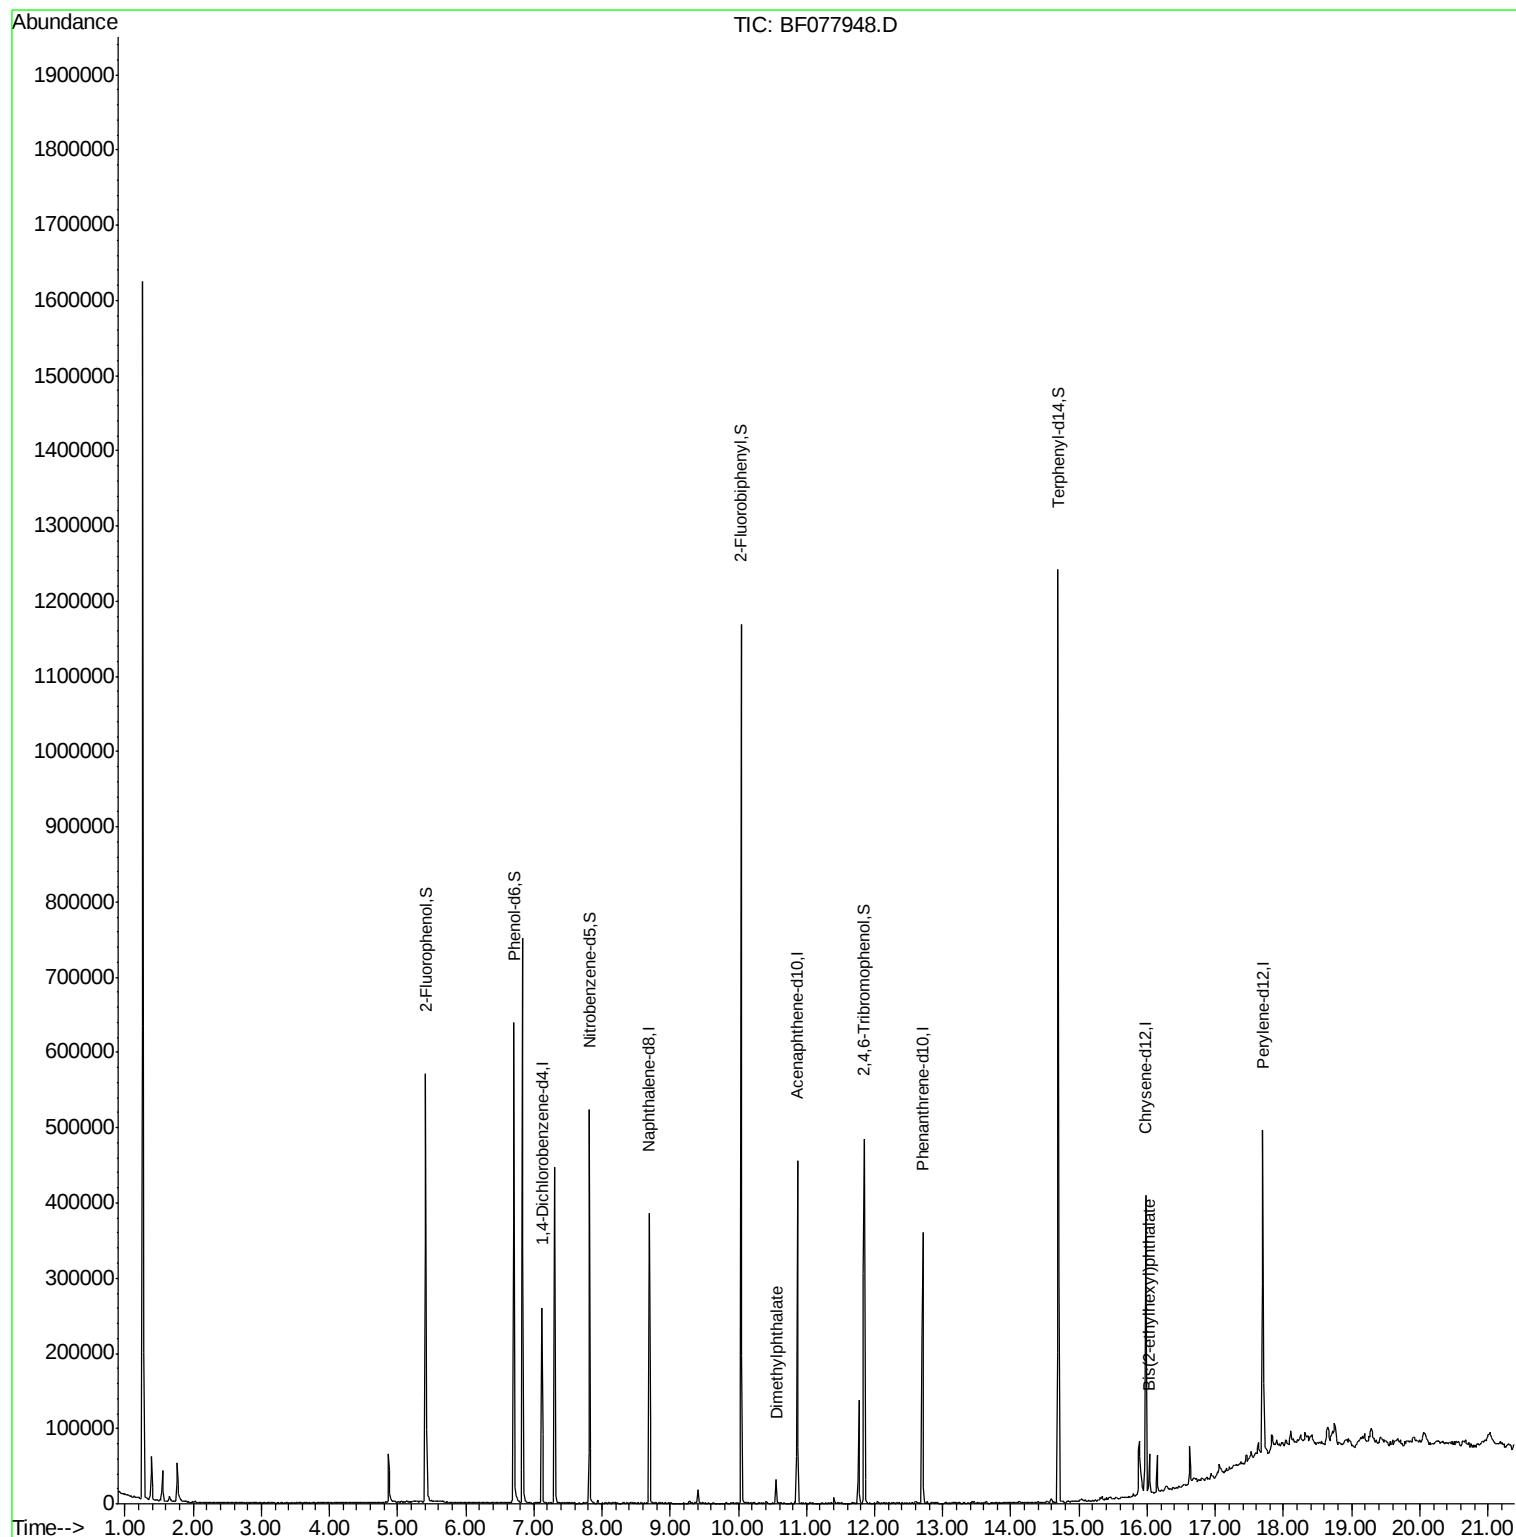

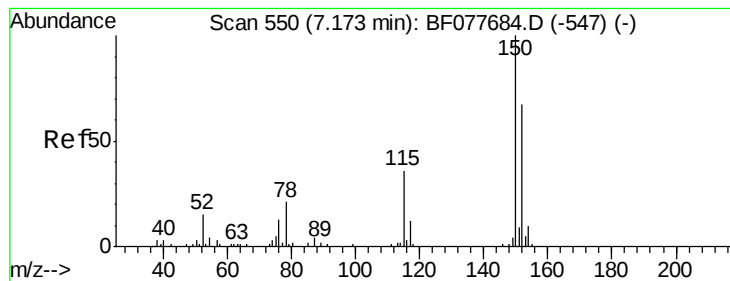


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.12 min Scan# 545
 Delta R.T. 0.00 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45

Instrument :
 BNA_F
 ClientSampleId :
 SB-14

Tgt Ion:152 Resp: 43488
 Ion Ratio Lower Upper
 152 100
 150 160.2 119.5 179.3
 115 63.8 43.0 64.4

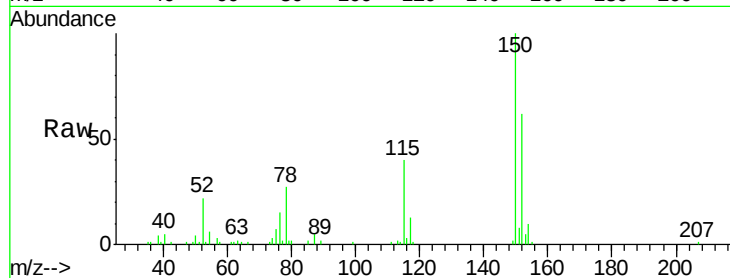


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

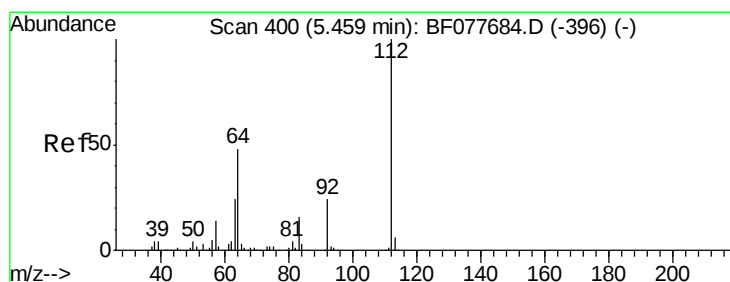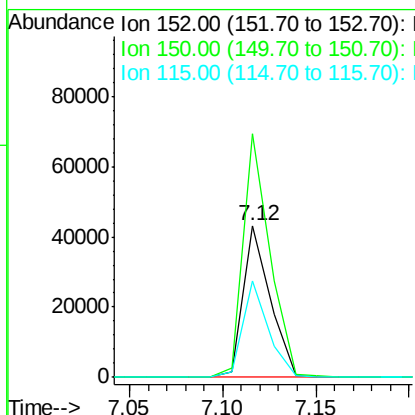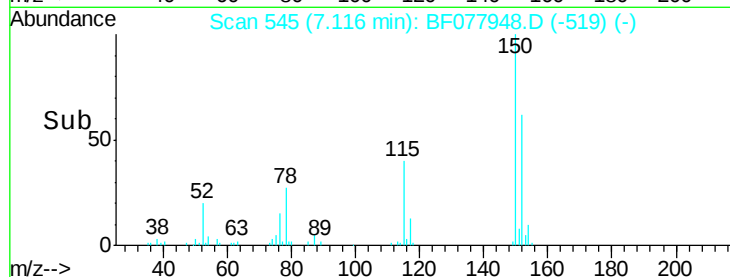



#5


2-Fluorophenol
 Concen: 88.67 ng
 RT: 5.41 min Scan# 396
 Delta R.T. 0.01 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45

Tgt Ion:112 Resp: 220918
 Ion Ratio Lower Upper
 112 100
 64 51.2 38.6 57.8
 63 26.6 19.3 28.9

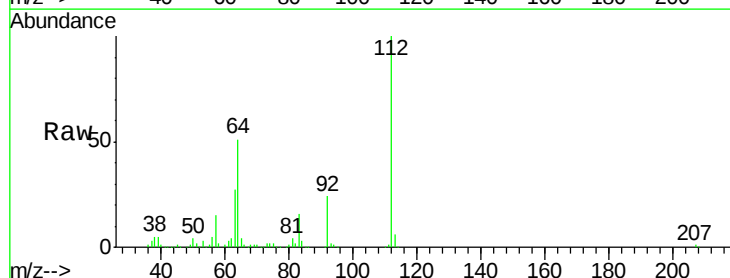

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

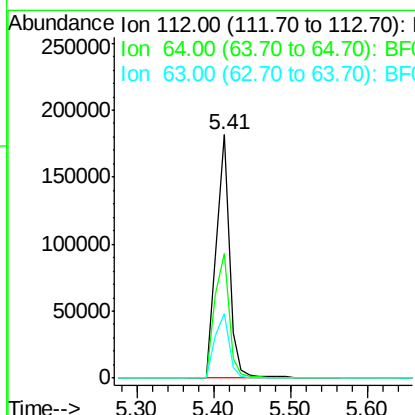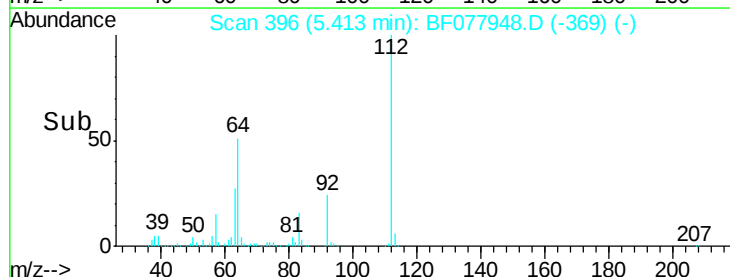

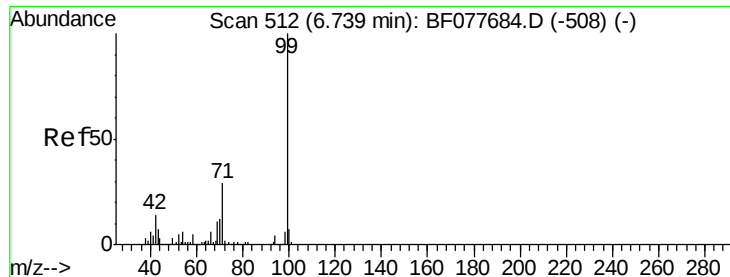

#7

Phenol-d6

Concen: 94.08 ng

RT: 6.70 min Scan# 509

Delta R.T. 0.01 min

Lab File: BF077948.D

Acq: 25 Mar 2015 10:45

Instrument :

BNA_F

ClientSampleId :

SB-14





Tgt Ion: 99 Resp: 289604

Ion Ratio Lower Upper

99 100

42 14.3 11.0 16.4

71 29.8 23.4 35.2

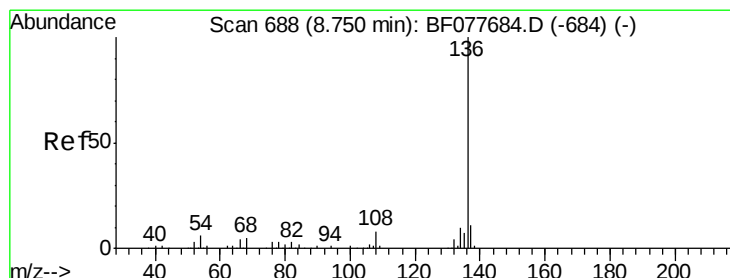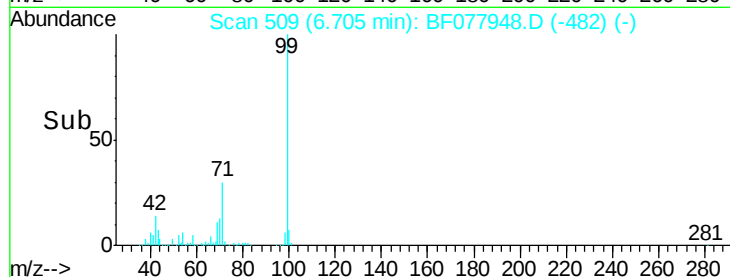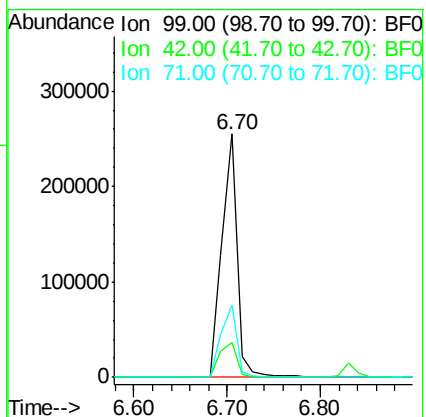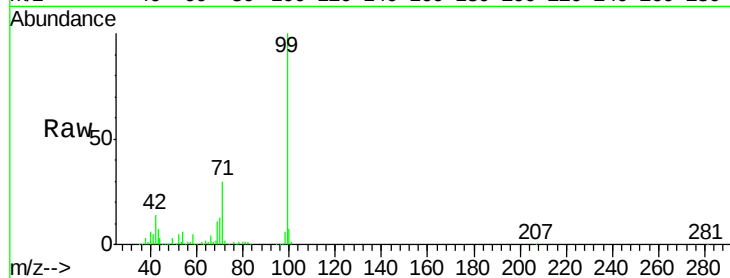

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.69 min Scan# 683

Delta R.T. 0.00 min

Lab File: BF077948.D

Acq: 25 Mar 2015 10:45

Tgt Ion: 136 Resp: 183894




Ion Ratio Lower Upper


136 100

137 10.9 8.7 13.1

54 7.8 4.6 6.8#

68 6.0 3.7 5.5#


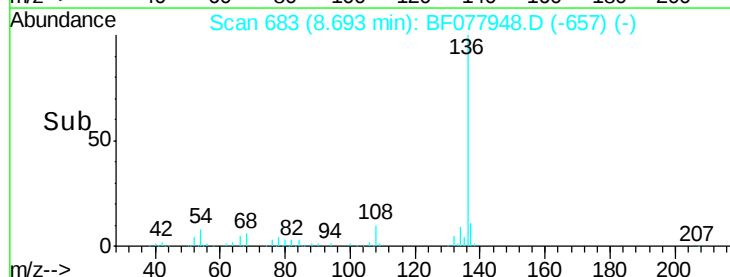
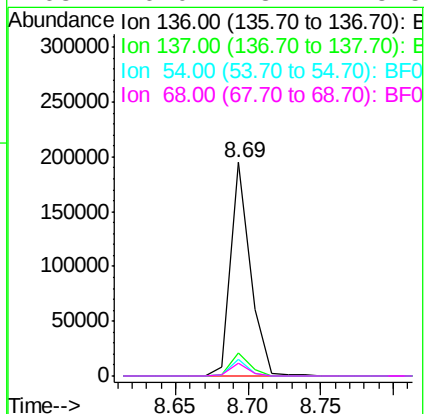
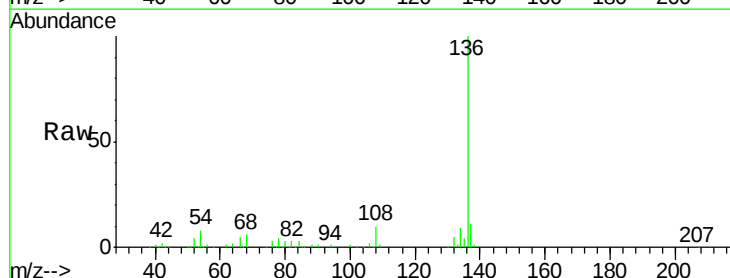


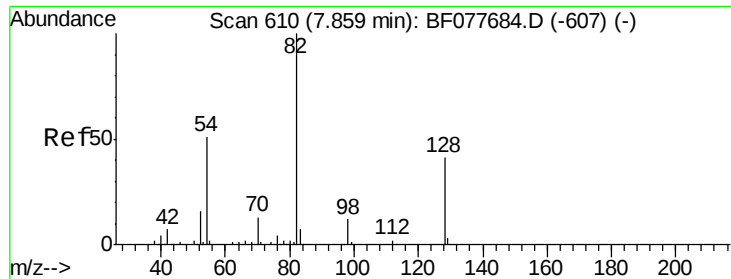

#23
 Nitrobenzene-d5
 Concen: 57.92 ng
 RT: 7.81 min Scan# 606
 Delta R.T. 0.00 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45




Instrument :
 BNA_F
 ClientSampled :
 SB-14

Tgt Ion: 82 Resp: 162476
 Ion Ratio Lower Upper
 82 100
 128 44.1 32.8 49.2
 54 48.5 40.6 60.8

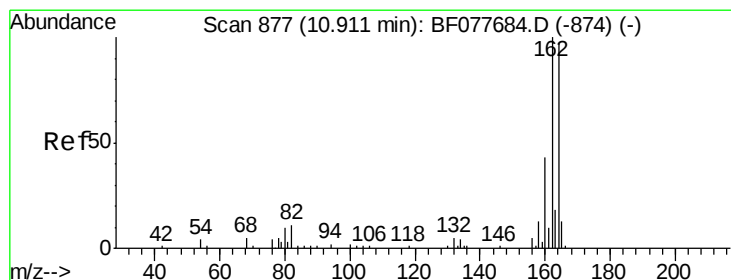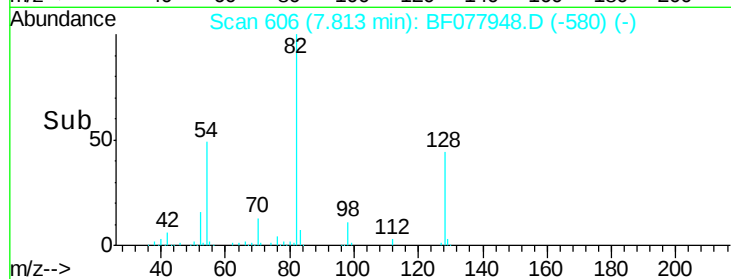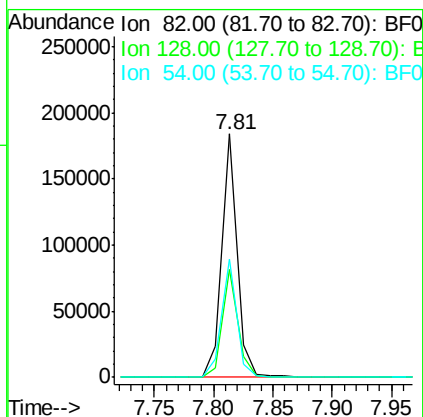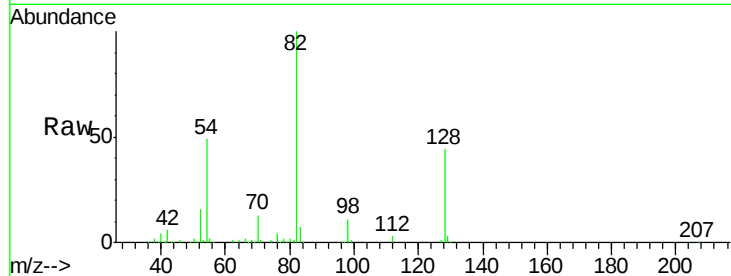

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.87 min Scan# 873
 Delta R.T. 0.00 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45

Tgt Ion: 164 Resp: 91087
 Ion Ratio Lower Upper
 164 100
 162 105.2 82.4 123.6
 160 45.2 35.8 53.6


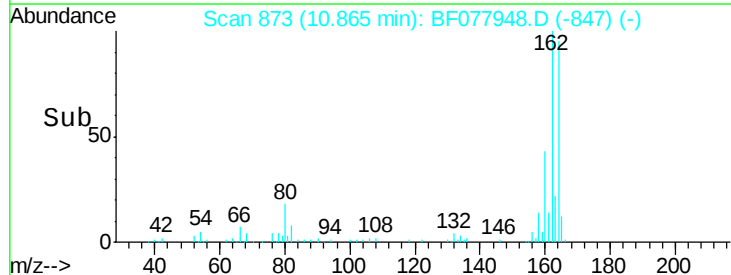
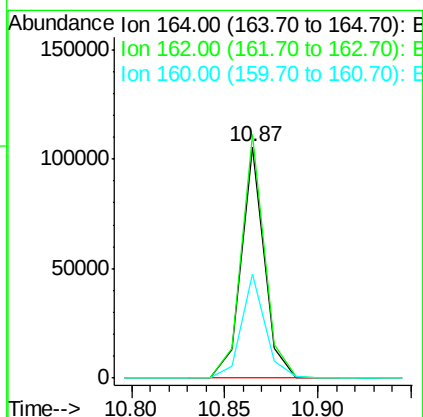
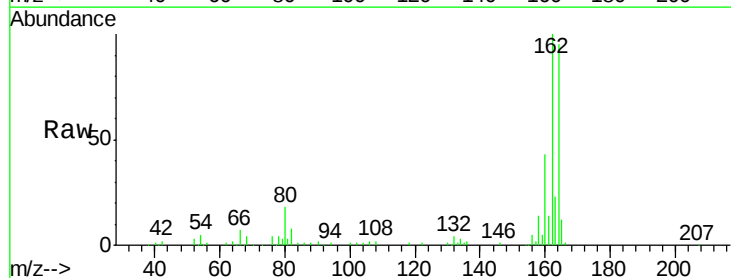




#41
 2,4,6-Tribromophenol
 Concen: 82.21 ng
 RT: 11.85 min Scan# 959
 Delta R.T. 0.01 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45




Instrument :
 BNA_F
 ClientSampled :
 SB-14


Tgt Ion:330 Resp: 71649
 Ion Ratio Lower Upper
 330 100
 332 95.0 0.0 0.0#
 141 36.6 0.0 0.0#

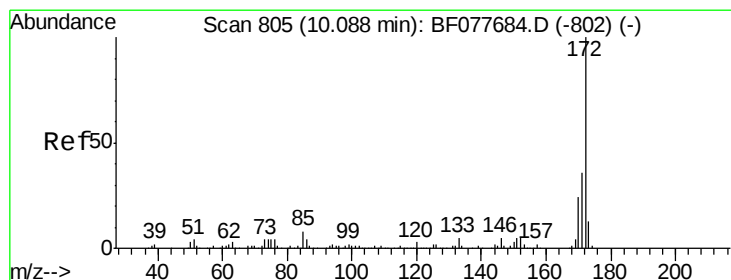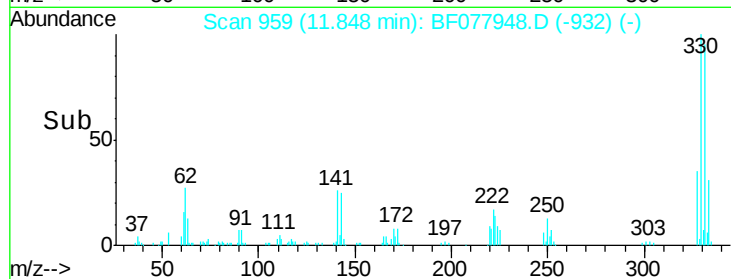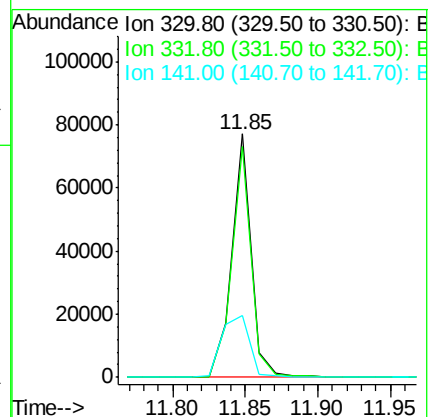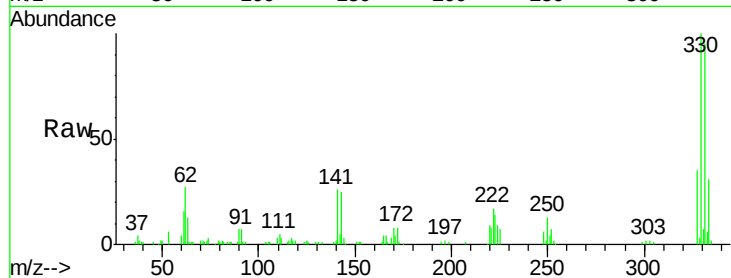

#44
 2-Fluorobiphenyl
 Concen: 59.36 ng
 RT: 10.04 min Scan# 801
 Delta R.T. 0.00 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45

Tgt Ion:172 Resp: 367944
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.5 42.7
 170 23.8 18.8 28.2

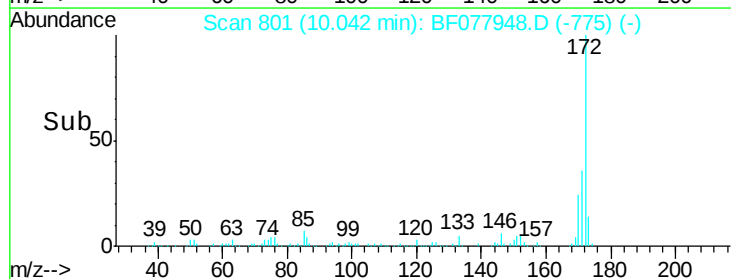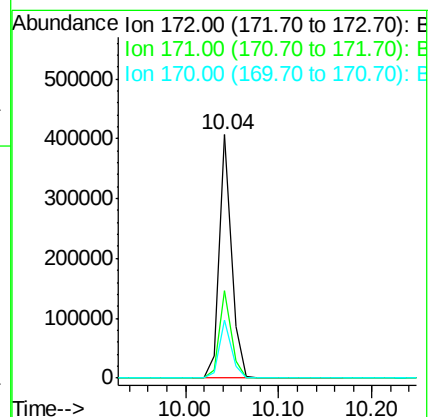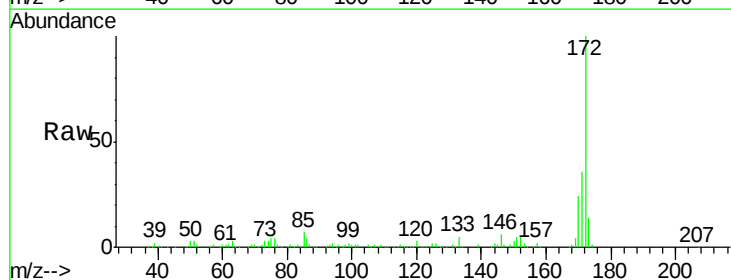

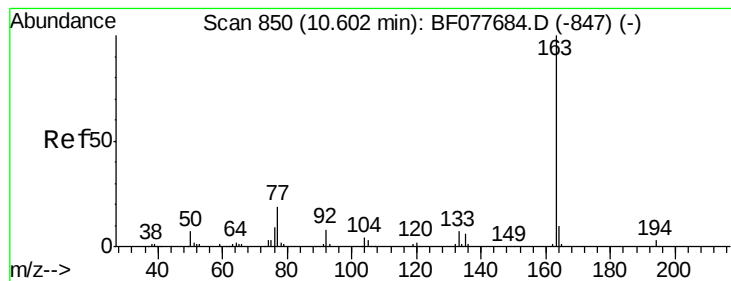

#49

Dimethylphthalate

Concen: 3.22 ng

RT: 10.56 min Scan# 846

Delta R.T. 0.00 min

Lab File: BF077948.D

Acq: 25 Mar 2015 10:45

Instrument :

BNA_F

ClientSampleId :

SB-14


Tgt Ion:163 Resp: 21766

Ion Ratio Lower Upper

163 100

194 4.4 2.7 4.1#




164 8.6 8.2 12.2

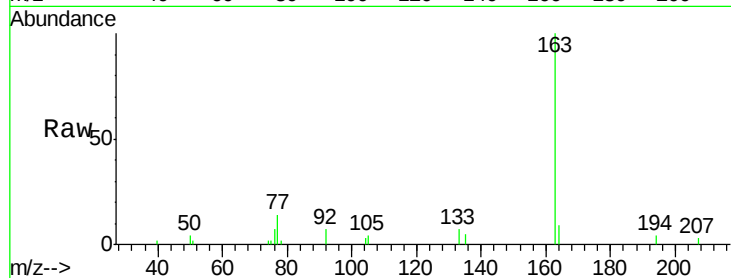

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

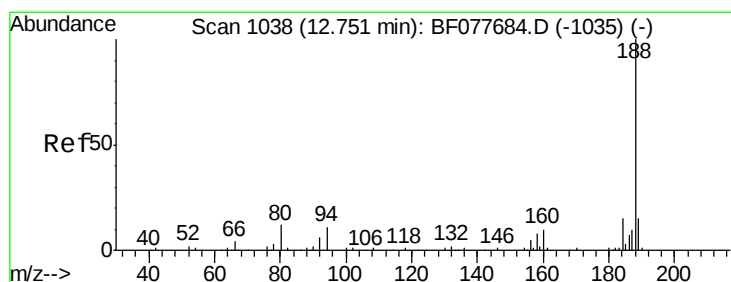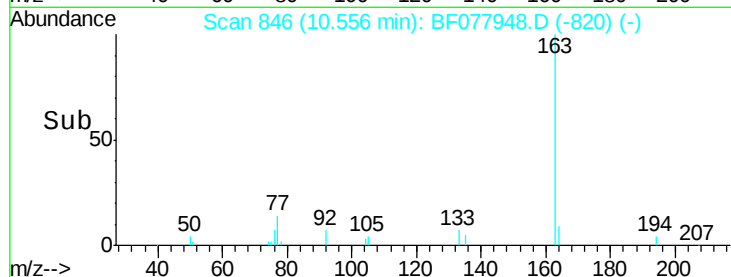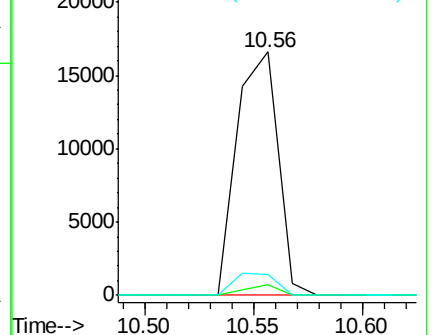

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.71 min Scan# 1034

Delta R.T. 0.01 min

Lab File: BF077948.D

Acq: 25 Mar 2015 10:45


Tgt Ion:188 Resp: 174083

Ion Ratio Lower Upper

188 100

94 7.4 8.7 13.1#



80 7.7 9.3 13.9#

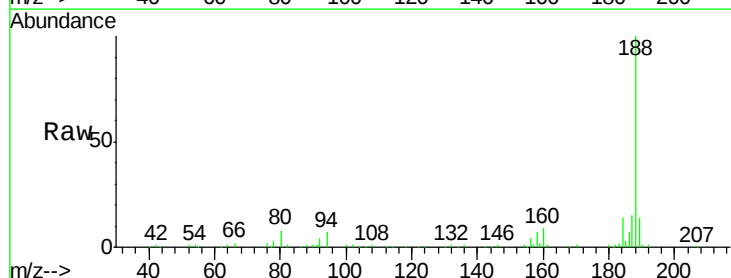


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

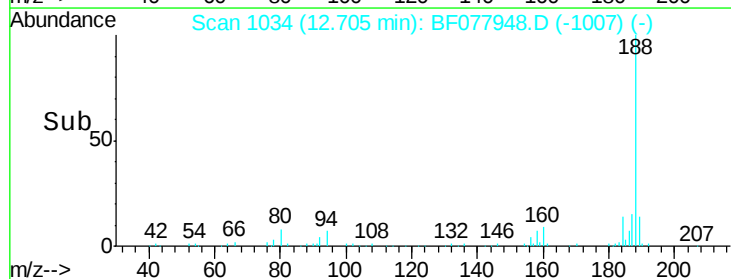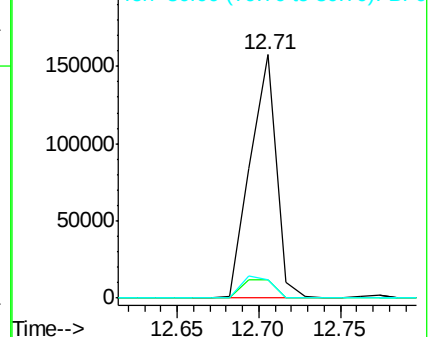

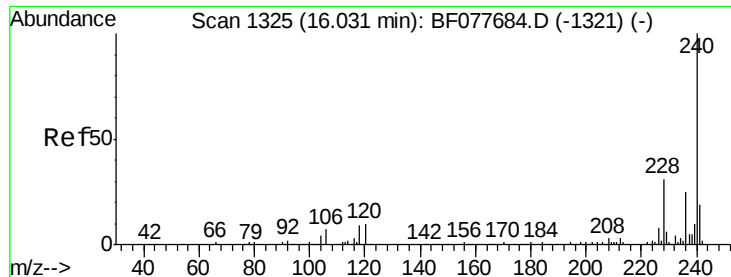

#75

Chrysene-d12

Concen: 20.00 ng

RT: 15.97 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BF077948.D

Acq: 25 Mar 2015 10:45

Instrument :

BNA_F

ClientSampleId :

SB-14


Tgt Ion:240 Resp: 192799

Ion Ratio Lower Upper

240 100

120 15.0 8.2 12.2#




236 24.4 20.0 30.0

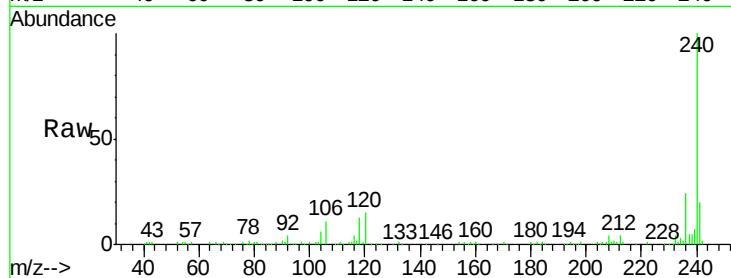

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

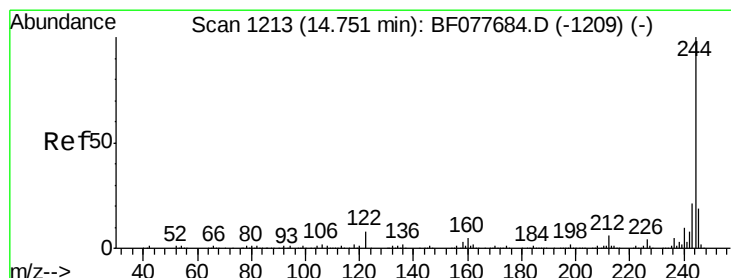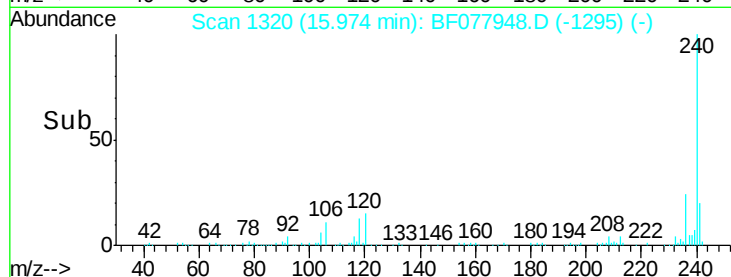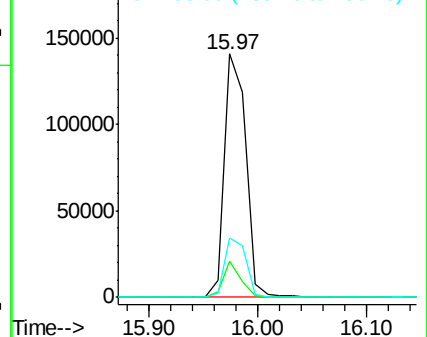

#78

Terphenyl-d14

Concen: 54.31 ng

RT: 14.69 min Scan# 1208

Delta R.T. 0.00 min

Lab File: BF077948.D

Acq: 25 Mar 2015 10:45


Tgt Ion:244 Resp: 428696

Ion Ratio Lower Upper

244 100

212 7.0 4.9 7.3



122 13.4 6.2 9.4#

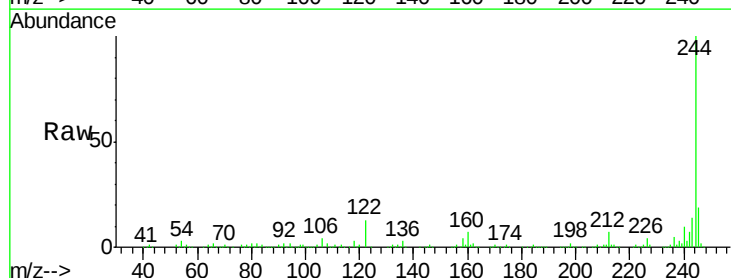


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



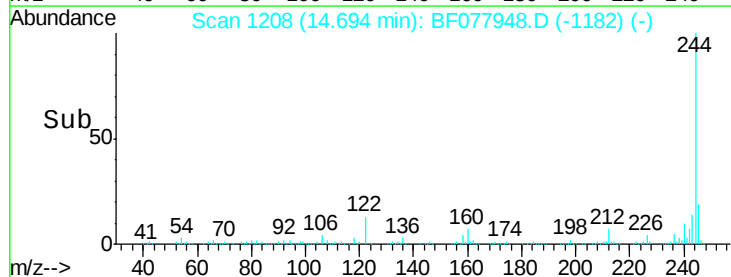
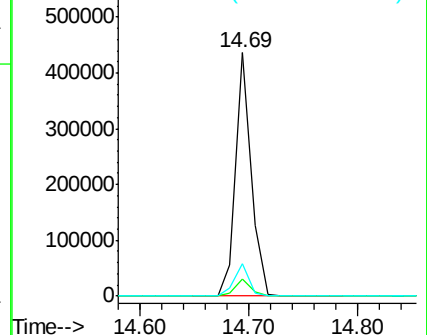


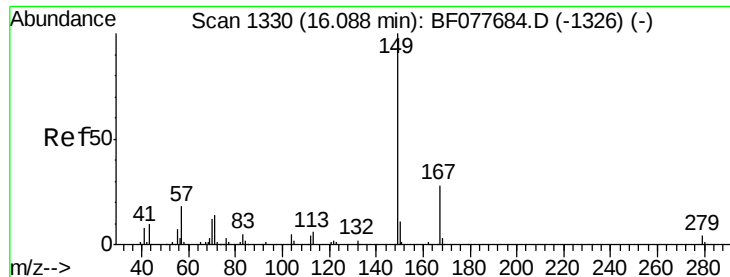

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 2.26 ng
 RT: 16.03 min Scan# 1325
 Delta R.T. -0.01 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45

Instrument :
 BNA_F
 ClientSampleId :
 SB-14

Tgt Ion:149 Resp: 16346
 Ion Ratio Lower Upper
 149 100
 167 26.6 22.4 33.6
 279 2.9 3.4 5.0#

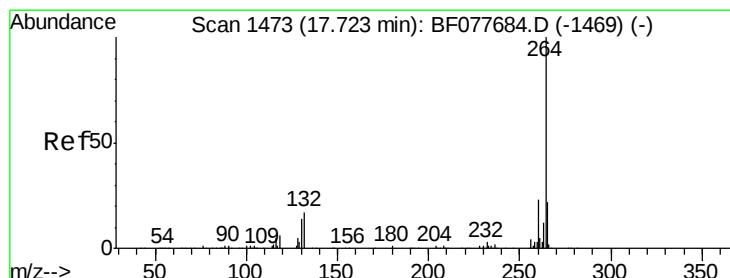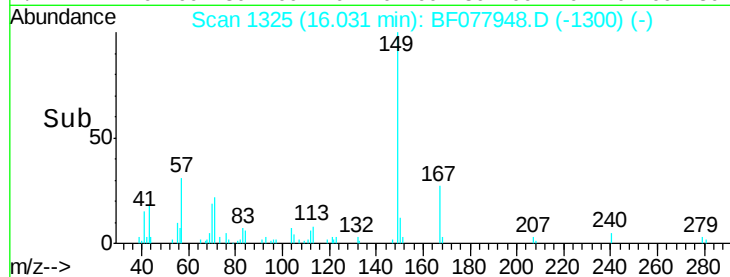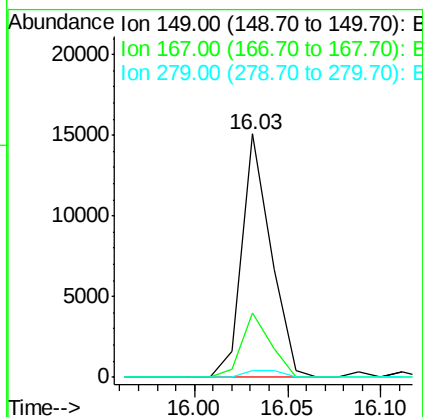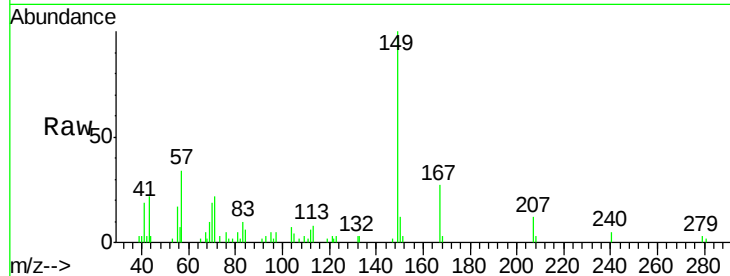

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.70 min Scan# 1471
 Delta R.T. -0.05 min
 Lab File: BF077948.D
 Acq: 25 Mar 2015 10:45

Tgt Ion:264 Resp: 191694
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.6 27.8
 265 21.2 17.3 25.9

