

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF032415\  
Data File : BF077918.D  
Acq On : 24 Mar 2015 18:24  
Operator : TP/IZ  
Sample : G1616-05  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031115.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.390       | 42            | 44          | 49           | rVB      | 48175          | 67013         | 7.27%           | 2.201%        |
| 2         | 1.767       | 75            | 77          | 96           | rVB      | 535948         | 921194        | 100.00%         | 30.258%       |
| 3         | 7.116       | 543           | 545         | 547          | rBV      | 224813         | 213214        | 23.15%          | 7.003%        |
| 4         | 8.693       | 680           | 683         | 685          | rBV      | 320072         | 299470        | 32.51%          | 9.837%        |
| 5         | 10.865      | 870           | 873         | 875          | rBV      | 260400         | 334615        | 36.32%          | 10.991%       |
| 6         | 12.694      | 1031          | 1033        | 1036         | rBV      | 355666         | 360826        | 39.17%          | 11.852%       |
| 7         | 15.997      | 1319          | 1322        | 1325         | rBV      | 380442         | 428640        | 46.53%          | 14.079%       |
| 8         | 17.826      | 1479          | 1482        | 1492         | rBV      | 328522         | 419457        | 45.53%          | 13.778%       |


Sum of corrected areas: 3044429

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF032415\  
Data File : BF077918.D  
Acq On : 24 Mar 2015 18:24  
Operator : TP/IZ  
Sample : G1616-05  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

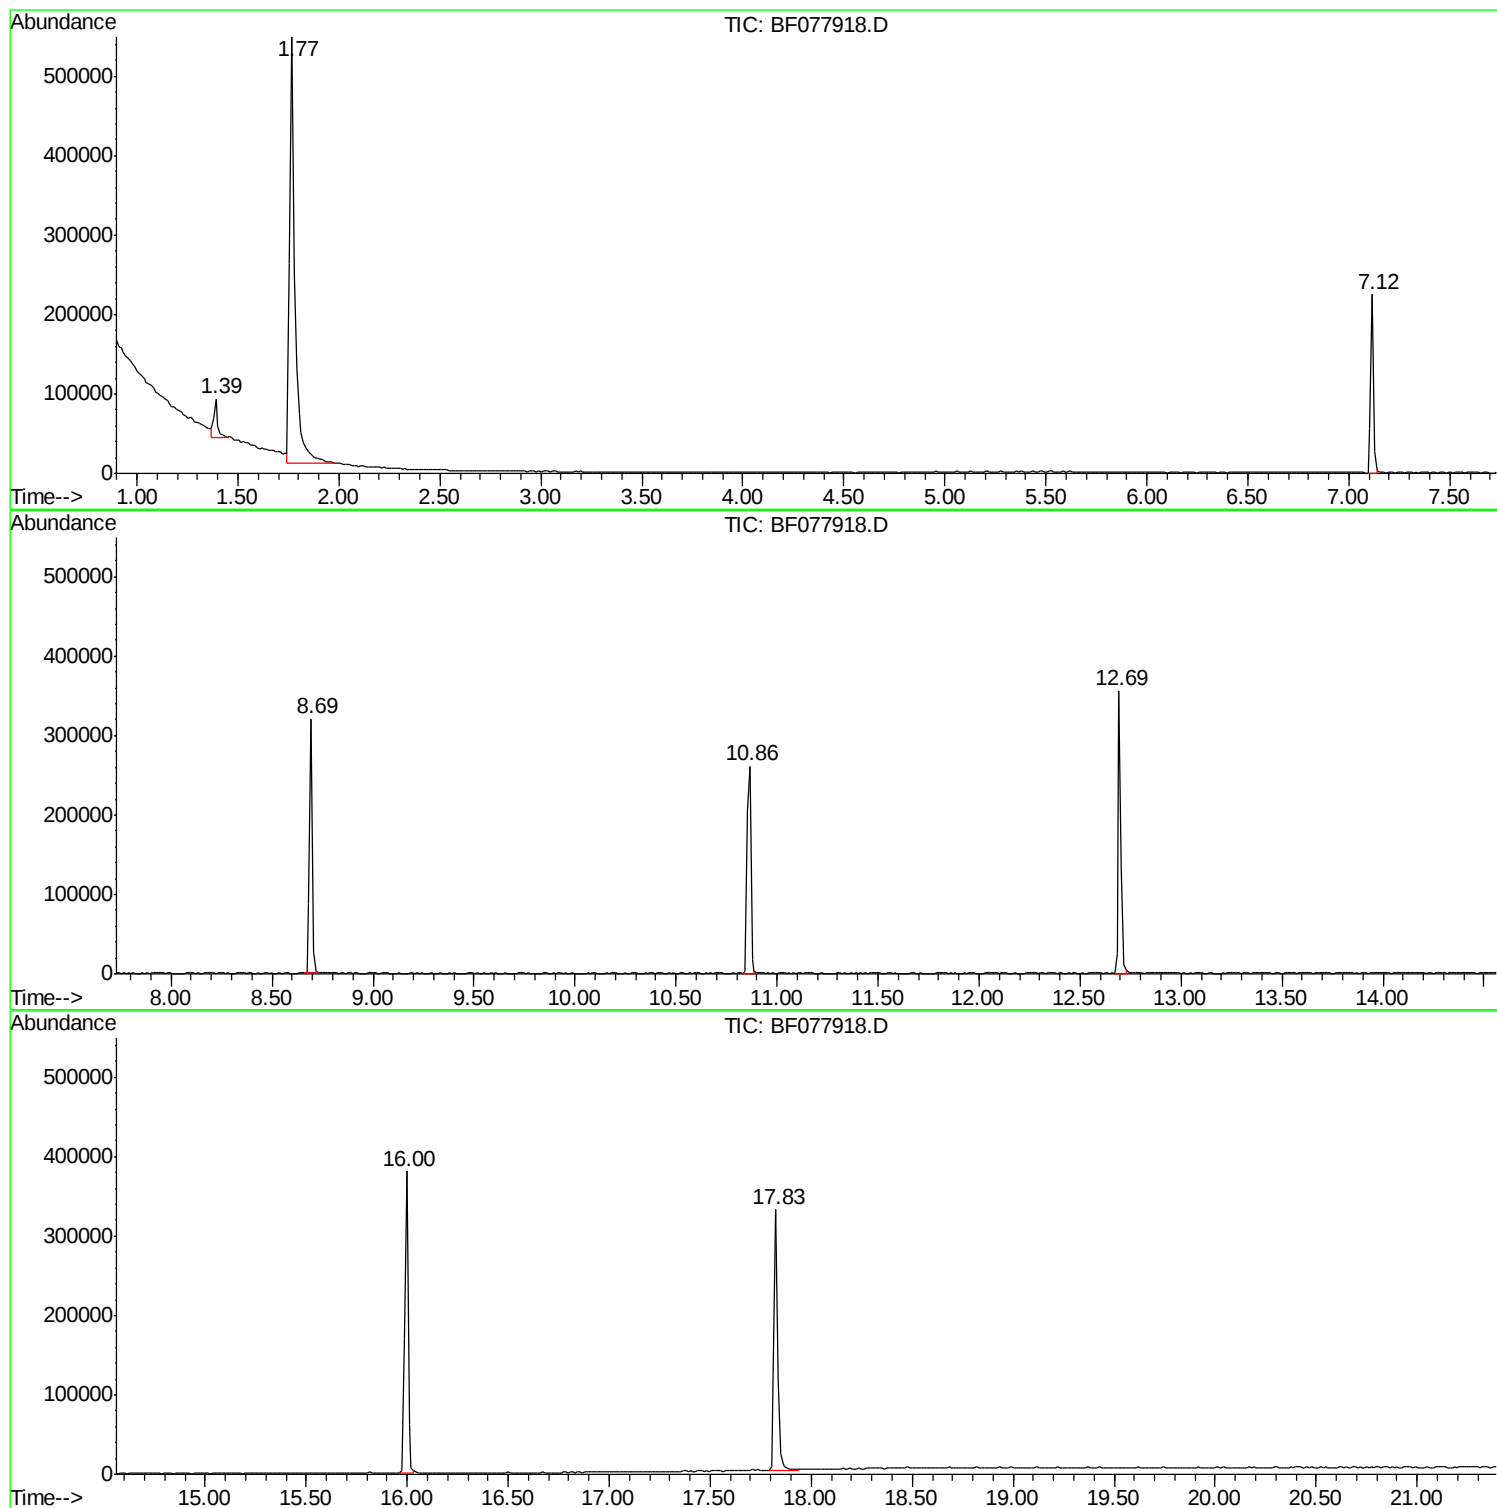

DbaaaPathh::ZZ\NRPBHHM1BBAFNDAAABBB022155\  
 DbaaaFile::BB079988DD  
 Aeqq00n ::24Mar2005 18224  
 Oppaaaor ::TPPIZ  
 Sample ::G66666005  
 Misc ::  
 AASSVal ::122 SampleMultiplier:11

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SVOC-GPC-BLANK

QqaabMebbdd::ZZ\NRPBHHM1BBAFMEH00S8270BB03115MM  
 QqaabTfile ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DAABASSEN0\$5002LL  
 TICInteggaionPaaameess:LS6CNTTP

| TIC Top Hit name | RT | EstConc | Units | Response | -Internal Standard- | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---------------------|---|----|------|------|
|------------------|----|---------|-------|----------|---------------------|---|----|------|------|

No Library Search Compounds Detected

\*\*\*\*\*