


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032415\
 Data File : BF077907.D
 Acq On : 24 Mar 2015 11:07
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 25 12:24:30 2015

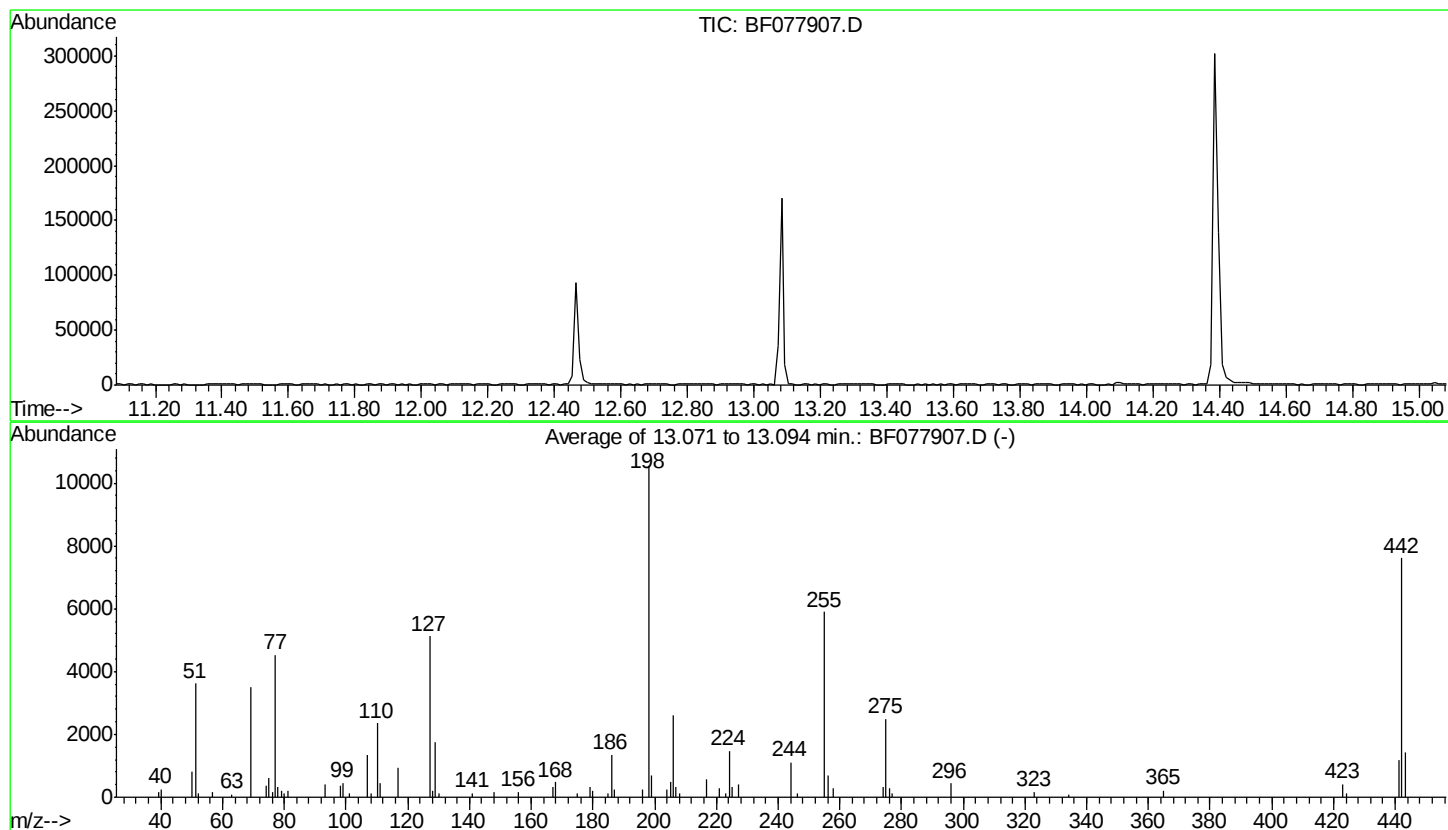

AutoFind: Scans 1066, 1067, 1068; Background Corrected with Scan 1063

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	3607	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.4	3520	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	5118	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10551	PASS
199	198	5	9	6.5	686	PASS
275	198	10	60	23.7	2497	PASS
365	198	1	100	1.9	205	PASS
441	442	0.01	24	15.4	1170	PASS
442	198	50	100	72.1	7606	PASS
443	442	15	24	19.0	1444	PASS